


Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP020320\
 Data File : BP001713.D
 Acq On : 03 Feb 2020 10:23
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 03 18:08:31 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP020320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 03 15:16:18 2020
 Response via : Initial Calibration

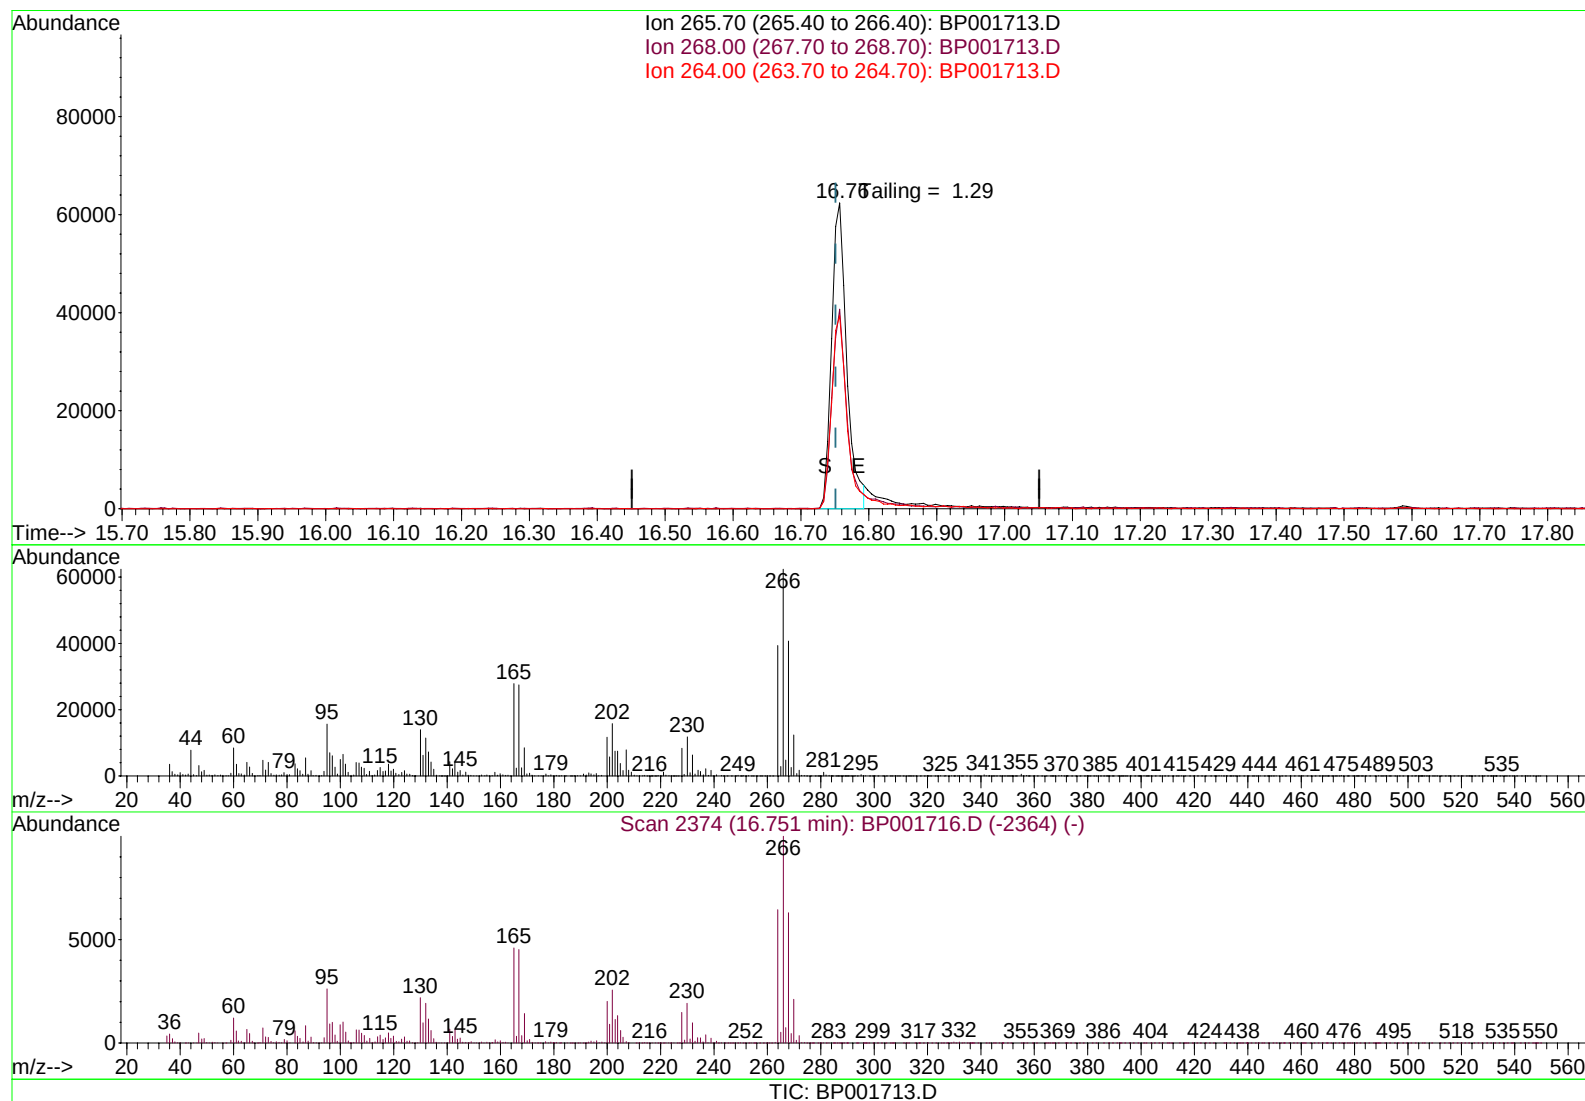

(70) Pentachlorophenol (C)




16.757min (+0.006) 1885445.93ng

response 103681

Ion	Exp%	Act%
265.70	100	100
268.00	63.00	65.24
264.00	64.50	63.10
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP020320\
 Data File : BP001713.D
 Acq On : 03 Feb 2020 10:23
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 03 18:08:31 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP020320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 03 15:16:18 2020
 Response via : Initial Calibration

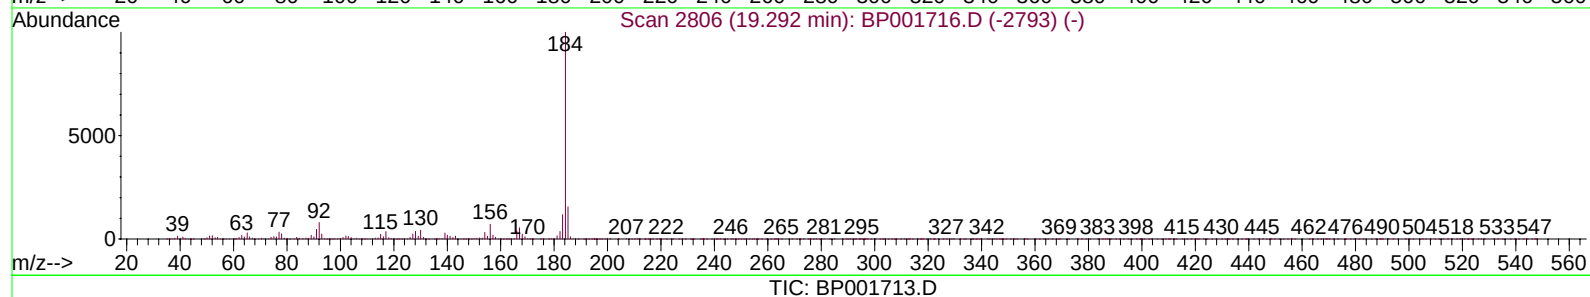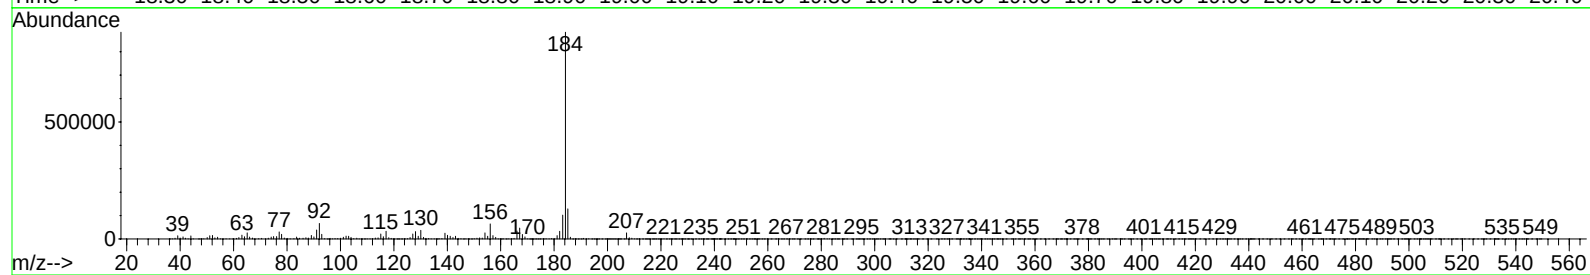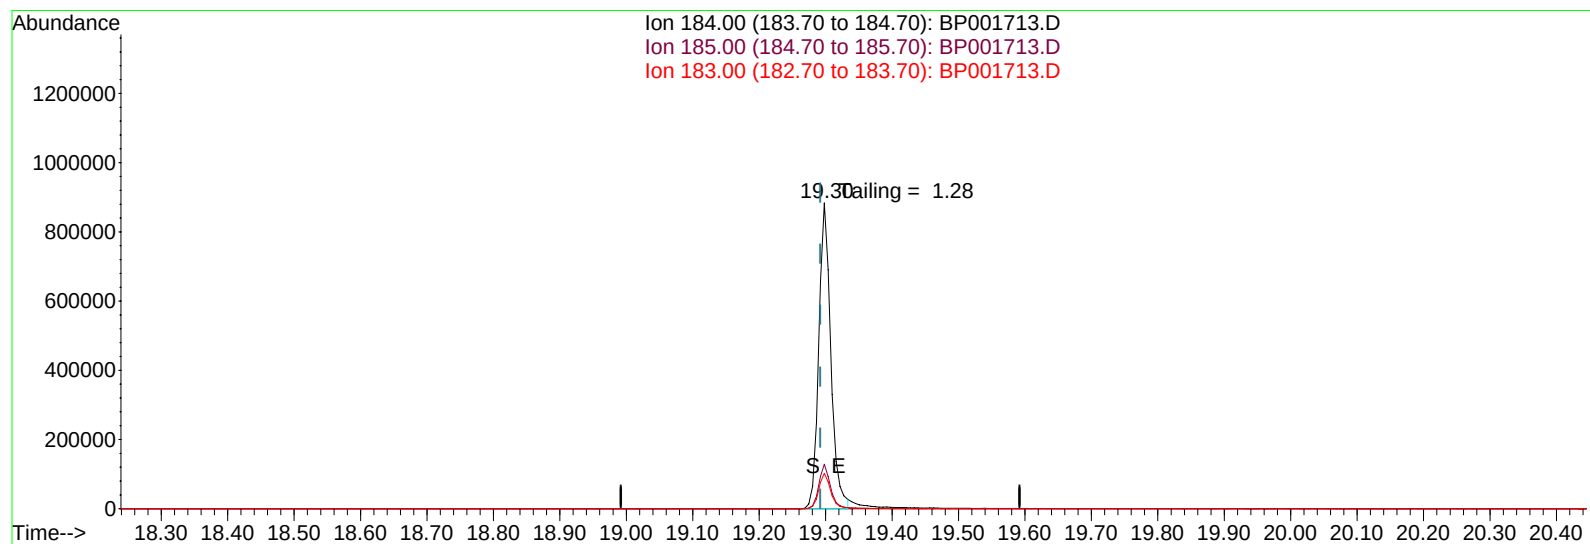

(77) Benzidine

19.298min (+0.006) 2734511.94ng

response 1156257

Ion	Exp%	Act%
184.00	100	100
185.00	15.60	14.57
183.00	11.80	11.55
0.00	0.00	0.00