


Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP020320\
 Data File : BP001713.D
 Acq On : 03 Feb 2020 10:23
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP020320.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Feb 03 15:16:18 2020

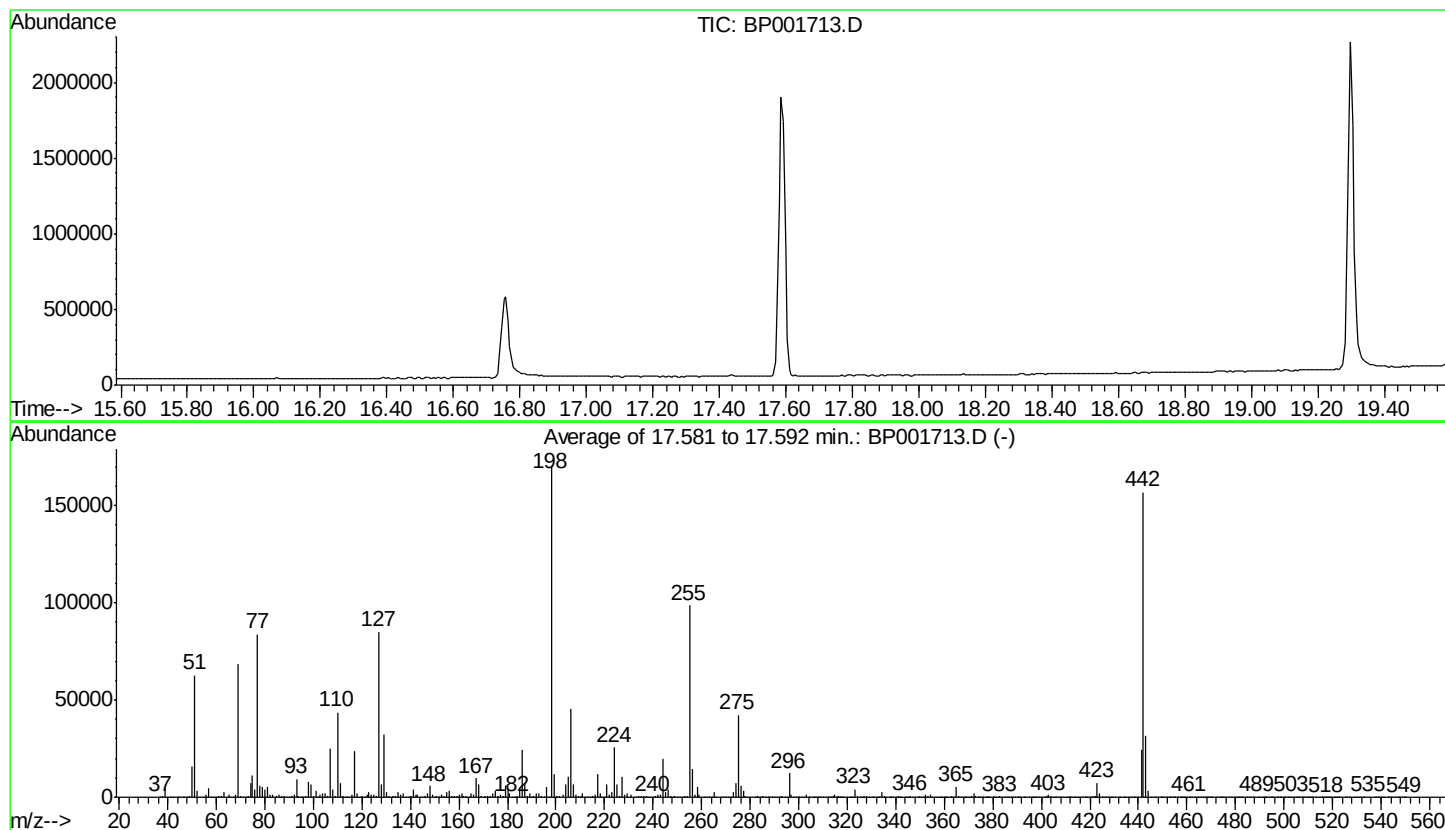

AutoFind: Scans 2515, 2516, 2517; Background Corrected with Scan 2507

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.8	62803	PASS
68	69	0.00	2	1.6	1108	PASS
69	198	0.00	100	40.3	68662	PASS
70	69	0.00	2	0.7	447	PASS
127	198	10	80	50.0	85272	PASS
197	198	0.00	2	0.2	323	PASS
198	198	100	100	100.0	170551	PASS
199	198	5	9	6.8	11617	PASS
275	198	10	60	24.8	42250	PASS
365	198	1	100	3.1	5317	PASS
441	198	0.01	100	14.3	24471	PASS
442	198	50	100	92.0	156957	PASS
443	442	15	24	20.2	31744	PASS