

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020322\
 Data File : BP009027.D
 Acq On : 03 Feb 2022 14:04
 Operator : CG/JU
 Sample : N1359-08
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 FB020122

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP009027.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.034	3	8	22	rVB	782771	1062154	8.62%	2.049%
2	5.411	406	412	432	rBV	1394801	2320442	18.84%	4.476%
3	7.005	671	683	701	rBV	657356	1315459	10.68%	2.537%
4	7.822	813	822	830	rBV	742908	1277932	10.38%	2.465%
5	8.981	1011	1019	1042	rBV	2233780	4132528	33.55%	7.971%
6	10.616	1290	1297	1314	rBV	873005	1665148	13.52%	3.212%
7	13.087	1709	1717	1743	rBV	6339762	10467023	84.98%	20.190%
8	14.463	1944	1951	1974	rBV	1356007	2280344	18.51%	4.399%
9	15.957	2198	2205	2227	rBV	4300026	7679477	62.35%	14.813%
10	17.222	2413	2420	2434	rBV	1560750	2633553	21.38%	5.080%
11	18.116	2567	2572	2582	rBV2	112546	243013	1.97%	0.469%
12	19.351	2778	2782	2795	rBV3	69418	182433	1.48%	0.352%
13	19.780	2849	2855	2872	rBV	9900708	12317376	100.00%	23.759%
14	21.316	3111	3116	3126	rBV	1499798	2217830	18.01%	4.278%
15	23.721	3519	3525	3539	rVB2	867257	2048388	16.63%	3.951%




Sum of corrected areas: 51843100

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020322\
Data File : BP009027.D
Acq On : 03 Feb 2022 14:04
Operator : CG/JU
Sample : N1359-08
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
FB020122

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

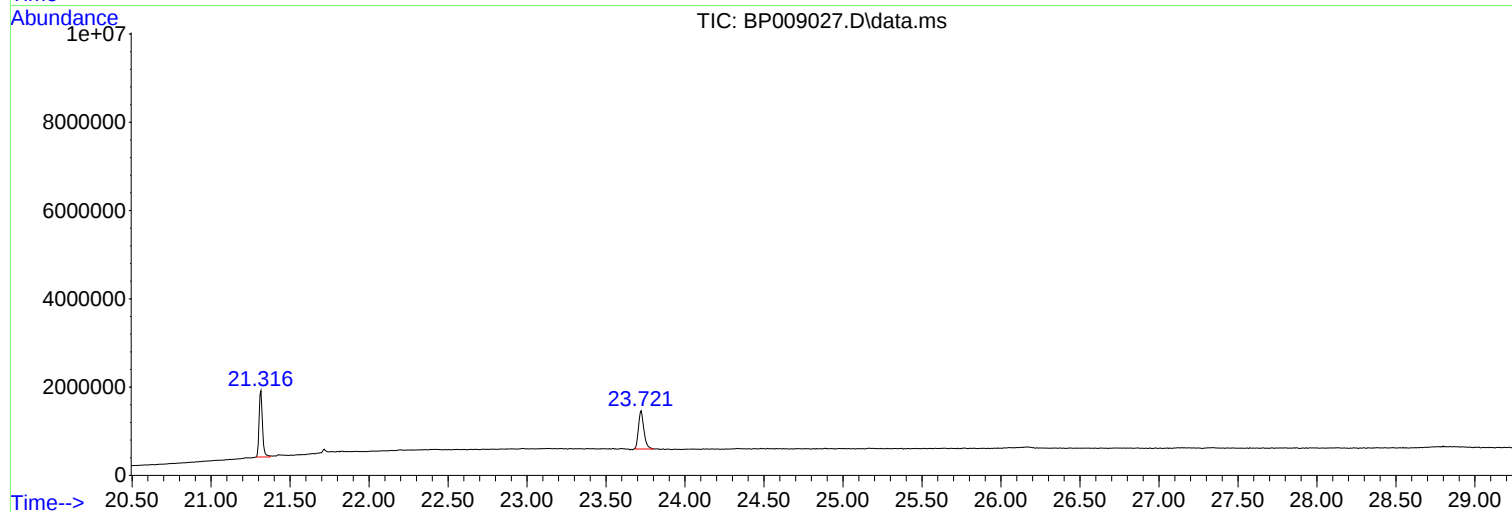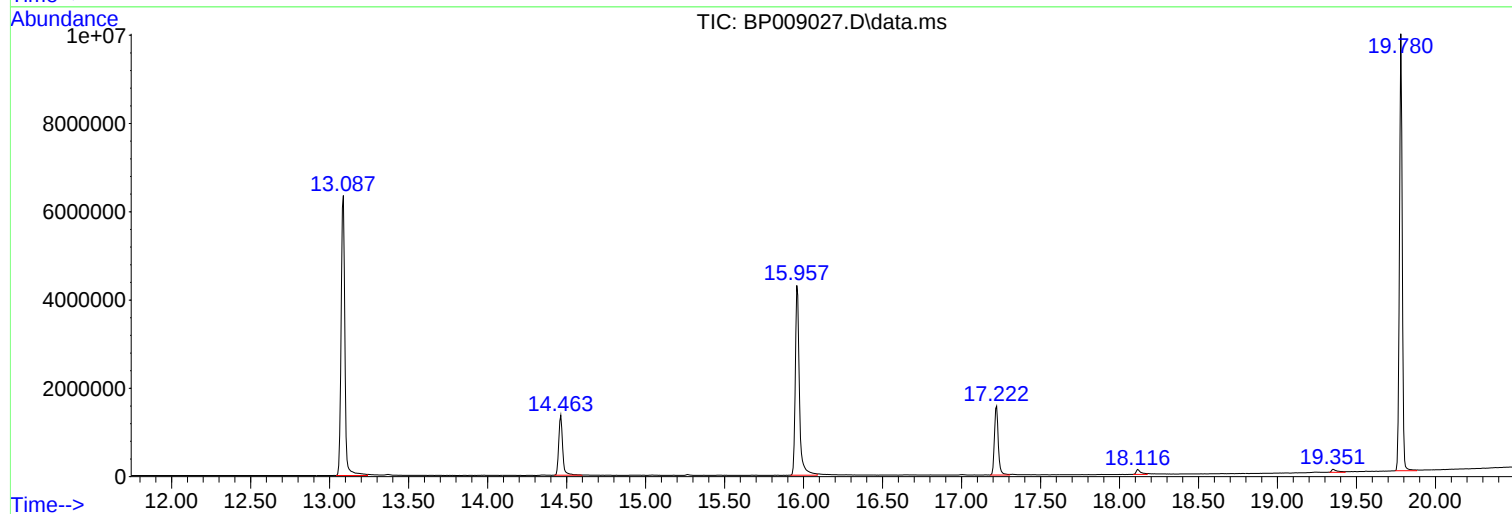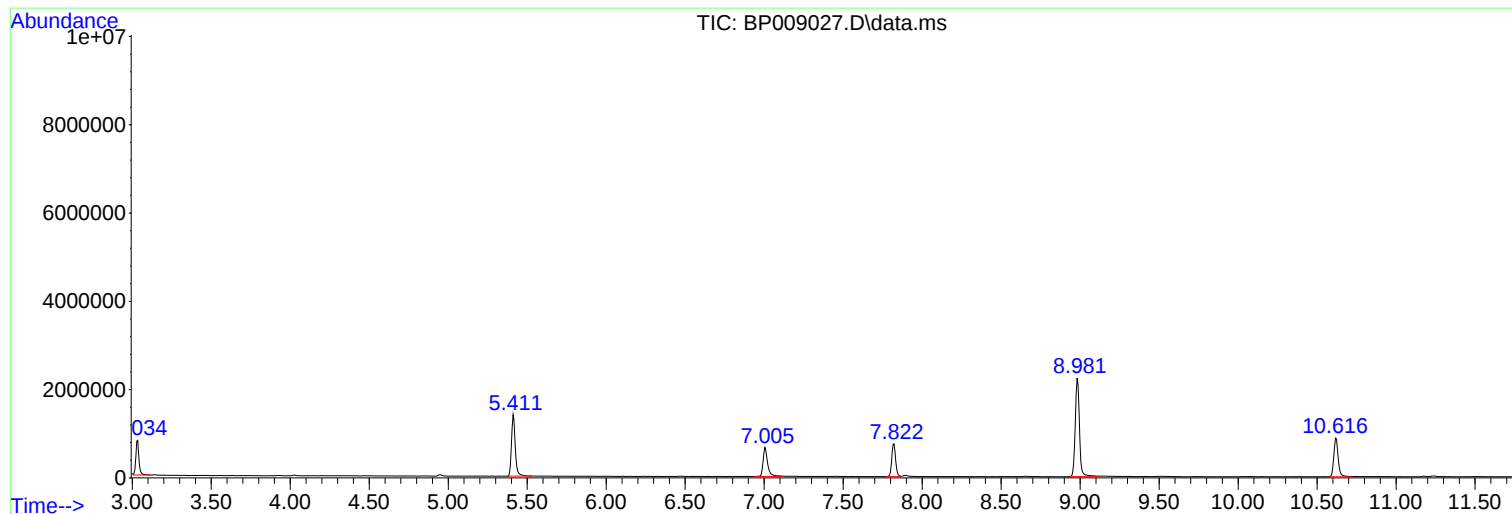

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020322\
Data File : BP009027.D
Acq On : 03 Feb 2022 14:04
Operator : CG/JU
Sample : N1359-08
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
FB020122










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.034	16.62 ng	1062150	1,4-Dichlorobenzene-d4	7.822

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	78
2			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	39
3			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	23
4			Acetamide, N-ethyl-	87	C4H9NO	000625-50-3	9
5			Silane, tetramethyl-	88	C4H12Si	000075-76-3	9

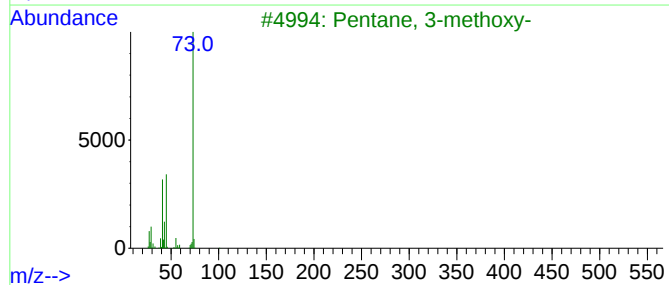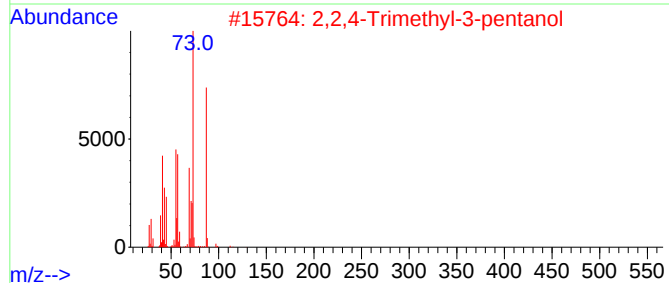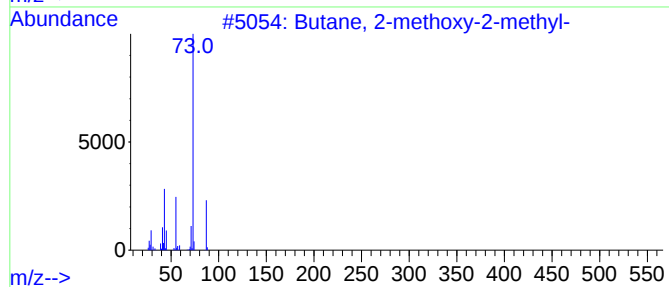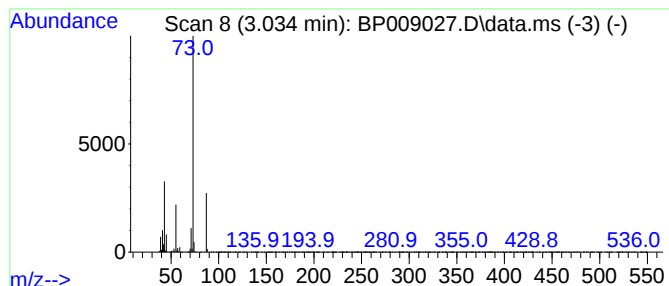

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020322\
Data File : BP009027.D
Acq On : 03 Feb 2022 14:04
Operator : CG/JU
Sample : N1359-08
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
FB020122

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	3.034	16.6	ng	1062150	1	7.822	1277930	20.0