


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020322\
 Data File : BP009020.D
 Acq On : 03 Feb 2022 09:56
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Feb 03 06:20:22 2022

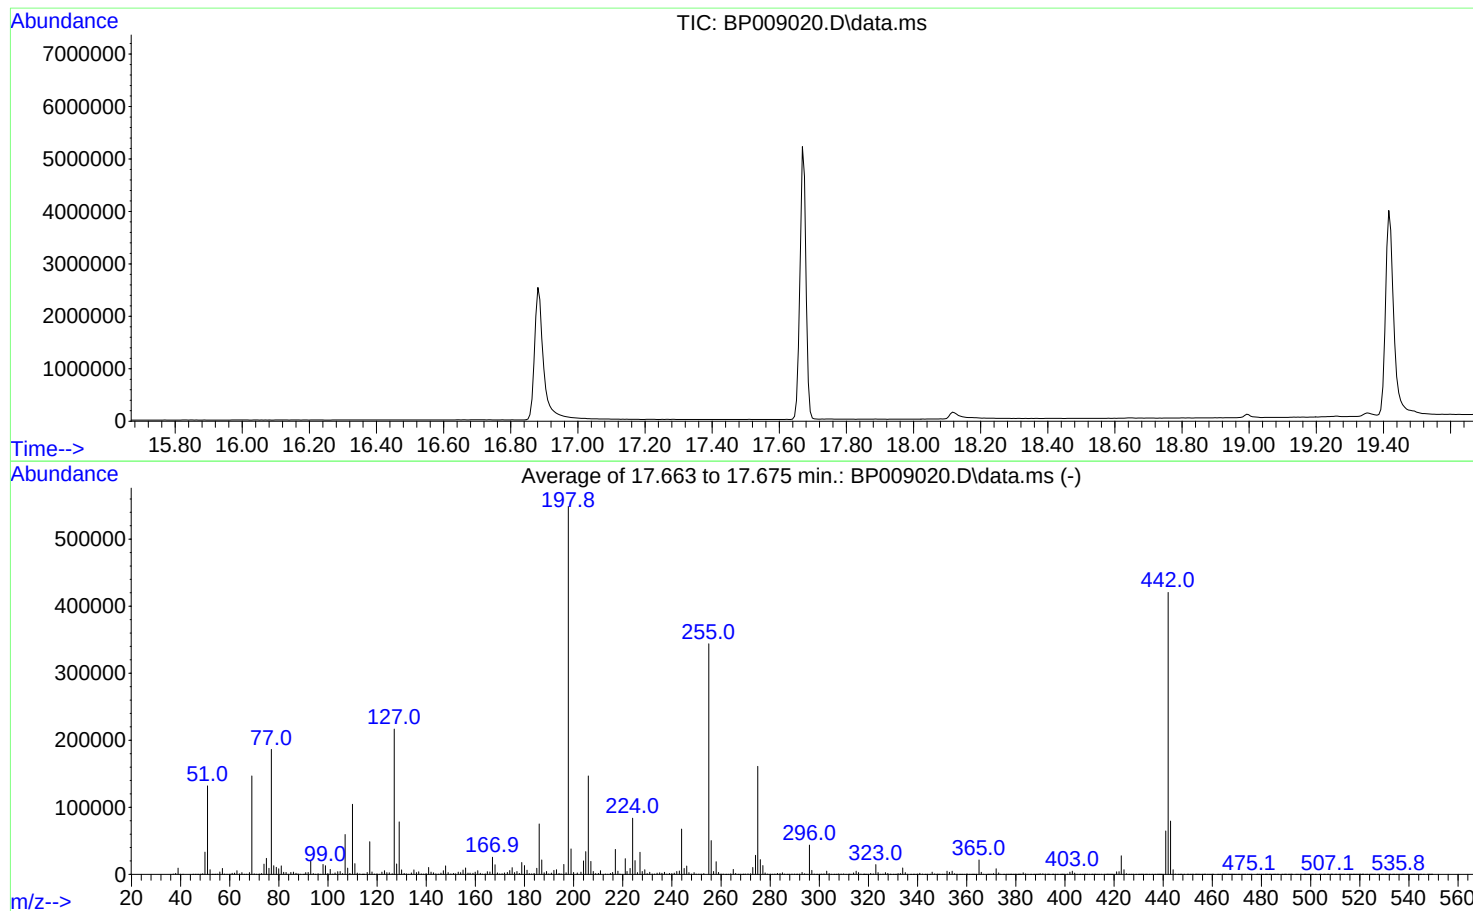


AutoFind: Scans 2495, 2496, 2497; Background Corrected with Scan 2487

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.1	131973	PASS
68	69	0.00	2	1.8	2585	PASS
69	198	0.00	100	26.8	146854	PASS
70	69	0.00	2	0.5	764	PASS
127	198	10	80	39.5	216663	PASS
197	198	0.00	2	0.4	2363	PASS
198	198	100	100	100.0	548703	PASS
199	198	5	9	6.9	37973	PASS
275	198	10	60	29.4	161241	PASS
365	198	1	100	3.9	21581	PASS
441	198	0.01	100	11.8	64747	PASS
442	442	100	100	100.0	420608	PASS
443	442	15	24	18.9	79453	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020322\
 Data File : BP009020.D
 Acq On : 03 Feb 2022 09:56
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Feb 03 13:27:29 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 03 06:20:22 2022
 Response via : Initial Calibration

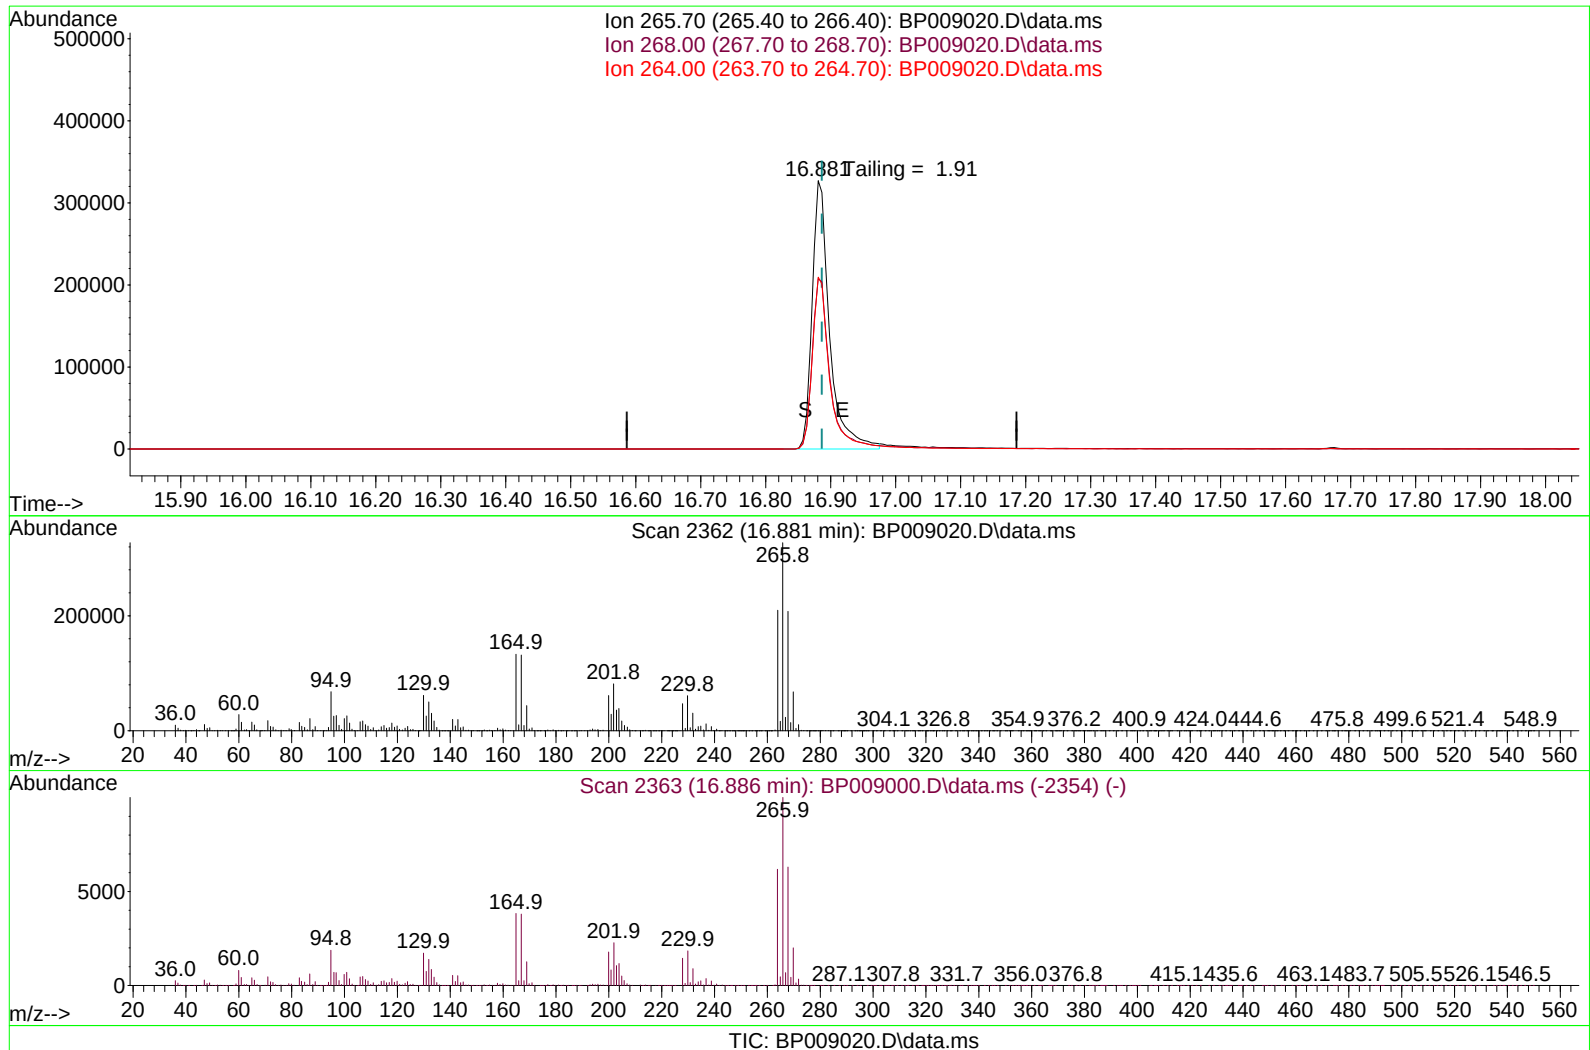

TIC: BP009020.D\data.ms

(70) Pentachlorophenol (C)

16.881min (-0.006) 2170969.71 ng




response 628780

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	63.48
264.00	62.90	64.05
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020322\
 Data File : BP009020.D
 Acq On : 03 Feb 2022 09:56
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Feb 03 13:27:29 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 03 06:20:22 2022
 Response via : Initial Calibration

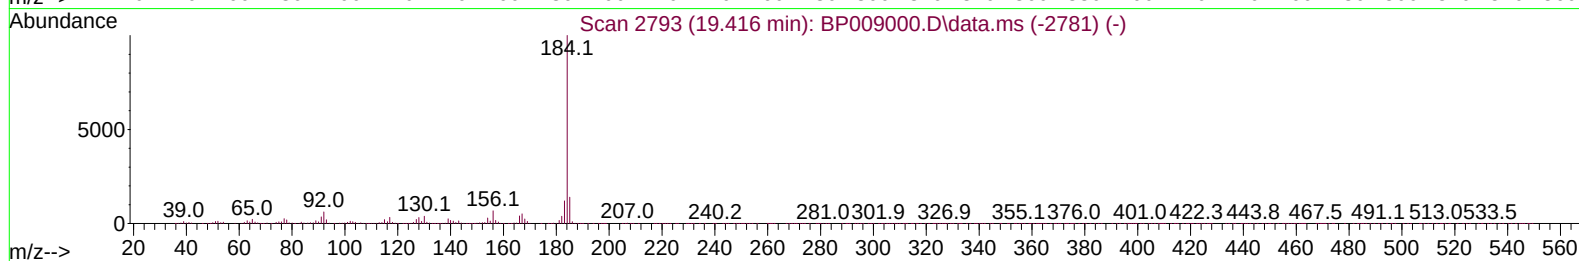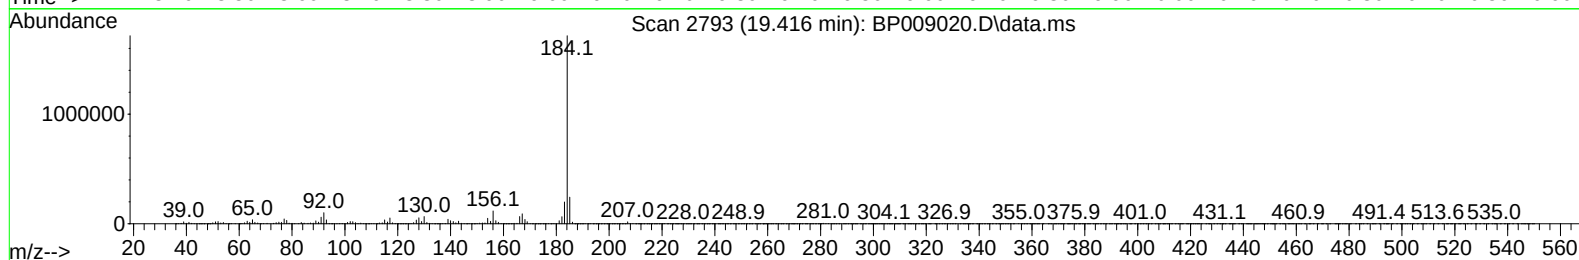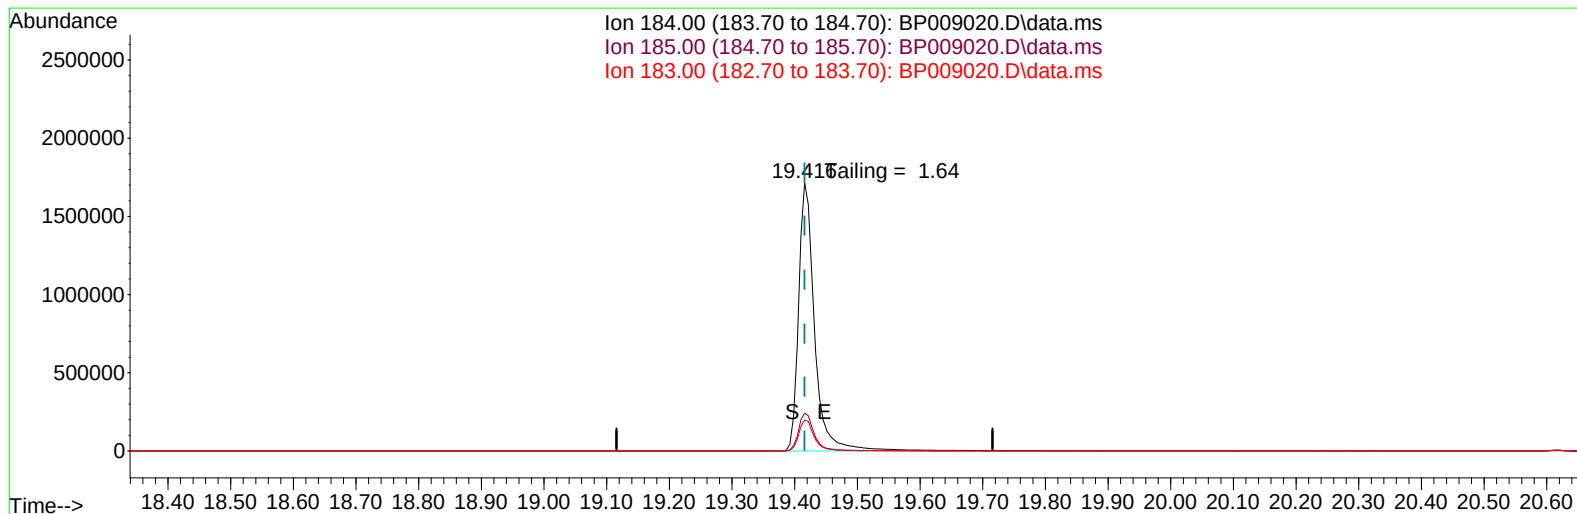

TIC: BP009020.D\data.ms

(77) Benzidine

19.416min (+ 0.000) 550520.77 ng

response 3053443

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.10
183.00	11.90	11.56
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/3/2022	BNA_P	<u>BP009020.D</u>
Compound Name	Response	Retention Time
DDT	1772942	20.61
DDD	80746	20.18
DDE	5439	19.69
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
86185	1859127	4.64

Instrument :
BNA_P
ClientSampleId :
DFTPP