

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020325\
 Data File : BP023887.D
 Acq On : 03 Feb 2025 19:56
 Operator : RC/JU
 Sample : Q1190-14
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A44T3

Quant Time: Feb 04 07:34:29 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Feb 03 11:19:36 2025
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.775	152	445555	20.000	ng/ul	0.00
20) Naphthalene-d8	10.545	136	1934755	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.392	164	1209566	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.204	188	2342684	20.000	ng/ul	0.02
79) Chrysene-d12	21.645	240	2295314	20.000	ng/ul	0.00
88) Perylene-d12	25.021	264	2502340	20.000	ng/ul	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.293	96	46136	4.302	ng/uL	0.00
4) Pyridine-d5	3.705	84	616236	19.915	ng/ul	0.00
7) Phenol-d5	6.957	99	841072	21.331	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.110	67	490877	23.520	ng/ul	0.00
11) 2-Chlorophenol-d4	7.316	132	692918	22.378	ng/ul	0.00
15) 4-Methylphenol-d8	8.481	113	513400	15.939	ng/ul	0.00
21) Nitrobenzene-d5	8.916	128	345996	22.352	ng/ul	0.00
24) 2-Nitrophenol-d4	9.634	143	358974	21.492	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.175	165	655104	21.380	ng/ul	0.00
31) 4-Chloroaniline-d4	10.681	131	451949	9.863	ng/ul	0.00
46) Dimethylphthalate-d6	13.798	166	1895065	21.004	ng/ul	0.00
49) Acenaphthylene-d8	14.086	160	2179915	21.423	ng/ul	0.00
54) 4-Nitrophenol-d4	14.616	143	273006	15.237	ng/ul	0.00
60) Fluorene-d10	15.398	176	1568908	20.650	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.522	200	155358	10.750	ng/ul	0.01
73) Anthracene-d10	17.298	188	2130113	18.519	ng/ul	0.01
81) Pyrene-d10	19.674	212	2325794	18.911	ng/ul	0.01
92) Benzo(a)pyrene-d12	24.768	264	1542822	11.817	ng/ul	0.00
Target Compounds						
					Qvalue	
8) Phenol	6.987	94	57278	1.415	ng/ul	93
30) Naphthalene	10.598	128	106611	1.029	ng/ul	99
36) 2-Methylnaphthalene	12.210	142	136194	1.870	ng/ul	99
72) Phenanthrene	17.245	178	335121	2.533	ng/ul	99
74) Anthracene	17.245	178	335813	2.517	ng/ul	99
80) Fluoranthene	19.327	202	475301	3.355	ng/ul	99
82) Pyrene	19.704	202	431465	2.912	ng/ul	98
85) Benzo(a)anthracene	21.621	228	177137	1.174	ng/ul#	88
87) Chrysene	21.692	228	346596	2.492	ng/ul#	93
90) Benzo(b)fluoranthene	23.933	252	336085	2.213	ng/ul#	94
93) Benzo(a)pyrene	24.839	252	189102	1.334	ng/ul#	89
96) Benzo(g,h,i)perylene	30.027	276	147319	1.046	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020325\
Data File : BP023887.D
Acq On : 03 Feb 2025 19:56
Operator : RC/JU
Sample : Q1190-14
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A44T3

Quant Time: Feb 04 07:34:29 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Feb 03 11:19:36 2025
Response via : Initial Calibration




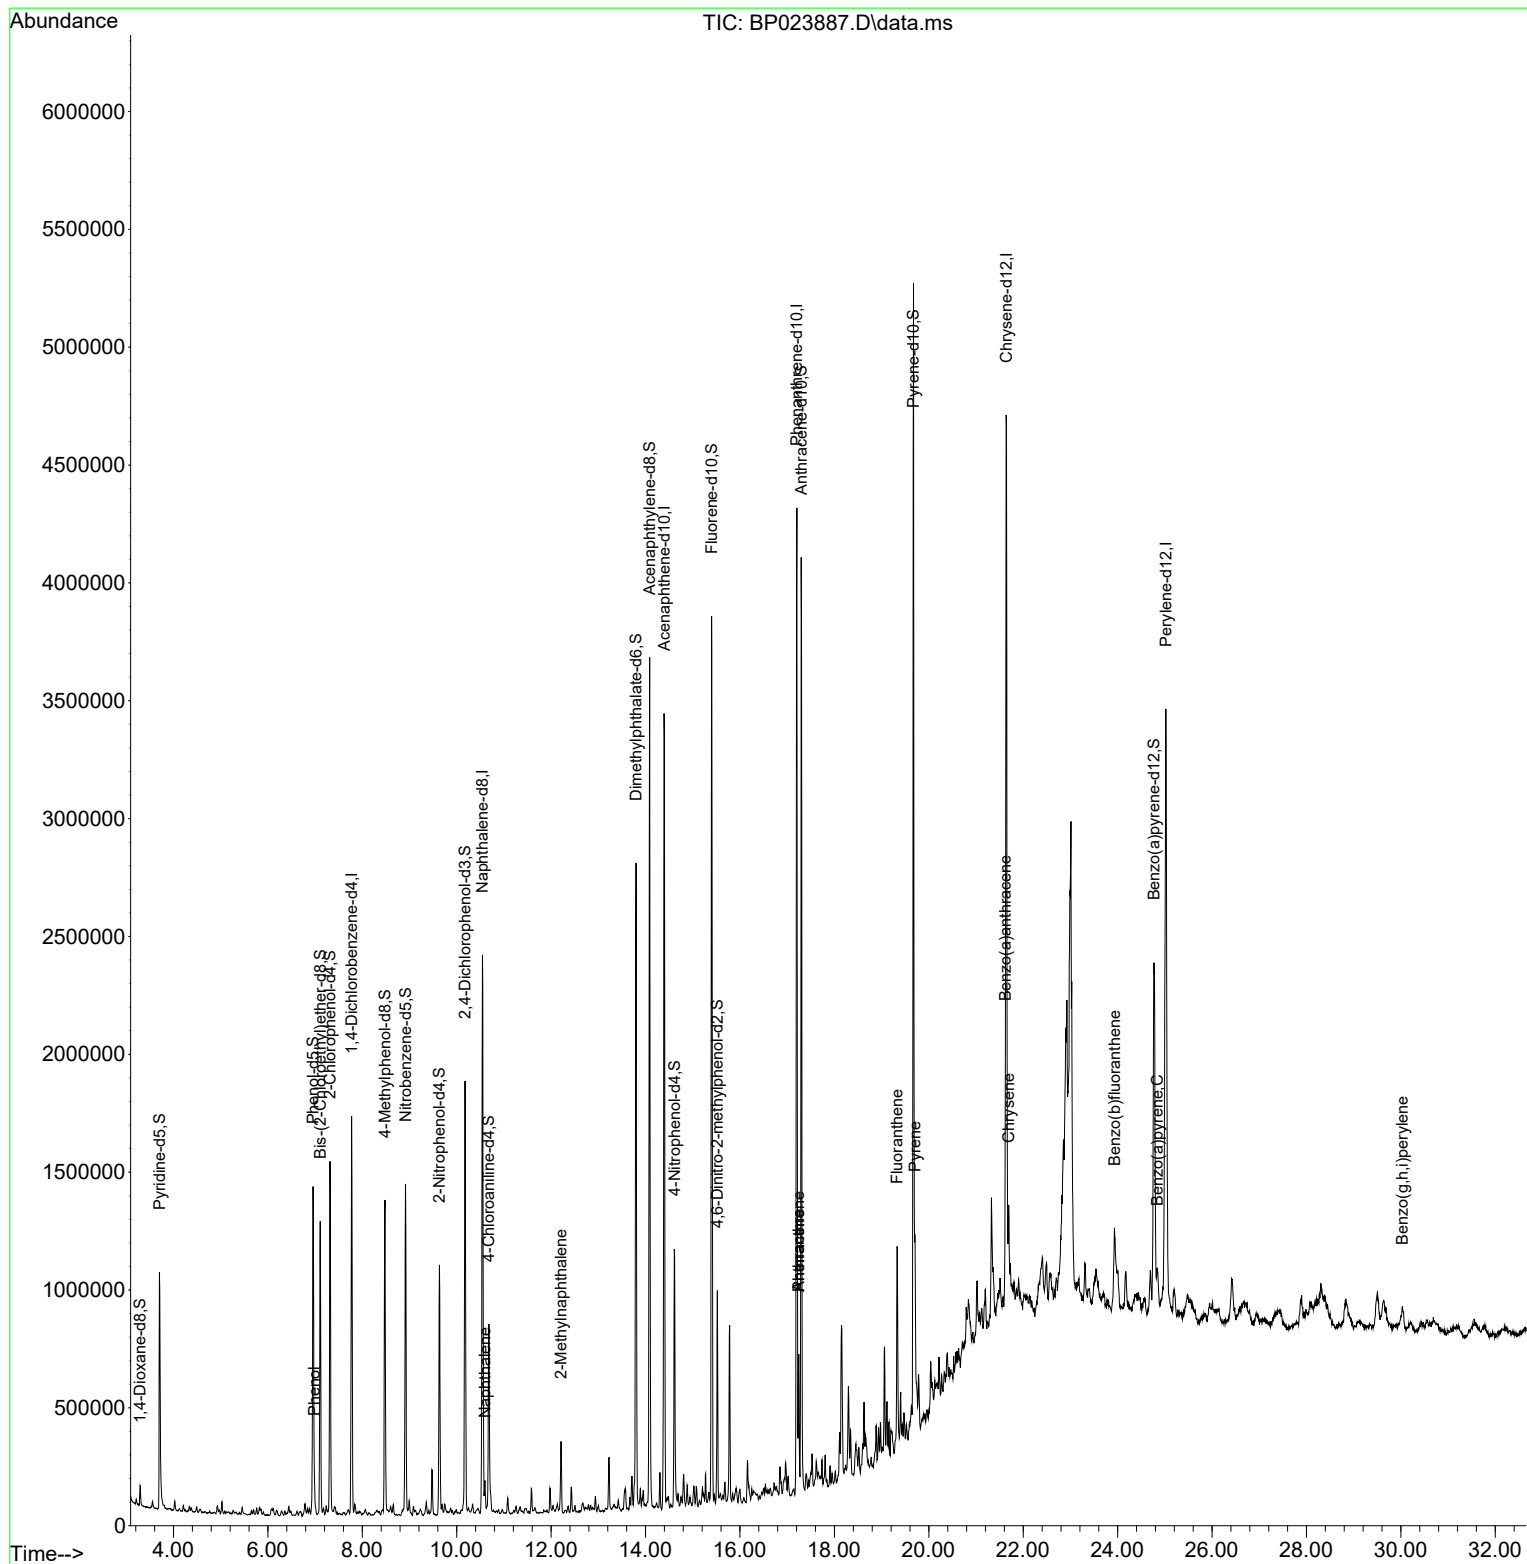




#8
Phenol
Concen: 1.415 ng/ul
RT: 6.987 min Scan# 60
Delta R.T. 0.006 min
Lab File: BP023887.D
Acq: 03 Feb 2025 19:56




Instrument :
BNA_P
ClientSampleId :
A44T3


Tgt Ion: 94 Resp: 57278
Ion Ratio Lower Upper
94 100
65 27.4 20.1 30.1
66 37.5 26.0 39.0

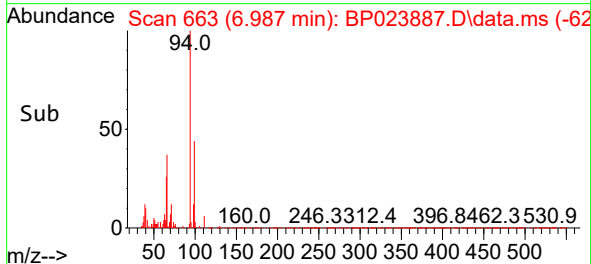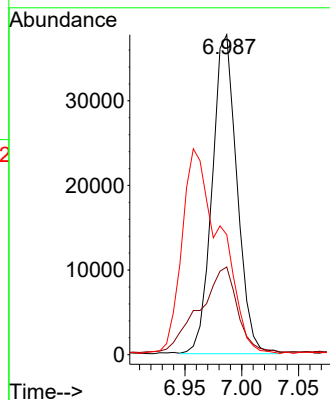

#30
Naphthalene
Concen: 1.029 ng/ul
RT: 10.598 min Scan# 1277
Delta R.T. 0.006 min
Lab File: BP023887.D
Acq: 03 Feb 2025 19:56

Tgt Ion: 128 Resp: 106611
Ion Ratio Lower Upper
128 100
129 11.4 8.7 13.1
127 13.4 10.5 15.7


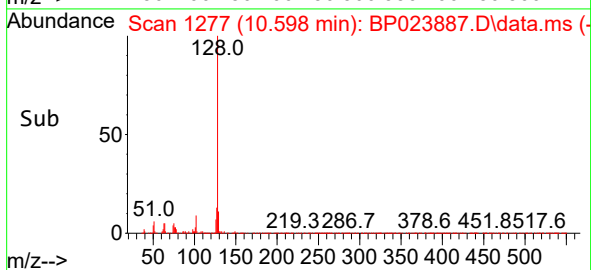
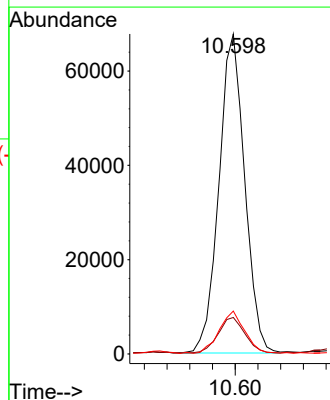
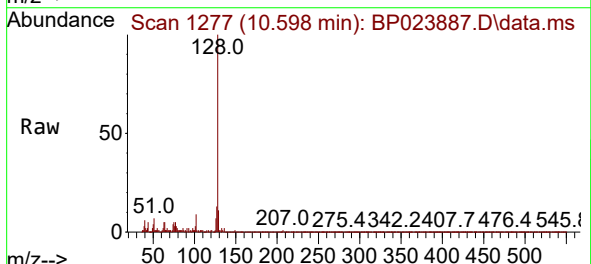




#36
2-Methylnaphthalene
Concen: 1.870 ng/ul
RT: 12.210 min Scan# 1
Delta R.T. 0.006 min
Lab File: BP023887.D
Acq: 03 Feb 2025 19:56




Instrument :
BNA_P
ClientSampleId :
A44T3


Tgt Ion:142 Resp: 136194
Ion Ratio Lower Upper
142 100
141 89.5 70.8 106.2

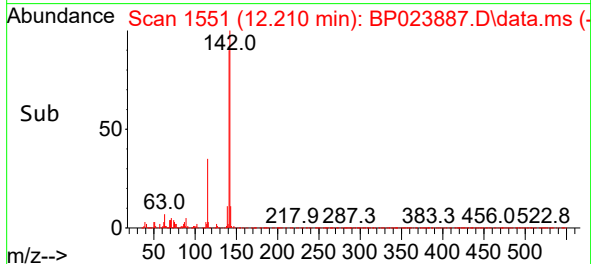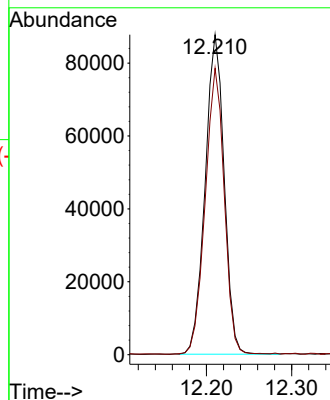

#72
Phenanthrene
Concen: 2.533 ng/ul
RT: 17.245 min Scan# 2407
Delta R.T. 0.017 min
Lab File: BP023887.D
Acq: 03 Feb 2025 19:56

Tgt Ion:178 Resp: 335121
Ion Ratio Lower Upper
178 100
179 15.8 12.2 18.4
176 19.5 15.6 23.4


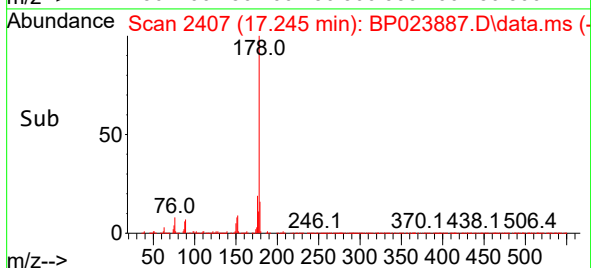
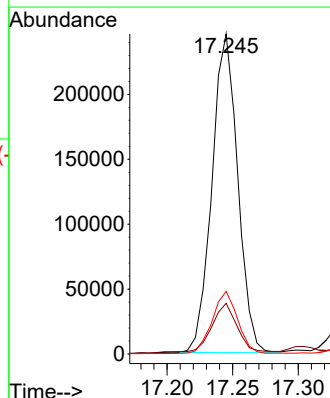
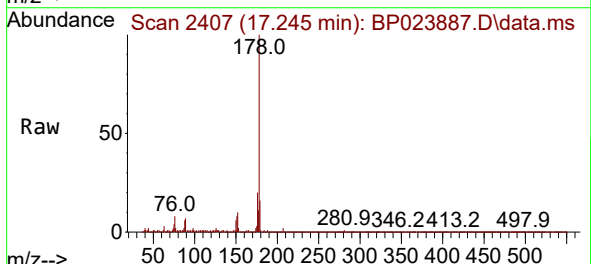




#74
 Anthracene
 Concen: 2.517 ng/ul
 RT: 17.245 min Scan# 2420
 Delta R.T. -0.077 min
 Lab File: BP023887.D
 Acq: 03 Feb 2025 19:56




Instrument :
 BNA_P
 ClientSampleId :
 A44T3


Tgt Ion:178 Resp: 335813
 Ion Ratio Lower Upper
 178 100
 179 15.8 12.4 18.6
 176 19.5 15.0 22.4

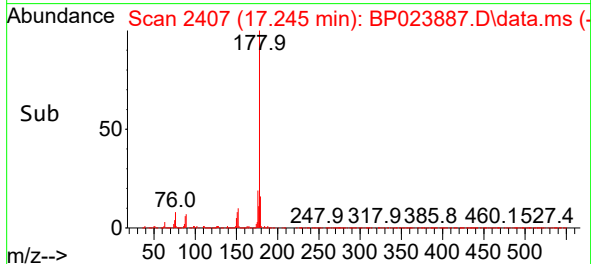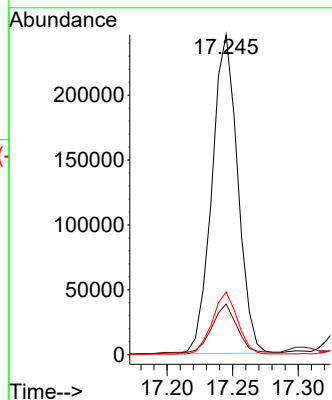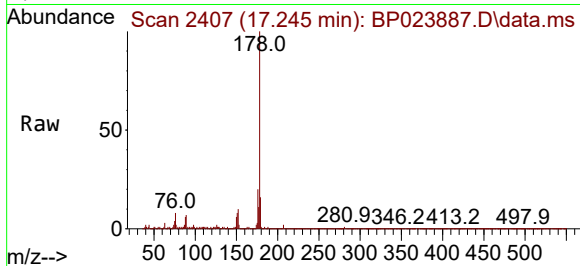

#80
 Fluoranthene
 Concen: 3.355 ng/ul
 RT: 19.327 min Scan# 2761
 Delta R.T. 0.012 min
 Lab File: BP023887.D
 Acq: 03 Feb 2025 19:56

Tgt Ion:202 Resp: 475301
 Ion Ratio Lower Upper
 202 100
 101 11.3 9.4 14.2
 100 8.7 7.0 10.6

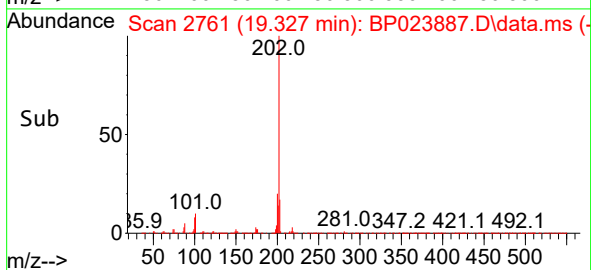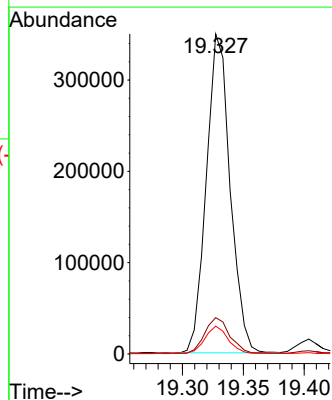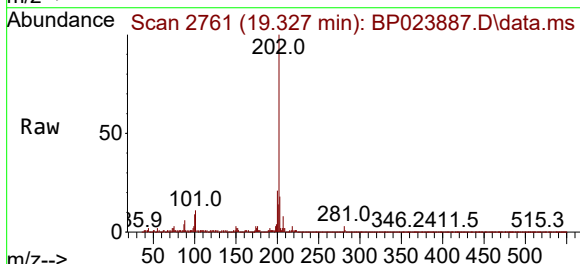

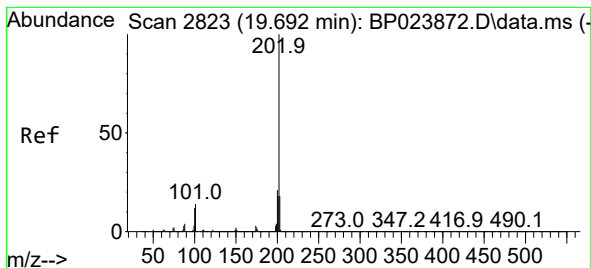

#82

Pyrene

Concen: 2.912 ng/ul

RT: 19.704 min Scan# 2825

Delta R.T. 0.011 min

Lab File: BP023887.D

Acq: 03 Feb 2025 19:56

Instrument :

BNA_P

ClientSampleId :

A44T3





Tgt Ion:202 Resp: 431465

Ion Ratio Lower Upper

202 100

101 14.3 10.4 15.6

100 11.2 8.6 12.8

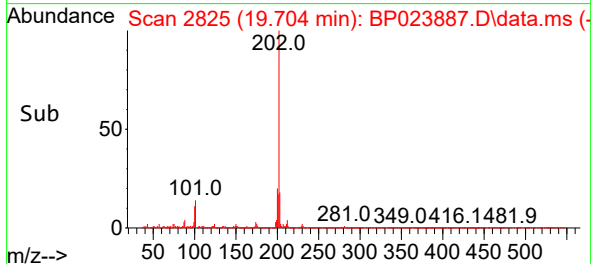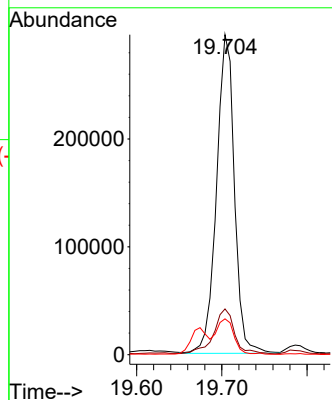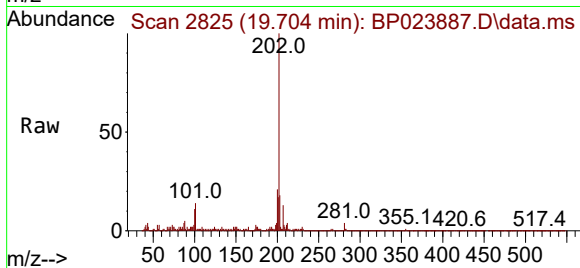

#85

Benzo(a)anthracene

Concen: 1.174 ng/ul

RT: 21.621 min Scan# 3151

Delta R.T. 0.006 min

Lab File: BP023887.D

Acq: 03 Feb 2025 19:56




Tgt Ion:228 Resp: 177137


Ion Ratio Lower Upper

228 100

229 26.1 15.9 23.9#

226 32.6 21.7 32.5#

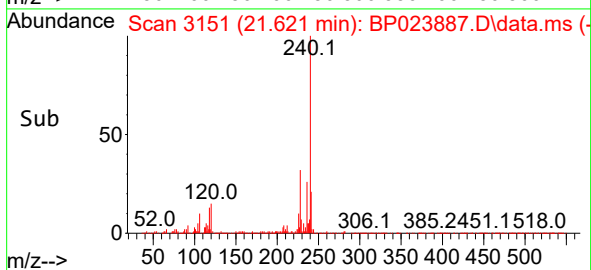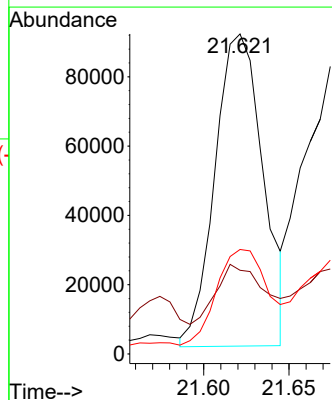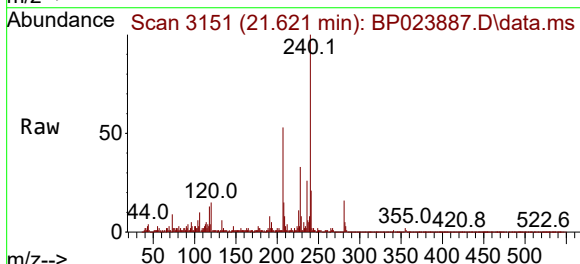



#87

Chrysene

Concen: 2.492 ng/ul

RT: 21.692 min Scan# 3163

Delta R.T. 0.006 min

Lab File: BP023887.D

Acq: 03 Feb 2025 19:56

Instrument :

BNA_P

ClientSampleId :

A44T3





Tgt Ion:228 Resp: 346596

Ion Ratio Lower Upper

228 100

226 31.3 23.8 35.6

229 25.2 15.7 23.5#

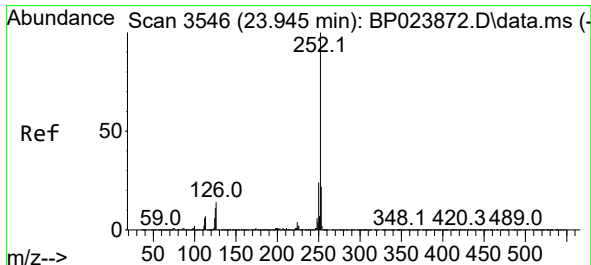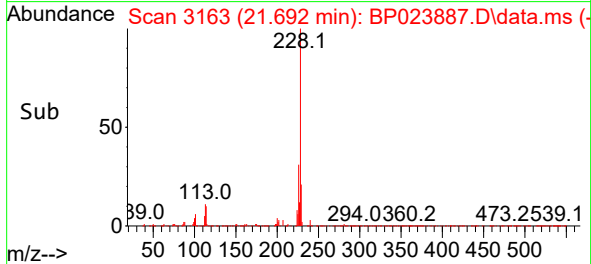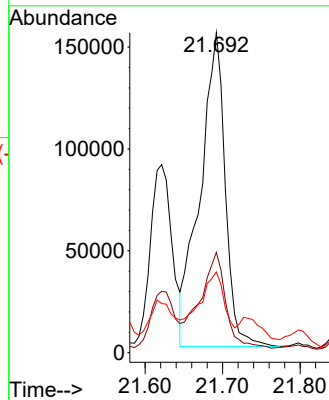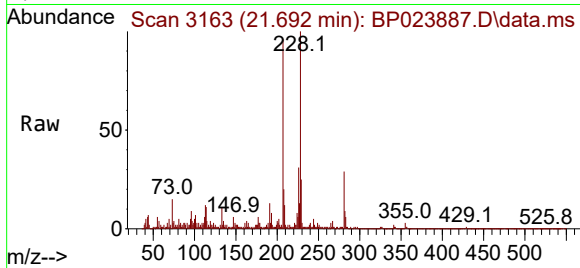

#90

Benzo(b)fluoranthene

Concen: 2.213 ng/ul

RT: 23.933 min Scan# 3544

Delta R.T. -0.012 min

Lab File: BP023887.D

Acq: 03 Feb 2025 19:56




Tgt Ion:252 Resp: 336085


Ion Ratio Lower Upper

252 100

253 23.9 17.5 26.3

125 13.7 8.2 12.2#

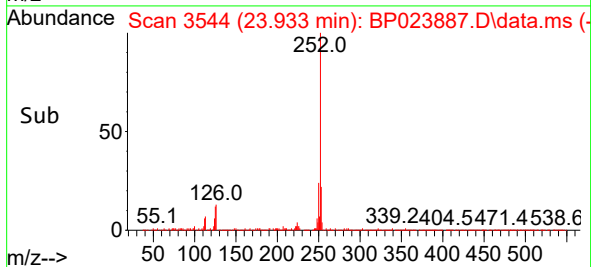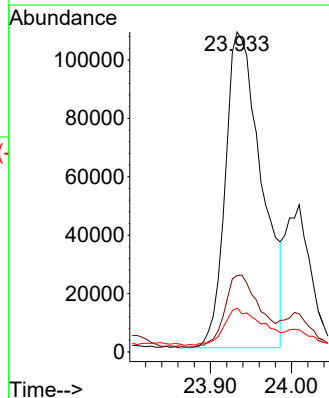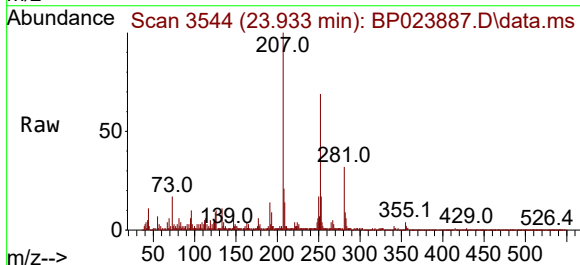

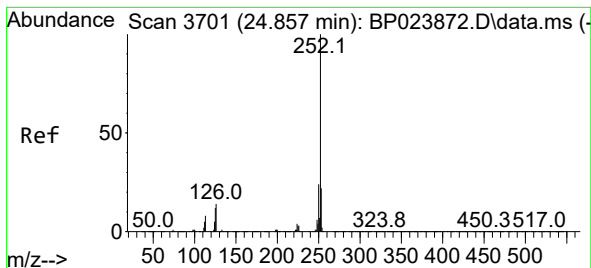

#93

Benzo(a)pyrene

Concen: 1.334 ng/ul

RT: 24.839 min Scan# 3

Delta R.T. -0.018 min

Lab File: BP023887.D

Acq: 03 Feb 2025 19:56

Instrument :

BNA_P

ClientSampleId :

A44T3





Tgt Ion:252 Resp: 189102

Ion Ratio Lower Upper

252 100

253 26.2 17.8 26.6

125 17.4 9.2 13.8#

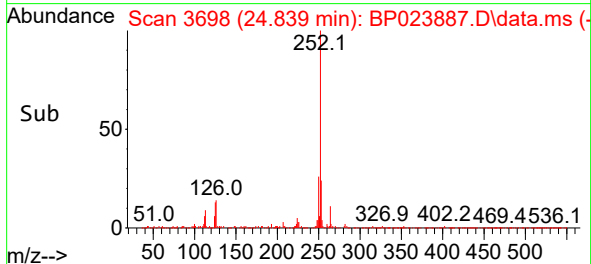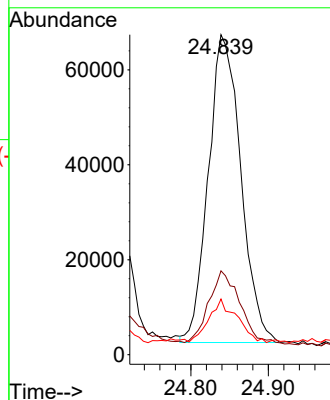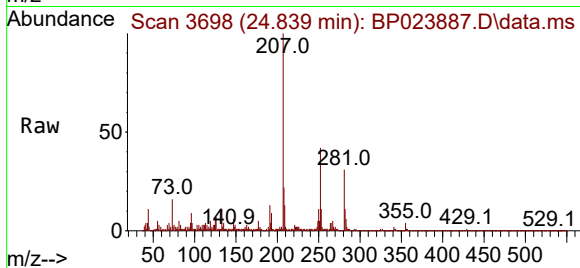

#96

Benzo(g,h,i)perylene

Concen: 1.046 ng/ul

RT: 30.027 min Scan# 4580

Delta R.T. 0.023 min

Lab File: BP023887.D

Acq: 03 Feb 2025 19:56

Tgt Ion:276 Resp: 147319

Ion Ratio Lower Upper

276 100

138 22.7 17.8 26.6

277 25.0 19.0 28.6

