

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020325\
 Data File : BP023889.D
 Acq On : 03 Feb 2025 21:17
 Operator : RC/JU
 Sample : Q1190-04
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A44S5

Quant Time: Feb 04 07:35:09 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Feb 03 11:19:36 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.775	152	428048	20.000	ng/ul	0.00
20) Naphthalene-d8	10.551	136	1845832	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.392	164	1183985	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.192	188	2314173	20.000	ng/ul	0.00
79) Chrysene-d12	21.633	240	2249608	20.000	ng/ul	0.00
88) Perylene-d12	25.015	264	2361099	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.293	96	43621	4.234	ng/uL	0.00
4) Pyridine-d5	3.704	84	539881	18.161	ng/ul	0.00
7) Phenol-d5	6.957	99	900262	23.766	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.110	67	480084	23.943	ng/ul	0.00
11) 2-Chlorophenol-d4	7.316	132	712653	23.957	ng/ul	0.00
15) 4-Methylphenol-d8	8.481	113	715949	23.136	ng/ul	0.00
21) Nitrobenzene-d5	8.922	128	342738	23.208	ng/ul	0.00
24) 2-Nitrophenol-d4	9.634	143	358300	22.485	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.181	165	687700	23.525	ng/ul	0.01
31) 4-Chloroaniline-d4	10.675	131	834026	19.078	ng/ul	0.00
46) Dimethylphthalate-d6	13.798	166	2084187	23.600	ng/ul	0.00
49) Acenaphthylene-d8	14.086	160	2259528	22.685	ng/ul	0.00
54) 4-Nitrophenol-d4	14.604	143	312118	17.796	ng/ul	0.00
60) Fluorene-d10	15.398	176	1625992	21.863	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.516	200	185463	12.991	ng/ul	0.00
73) Anthracene-d10	17.292	188	2354567	20.722	ng/ul	0.00
81) Pyrene-d10	19.657	212	2564871	21.279	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.774	264	2209436	17.935	ng/ul	0.00
Target Compounds						
					Qvalue	
8) Phenol	6.987	94	56146	1.443	ng/ul	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020325\
Data File : BP023889.D
Acq On : 03 Feb 2025 21:17
Operator : RC/JU
Sample : Q1190-04
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A44S5

Quant Time: Feb 04 07:35:09 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Feb 03 11:19:36 2025
Response via : Initial Calibration

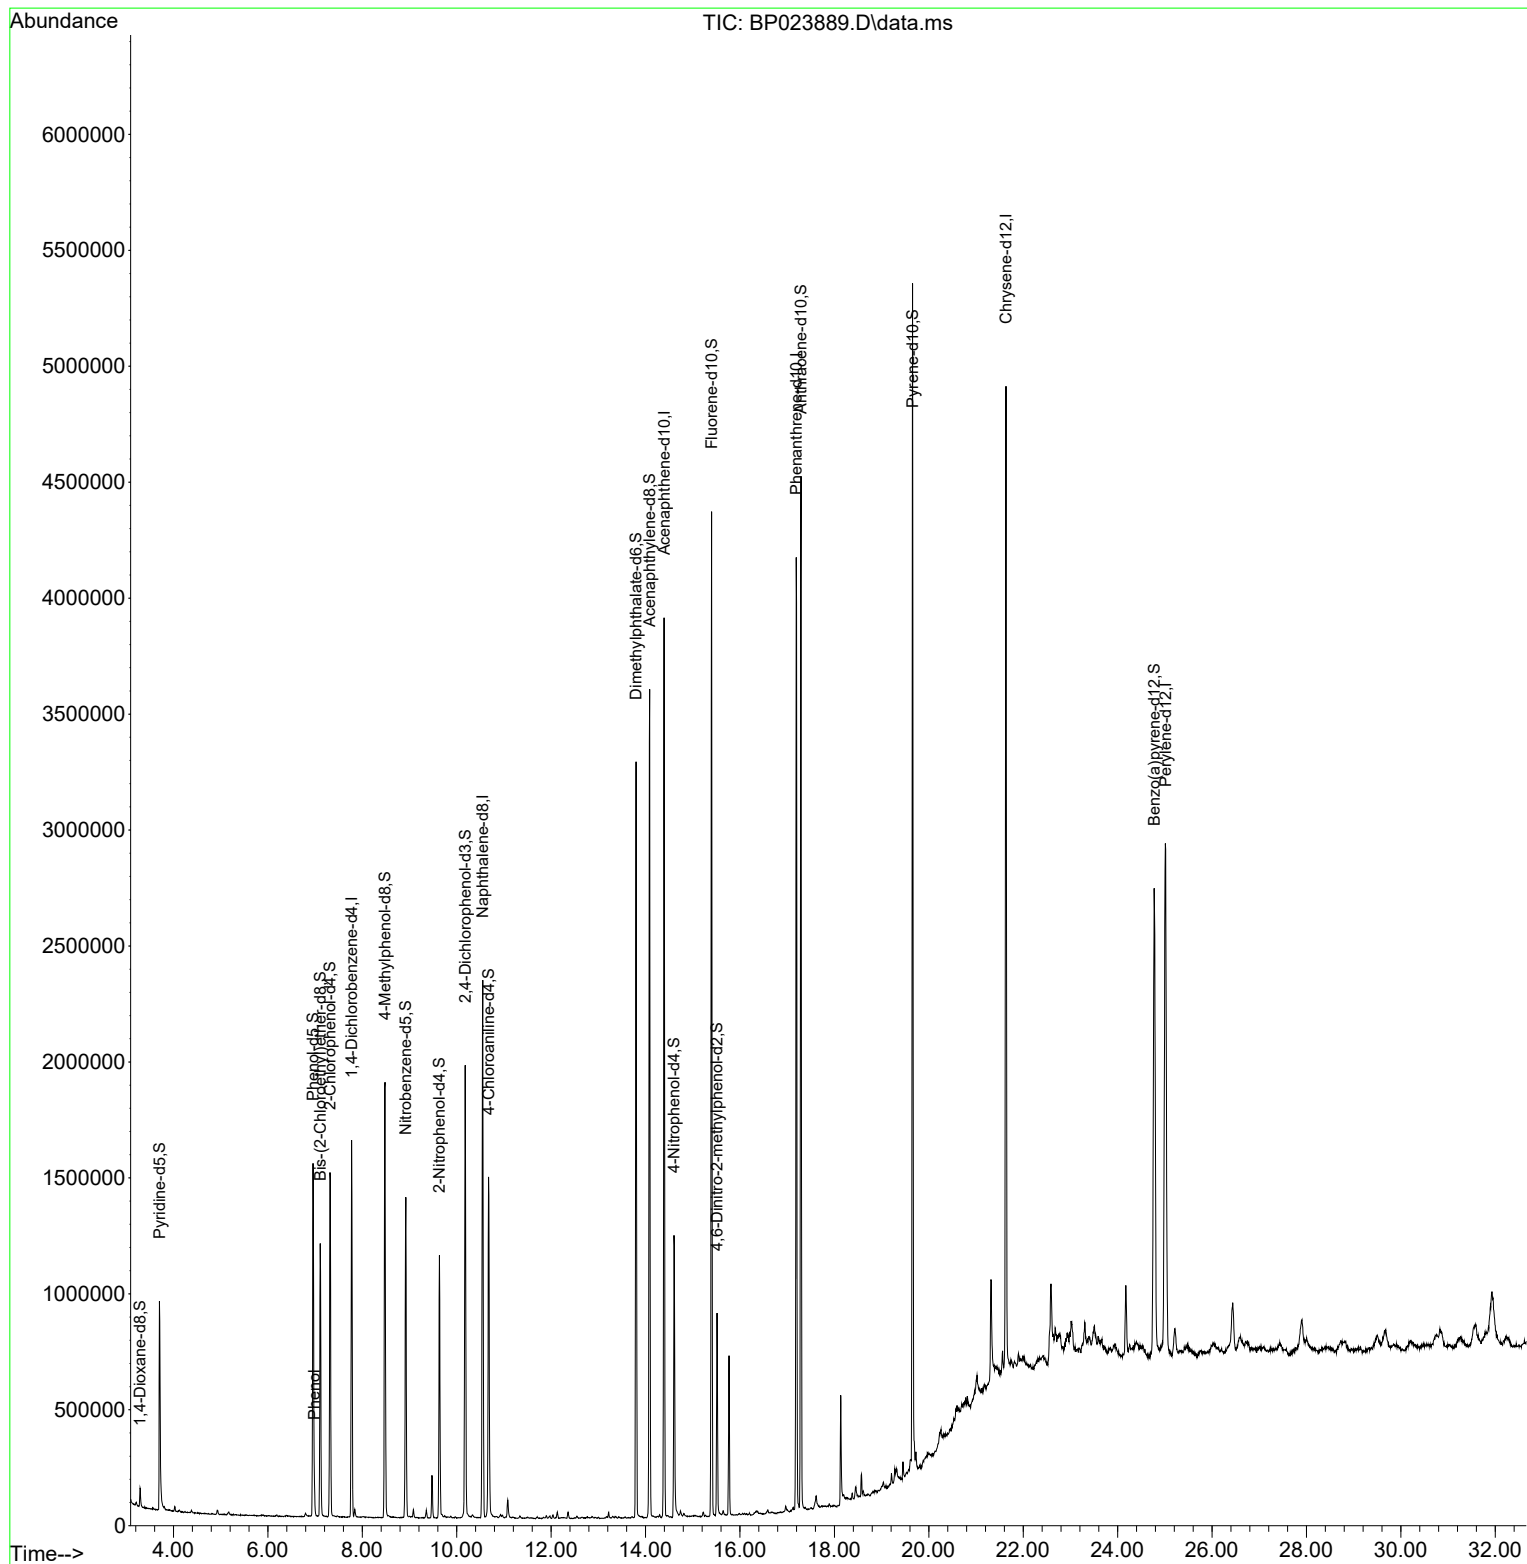

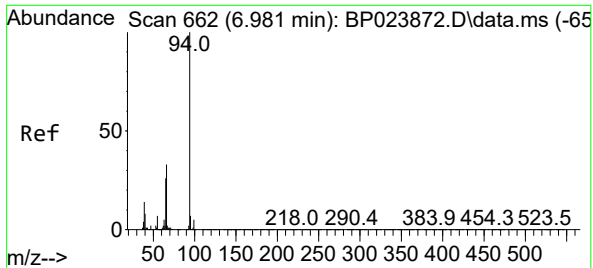

#8
 Phenol
 Concen: 1.443 ng/ul
 RT: 6.987 min Scan# 60
 Delta R.T. 0.005 min
 Lab File: BP023889.D
 Acq: 03 Feb 2025 21:17

Instrument :
 BNA_P
 ClientSampleId :
 A44S5

Tgt Ion: 94	Resp:	56146
Ion	Ratio	Lower Upper
94	100	
65	25.9	20.1 30.1
66	37.8	26.0 39.0

