

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020325\
 Data File : BP023890.D
 Acq On : 03 Feb 2025 21:58
 Operator : RC/JU
 Sample : Q1190-13
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A44T2

Quant Time: Feb 04 07:35:23 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Feb 03 11:19:36 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.775	152	473730	20.000	ng/ul	0.00
20) Naphthalene-d8	10.551	136	2045804	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.398	164	1261596	20.000	ng/ul	0.01
64) Phenanthrene-d10	17.192	188	2443209	20.000	ng/ul	0.00
79) Chrysene-d12	21.633	240	2315025	20.000	ng/ul	0.00
88) Perylene-d12	25.009	264	2433787	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.293	96	41760	3.663	ng/uL	0.00
4) Pyridine-d5	3.705	84	530104	16.112	ng/ul	0.00
7) Phenol-d5	6.957	99	833978	19.893	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.110	67	449986	20.278	ng/ul	0.00
11) 2-Chlorophenol-d4	7.316	132	670171	20.357	ng/ul	0.00
15) 4-Methylphenol-d8	8.475	113	659785	19.265	ng/ul	0.00
21) Nitrobenzene-d5	8.916	128	311453	19.028	ng/ul	0.00
24) 2-Nitrophenol-d4	9.634	143	320843	18.167	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.175	165	612764	18.913	ng/ul	0.00
31) 4-Chloroaniline-d4	10.681	131	714954	14.755	ng/ul	0.00
46) Dimethylphthalate-d6	13.798	166	1699833	18.064	ng/ul	0.00
49) Acenaphthylene-d8	14.086	160	2037077	19.193	ng/ul	0.00
54) 4-Nitrophenol-d4	14.610	143	270555	14.477	ng/ul	0.00
60) Fluorene-d10	15.398	176	1484794	18.737	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.516	200	155629	10.325	ng/ul	0.00
73) Anthracene-d10	17.292	188	2187616	18.236	ng/ul	0.00
81) Pyrene-d10	19.657	212	2424325	19.544	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.780	264	2285569	17.999	ng/ul	0.00
Target Compounds						
					Qvalue	
8) Phenol	6.981	94	53597	1.245	ng/ul	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020325\
Data File : BP023890.D
Acq On : 03 Feb 2025 21:58
Operator : RC/JU
Sample : Q1190-13
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A44T2

Quant Time: Feb 04 07:35:23 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Feb 03 11:19:36 2025
Response via : Initial Calibration

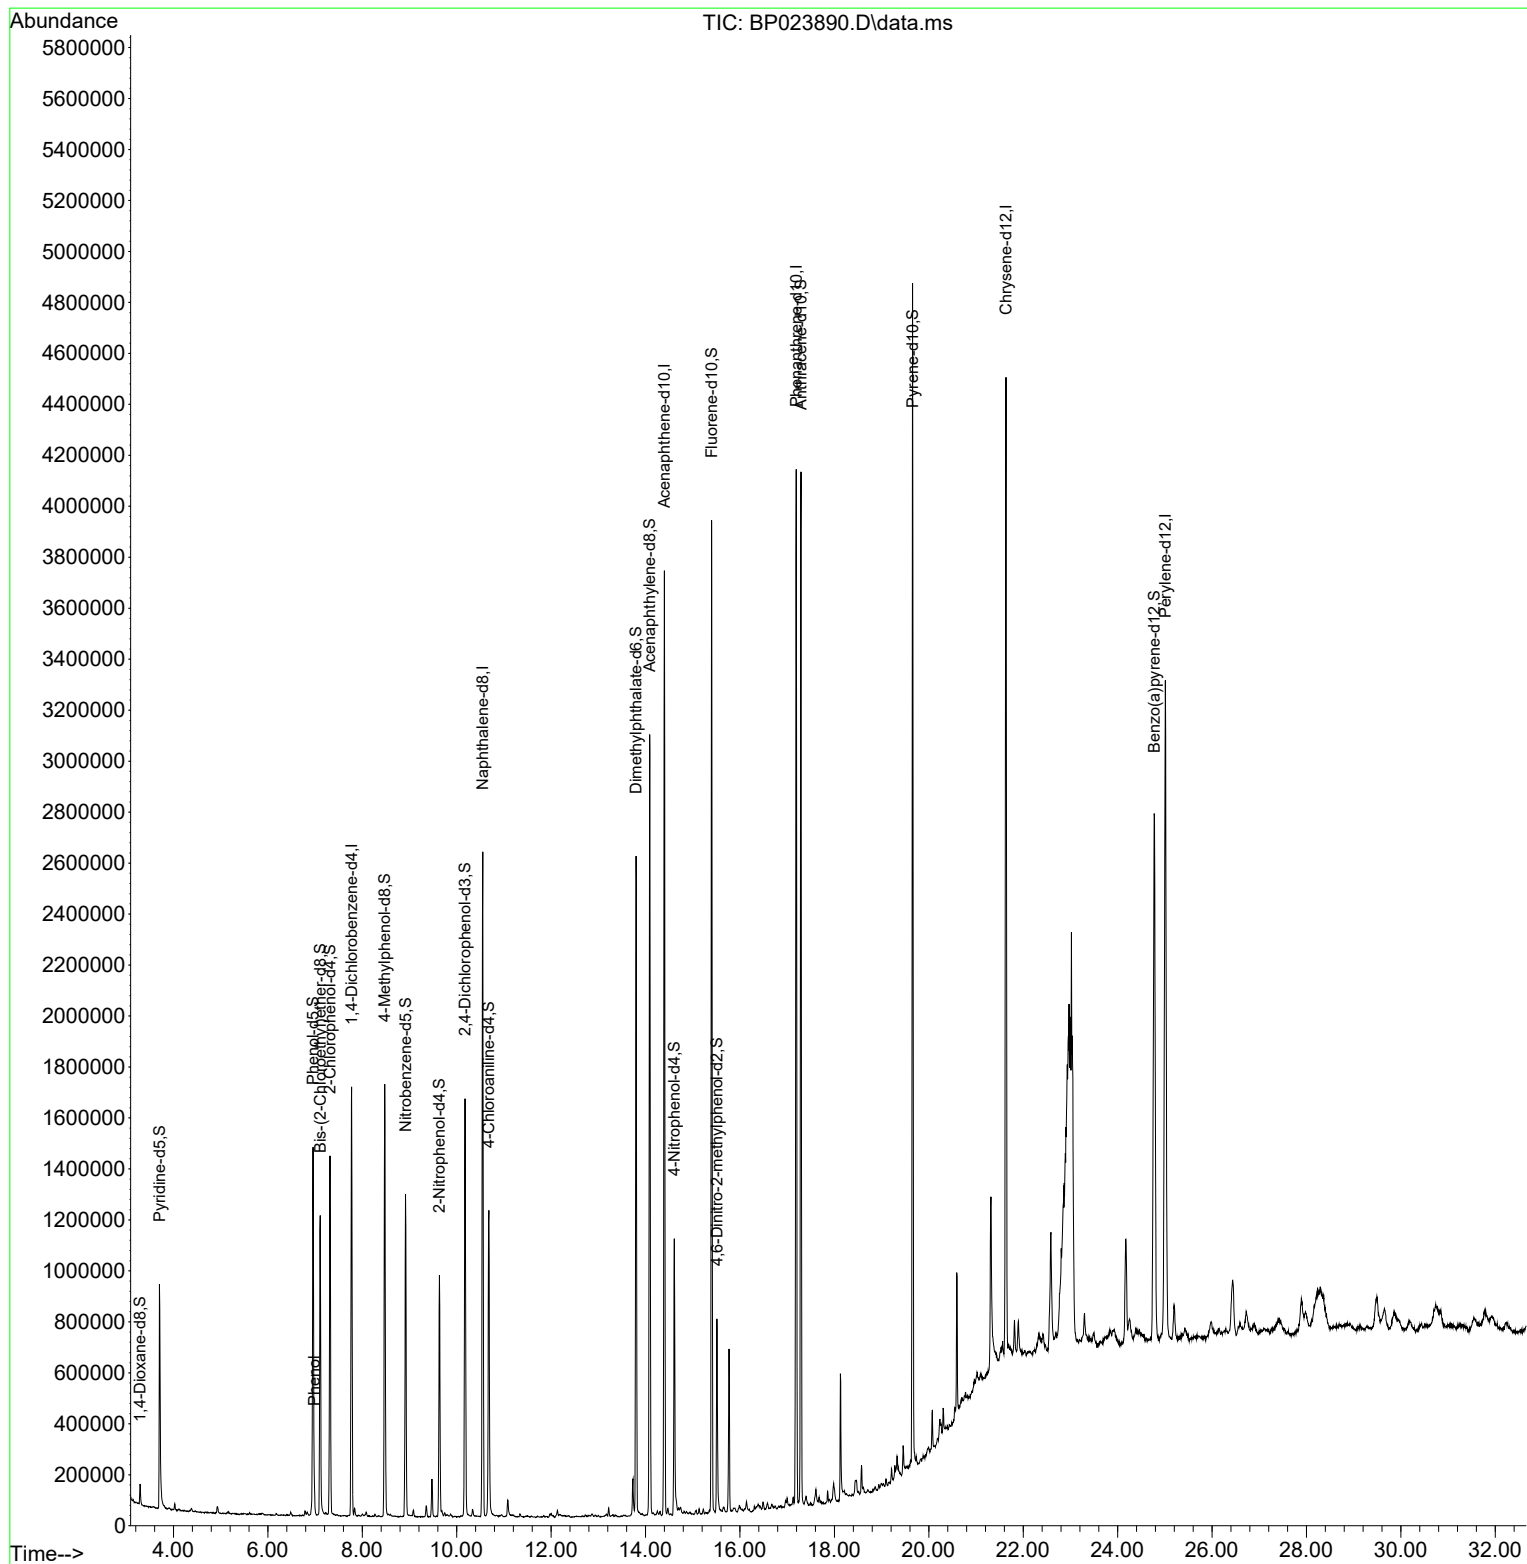

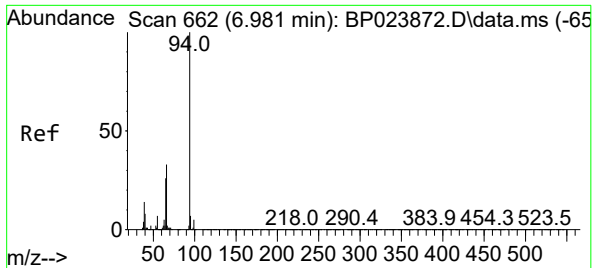

#8
Phenol
Concen: 1.245 ng/ul
RT: 6.981 min Scan# 6
Delta R.T. -0.000 min
Lab File: BP023890.D
Acq: 03 Feb 2025 21:58

Instrument :
BNA_P
ClientSampleId :
A44T2

Tgt Ion:	94	Resp:	53597
Ion	Ratio	Lower	Upper
94	100		
65	27.5	20.1	30.1
66	36.7	26.0	39.0

