

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020325\
 Data File : BP023892.D
 Acq On : 03 Feb 2025 23:19
 Operator : RC/JU
 Sample : Q1247-09
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A6336

Quant Time: Feb 04 07:35:53 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Feb 03 11:19:36 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.775	152	374169	20.000	ng/ul	0.00
20) Naphthalene-d8	10.552	136	1647105	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.398	164	1038659	20.000	ng/ul	0.01
64) Phenanthrene-d10	17.181	188	2053108	20.000	ng/ul	0.00
79) Chrysene-d12	21.645	240	1995084	20.000	ng/ul	0.00
88) Perylene-d12	25.015	264	2128815	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.299	96	24661	2.738	ng/uL	0.00
4) Pyridine-d5	3.717	84	121494	4.675	ng/ul	0.01
7) Phenol-d5	6.958	99	288532	8.714	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.111	67	334583	19.089	ng/ul	0.00
11) 2-Chlorophenol-d4	7.316	132	549792	21.144	ng/ul	0.00
15) 4-Methylphenol-d8	8.481	113	477607	17.657	ng/ul	0.00
21) Nitrobenzene-d5	8.922	128	217648	16.516	ng/ul	0.00
24) 2-Nitrophenol-d4	9.634	143	223953	15.750	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.181	165	508903	19.509	ng/ul	0.01
31) 4-Chloroaniline-d4	10.681	131	82937	2.126	ng/ul	0.00
46) Dimethylphthalate-d6	13.804	166	1420574	18.336	ng/ul	0.01
49) Acenaphthylene-d8	14.087	160	1440499	16.486	ng/ul	0.00
54) 4-Nitrophenol-d4	14.616	143	113362	7.368	ng/ul	0.00
60) Fluorene-d10	15.398	176	1184600	18.157	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.516	200	135175	10.672	ng/ul	0.00
73) Anthracene-d10	17.286	188	1787108	17.728	ng/ul	0.00
81) Pyrene-d10	19.669	212	2062061	19.290	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.786	264	1870066	16.837	ng/ul	0.01
Target Compounds						
					Qvalue	
8) Phenol	6.987	94	53590	1.576	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020325\
Data File : BP023892.D
Acq On : 03 Feb 2025 23:19
Operator : RC/JU
Sample : Q1247-09
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A6336

Quant Time: Feb 04 07:35:53 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Feb 03 11:19:36 2025
Response via : Initial Calibration

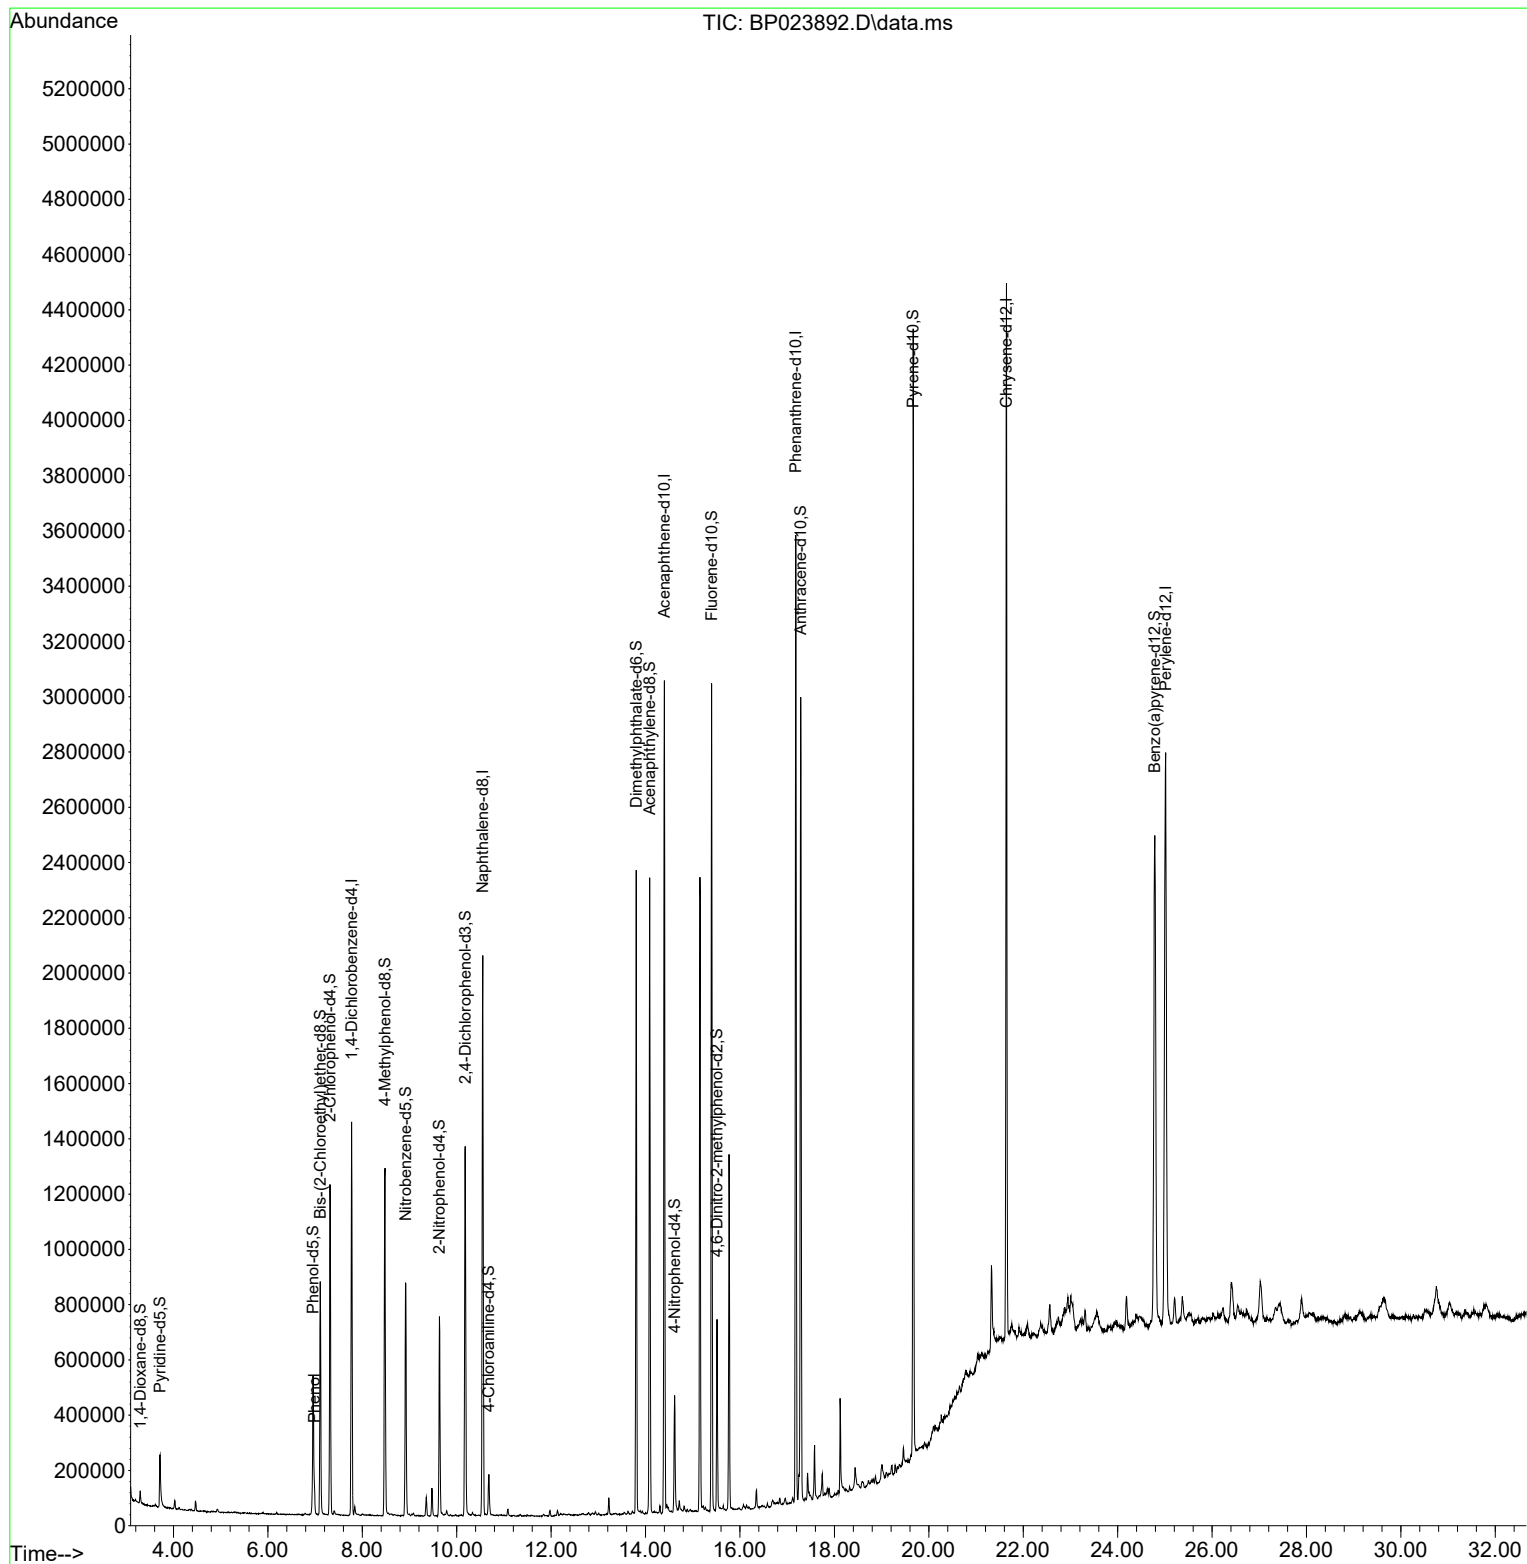

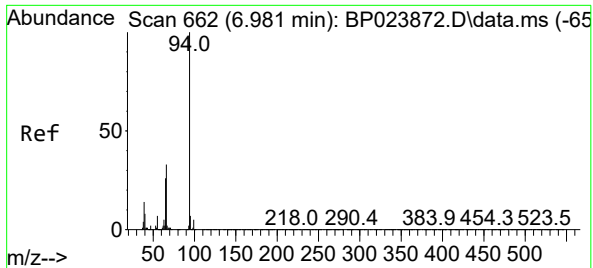

#8
Phenol
Concen: 1.576 ng/ul
RT: 6.987 min Scan# 60
Delta R.T. 0.006 min
Lab File: BP023892.D
Acq: 03 Feb 2025 23:19

Instrument :
BNA_P
ClientSampleId :
A6336

Tgt Ion: 94	Resp:	53590
Ion	Ratio	Lower Upper
94	100	
65	25.3	20.1 30.1
66	32.7	26.0 39.0

