

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020325\
 Data File : BP023915.D
 Acq On : 04 Feb 2025 16:46
 Operator : RC/JU
 Sample : Q1202-09
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E29A0

Quant Time: Feb 05 07:34:08 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Feb 03 11:19:36 2025
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.758	152	409931	20.000	ng/ul	-0.02
20) Naphthalene-d8	10.534	136	1741957	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.387	164	1089989	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.187	188	2195941	20.000	ng/ul	0.00
79) Chrysene-d12	21.639	240	2222692	20.000	ng/ul	0.00
88) Perylene-d12	25.010	264	2388171	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.281	96	61742	6.258	ng/uL	-0.01
4) Pyridine-d5	3.693	84	320147	11.245	ng/ul	-0.01
7) Phenol-d5	6.940	99	366701	10.108	ng/ul	-0.02
9) Bis-(2-Chloroethyl)eth...	7.093	67	566781	29.516	ng/ul	-0.01
11) 2-Chlorophenol-d4	7.299	132	785856	27.586	ng/ul	-0.02
15) 4-Methylphenol-d8	8.464	113	637078	21.498	ng/ul	-0.01
21) Nitrobenzene-d5	8.905	128	395069	28.347	ng/ul	-0.01
24) 2-Nitrophenol-d4	9.622	143	419204	27.876	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.163	165	763300	27.668	ng/ul	0.00
31) 4-Chloroaniline-d4	10.669	131	1306602	31.670	ng/ul	0.00
46) Dimethylphthalate-d6	13.787	166	2448551	30.117	ng/ul	0.00
49) Acenaphthylene-d8	14.075	160	2777555	30.290	ng/ul	0.00
54) 4-Nitrophenol-d4	14.604	143	144153	8.928	ng/ul	0.00
60) Fluorene-d10	15.398	176	2141356	31.276	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.510	200	309249	22.827	ng/ul	0.00
73) Anthracene-d10	17.287	188	3715770	34.463	ng/ul	0.00
81) Pyrene-d10	19.663	212	4364710	36.649	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.786	264	4556305	36.566	ng/ul	0.01
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.557	149	123751	1.373	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020325\
Data File : BP023915.D
Acq On : 04 Feb 2025 16:46
Operator : RC/JU
Sample : Q1202-09
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E29A0

Quant Time: Feb 05 07:34:08 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Feb 03 11:19:36 2025
Response via : Initial Calibration

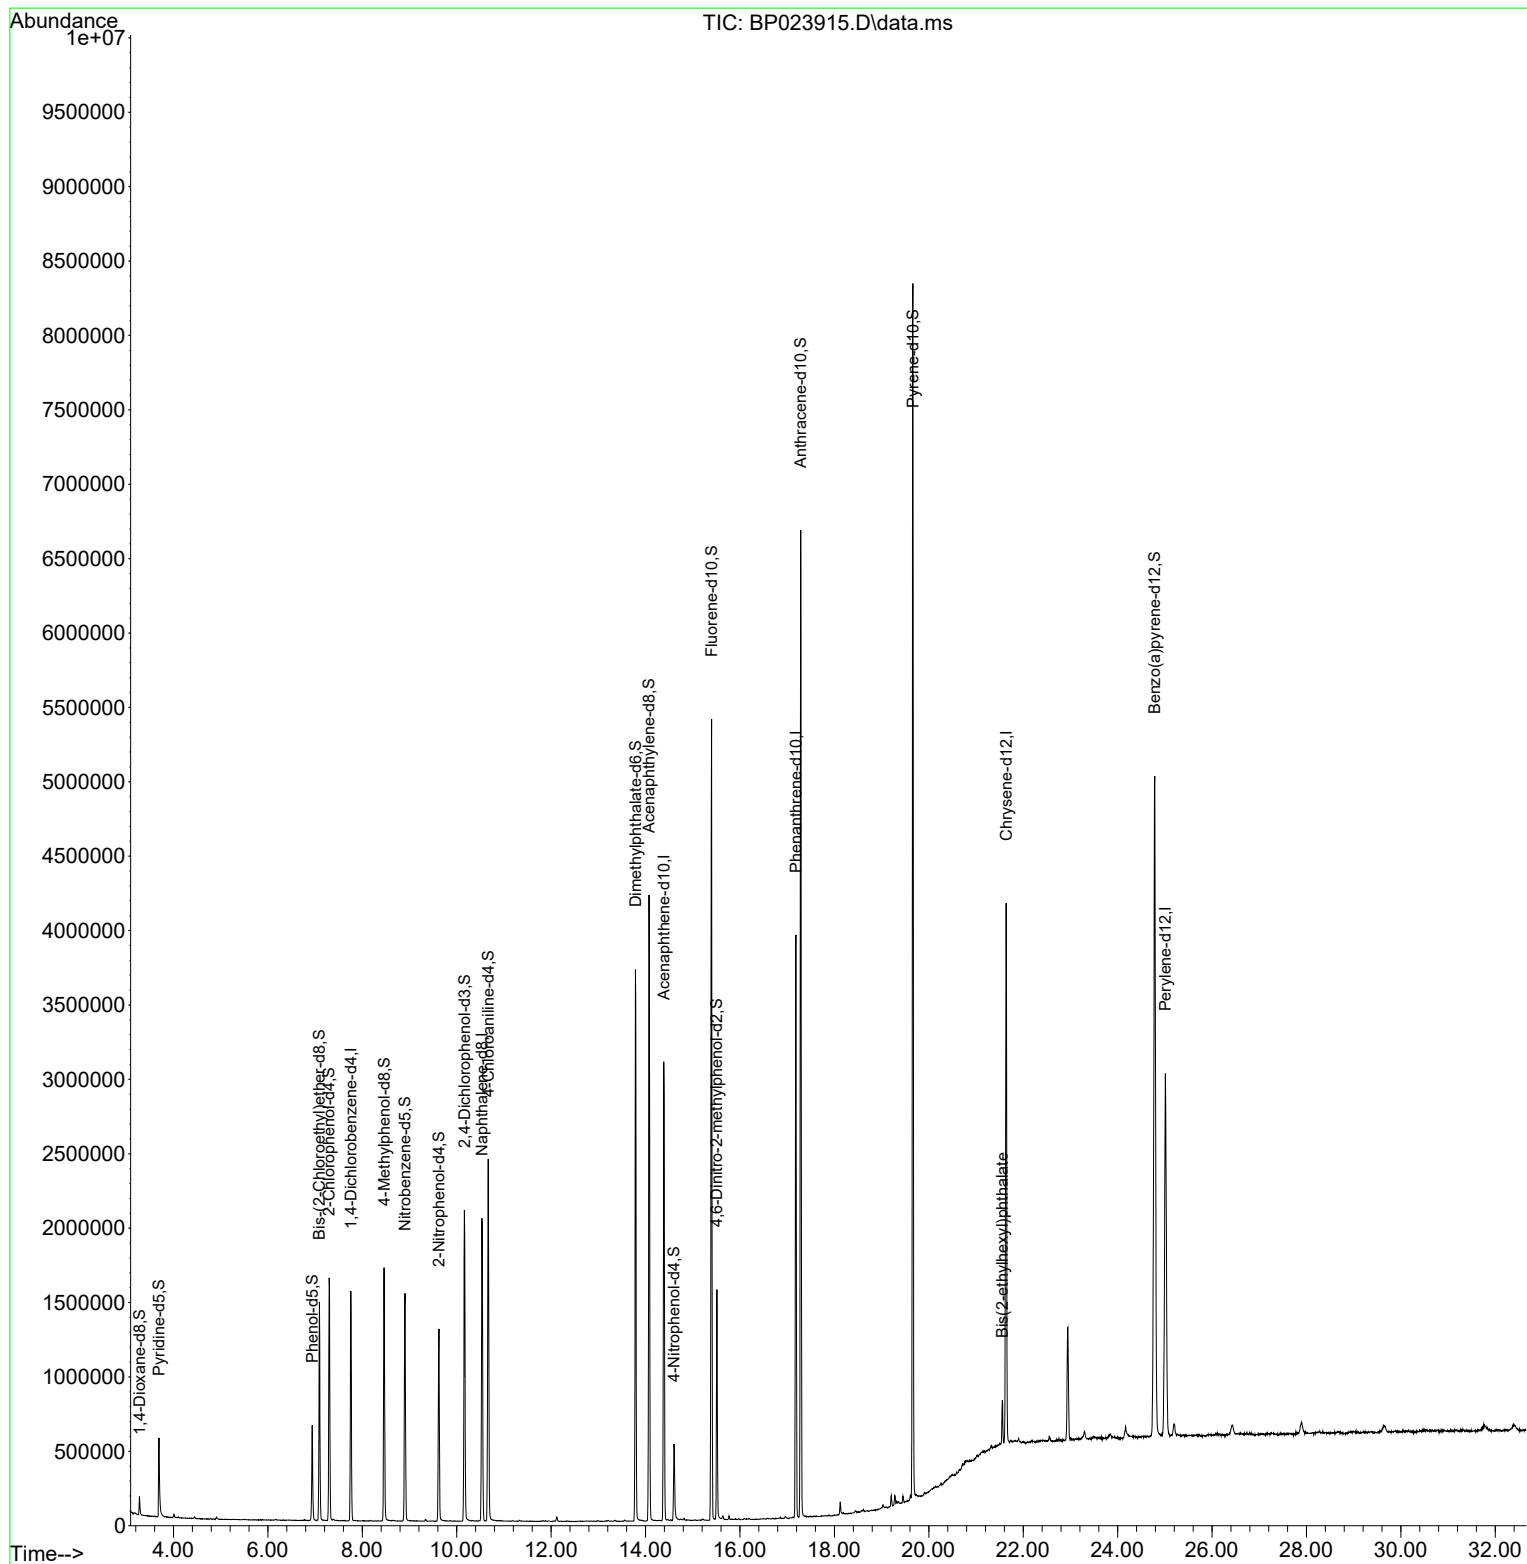

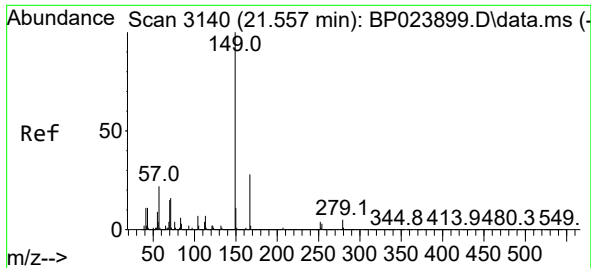

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 1.373 ng/ul
 RT: 21.557 min Scan# 31
 Delta R.T. -0.006 min
 Lab File: BP023915.D
 Acq: 04 Feb 2025 16:46

Instrument :
 BNA_P
 ClientSampleId :
 E29A0

Tgt Ion:149 Resp: 123751
 Ion Ratio Lower Upper
 149 100
 167 26.5 22.6 33.8
 279 4.5 3.8 5.6

