

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP020325\  
 Data File : BP023915.D  
 Acq On : 04 Feb 2025 16:46  
 Operator : RC/JU  
 Sample : Q1202-09  
 Misc :  
 ALS Vial : 45 Sample Multiplier: 1

Instrument :  
 BNA\_P  
 ClientSampleId :  
 E29A0

Quant Time: Feb 05 07:34:08 2025  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\SFAM-EPA-BP012925.MA.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Mon Feb 03 11:19:36 2025  
 Response via : Initial Calibration


| Compound                      | R.T.   | QIon | Response | Conc   | Units | Dev(Min)  |
|-------------------------------|--------|------|----------|--------|-------|-----------|
| -----                         |        |      |          |        |       |           |
| Internal Standards            |        |      |          |        |       |           |
| 1) 1,4-Dichlorobenzene-d4     | 7.758  | 152  | 409931   | 20.000 | ng/u1 | -0.02     |
| 20) Naphthalene-d8            | 10.534 | 136  | 1741957  | 20.000 | ng/u1 | -0.01     |
| 38) Acenaphthene-d10          | 14.387 | 164  | 1089989  | 20.000 | ng/u1 | 0.00      |
| 64) Phenanthrene-d10          | 17.187 | 188  | 2195941  | 20.000 | ng/u1 | 0.00      |
| 79) Chrysene-d12              | 21.639 | 240  | 2222692  | 20.000 | ng/u1 | 0.00      |
| 88) Perylene-d12              | 25.010 | 264  | 2388171  | 20.000 | ng/u1 | 0.00      |
| System Monitoring Compounds   |        |      |          |        |       |           |
| 3) 1,4-Dioxane-d8             | 3.281  | 96   | 61742    | 6.258  | ng/uL | -0.01     |
| 4) Pyridine-d5                | 3.693  | 84   | 320147   | 11.245 | ng/u1 | -0.01     |
| 7) Phenol-d5                  | 6.940  | 99   | 366701   | 10.108 | ng/u1 | -0.02     |
| 9) Bis-(2-Chloroethyl)eth...  | 7.093  | 67   | 566781   | 29.516 | ng/u1 | -0.01     |
| 11) 2-Chlorophenol-d4         | 7.299  | 132  | 785856   | 27.586 | ng/u1 | -0.02     |
| 15) 4-Methylphenol-d8         | 8.464  | 113  | 637078   | 21.498 | ng/u1 | -0.01     |
| 21) Nitrobenzene-d5           | 8.905  | 128  | 395069   | 28.347 | ng/u1 | -0.01     |
| 24) 2-Nitrophenol-d4          | 9.622  | 143  | 419204   | 27.876 | ng/u1 | 0.00      |
| 28) 2,4-Dichlorophenol-d3     | 10.163 | 165  | 763300   | 27.668 | ng/u1 | 0.00      |
| 31) 4-Chloroaniline-d4        | 10.669 | 131  | 1306602  | 31.670 | ng/u1 | 0.00      |
| 46) Dimethylphthalate-d6      | 13.787 | 166  | 2448551  | 30.117 | ng/u1 | 0.00      |
| 49) Acenaphthylene-d8         | 14.075 | 160  | 2777555  | 30.290 | ng/u1 | 0.00      |
| 54) 4-Nitrophenol-d4          | 14.604 | 143  | 144153   | 8.928  | ng/u1 | 0.00      |
| 60) Fluorene-d10              | 15.398 | 176  | 2141356  | 31.276 | ng/u1 | 0.00      |
| 65) 4,6-Dinitro-2-methylph... | 15.510 | 200  | 309249   | 22.827 | ng/u1 | 0.00      |
| 73) Anthracene-d10            | 17.287 | 188  | 3715770  | 34.463 | ng/u1 | 0.00      |
| 81) Pyrene-d10                | 19.663 | 212  | 4364710  | 36.649 | ng/u1 | 0.00      |
| 92) Benzo(a)pyrene-d12        | 24.786 | 264  | 4556305  | 36.566 | ng/u1 | 0.01      |
| Target Compounds              |        |      |          |        |       |           |
| 86) Bis(2-ethylhexyl)phtha... | 21.557 | 149  | 123751   | 1.373  | ng/u1 | Qvalue 97 |
| -----                         |        |      |          |        |       |           |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP020325\  
Data File : BP023915.D  
Acq On : 04 Feb 2025 16:46  
Operator : RC/JU  
Sample : Q1202-09  
Misc :  
ALS Vial : 45 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
E29A0

Quant Time: Feb 05 07:34:08 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\SFAM-EPA-BP012925.MA.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Mon Feb 03 11:19:36 2025  
Response via : Initial Calibration

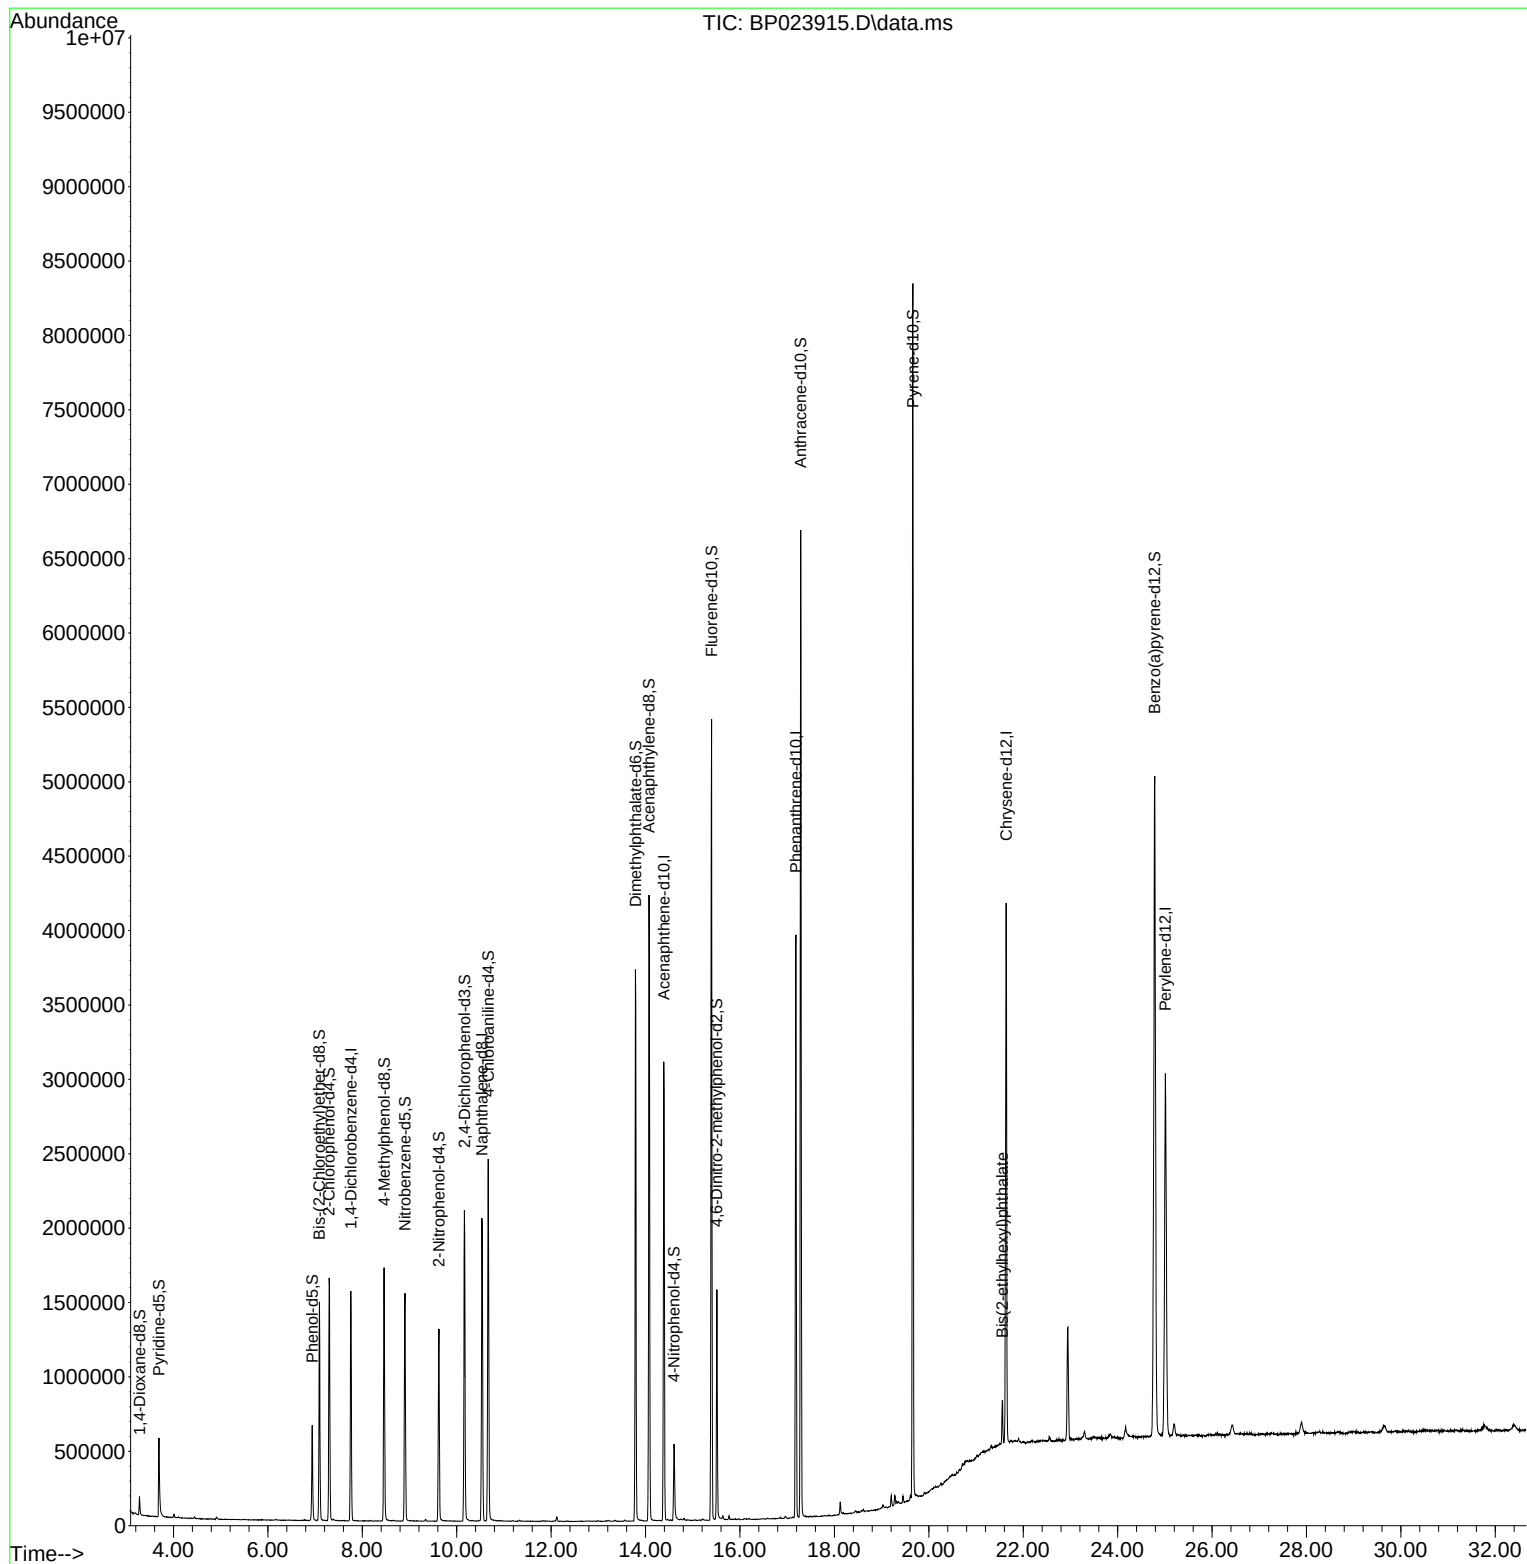

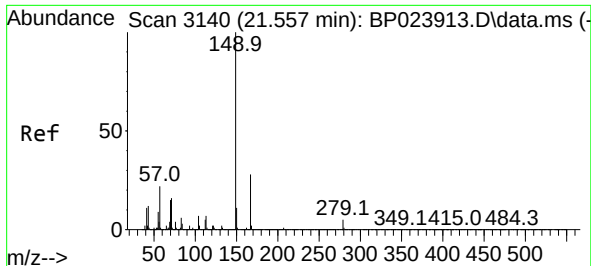

#86  
 Bis(2-ethylhexyl)phthalate  
 Concen: 1.373 ng/ul  
 RT: 21.557 min Scan# 31  
 Delta R.T. -0.006 min  
 Lab File: BP023915.D  
 Acq: 04 Feb 2025 16:46

Instrument :  
 BNA\_P  
 ClientSampleId :  
 E29A0

Tgt Ion:149 Resp: 123751  
 Ion Ratio Lower Upper  
 149 100  
 167 26.5 22.6 33.8  
 279 4.5 3.8 5.6

