

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020325\
 Data File : BP023876.D
 Acq On : 03 Feb 2025 12:32
 Operator : RC/JU
 Sample : Q1247-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A6317

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP023876.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.293	32	35	47	rVB	124462	173835	1.17%	0.126%
2	3.705	101	105	126	rBV	1607675	2411548	16.17%	1.744%
3	3.852	127	130	140	rVB	40312	59331	0.40%	0.043%
4	3.970	147	150	154	rBV3	13273	18391	0.12%	0.013%
5	4.028	157	160	167	rVB	30689	41259	0.28%	0.030%
6	4.928	309	313	320	rVB	18008	24676	0.17%	0.018%
7	6.964	651	659	667	rBV	2033448	3302675	22.14%	2.388%
8	7.111	677	684	698	rBV	1696942	2604025	17.46%	1.883%
9	7.322	712	720	730	rBV	2169510	3298731	22.11%	2.385%
10	7.411	732	735	741	rVB	23145	35913	0.24%	0.026%
11	7.781	791	798	807	rVB	1379772	2187584	14.67%	1.582%
12	8.481	909	917	931	rBV	2748933	4361133	29.24%	3.153%
13	8.916	984	991	1000	rBV	1919145	3141479	21.06%	2.271%
14	9.640	1101	1114	1126	rBV	1553105	2661892	17.85%	1.925%
15	10.181	1198	1206	1225	rBV	2794350	4411655	29.58%	3.190%
16	10.552	1259	1269	1275	rBV	1966428	3313884	22.22%	2.396%
17	10.605	1275	1278	1284	rVB	276684	404115	2.71%	0.292%
18	10.687	1284	1292	1304	rBV	2839502	4593191	30.79%	3.321%
19	12.140	1534	1539	1546	rVB	44139	73020	0.49%	0.053%
20	13.357	1739	1746	1752	rVB6	8204	17809	0.12%	0.013%
21	13.798	1814	1821	1835	rBV	4757625	6629806	44.45%	4.793%
22	14.087	1863	1870	1874	rBV2	5481233	8991562	60.28%	6.501%
23	14.398	1914	1923	1929	rBV	2967426	4438181	29.75%	3.209%
24	14.463	1929	1934	1945	rVB	2310060	3335763	22.36%	2.412%
25	14.610	1952	1959	1980	rBV	1973461	3240645	21.73%	2.343%
26	14.822	1991	1995	2000	rVB4	43671	58745	0.39%	0.042%
27	15.410	2087	2095	2101	rBV	6809598	10260259	68.79%	7.418%
28	15.469	2101	2105	2109	rVV	448815	606348	4.06%	0.438%
29	15.516	2109	2113	2126	rVB	1708273	2358599	15.81%	1.705%
30	15.645	2131	2135	2144	rVV	31001	64132	0.43%	0.046%
31	16.981	2357	2362	2370	rBV3	24557	48390	0.32%	0.035%
32	17.198	2391	2399	2403	rBV2	3189505	5141880	34.47%	3.718%
33	17.239	2403	2406	2410	rVV	869901	1205128	8.08%	0.871%
34	17.298	2410	2416	2420	rVV	8627659	11741544	78.72%	8.489%
35	17.334	2420	2422	2429	rVV	963650	1009861	6.77%	0.730%
36	17.398	2430	2433	2437	rVB5	24034	31443	0.21%	0.023%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020325\
Data File : BP023876.D
Acq On : 03 Feb 2025 12:32
Operator : RC/JU
Sample : Q1247-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A6317

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Title : SVOA CALIBRATION

37	19.210	2736	2741	2745	rBV	90264	130429	0.87%	0.094%
38	19.281	2750	2753	2754	rVV	81286	85304	0.57%	0.062%
39	19.310	2754	2758	2765	rVB	759773	1093266	7.33%	0.790%
40	19.657	2811	2817	2831	rVB	9827574	14916364	100.00%	10.785%
41	21.627	3145	3152	3158	rBV2	3513488	5986898	40.14%	4.329%
42	21.680	3158	3161	3167	rVB	260831	381949	2.56%	0.276%
43	23.933	3539	3544	3551	rVB	481880	1024566	6.87%	0.741%
44	24.774	3679	3687	3697	rBV	5253516	12829025	86.01%	9.276%
45	24.998	3717	3725	3739	rVB	2043499	5563265	37.30%	4.022%




Sum of corrected areas: 138309498

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020325\
Data File : BP023876.D
Acq On : 03 Feb 2025 12:32
Operator : RC/JU
Sample : Q1247-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A6317

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

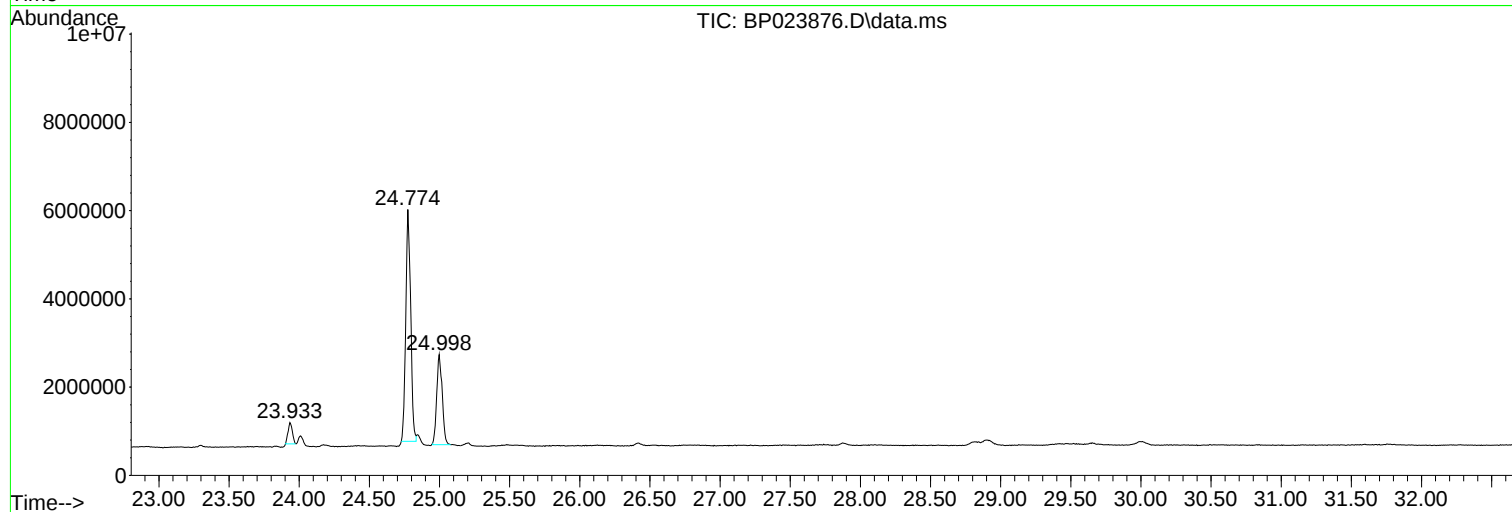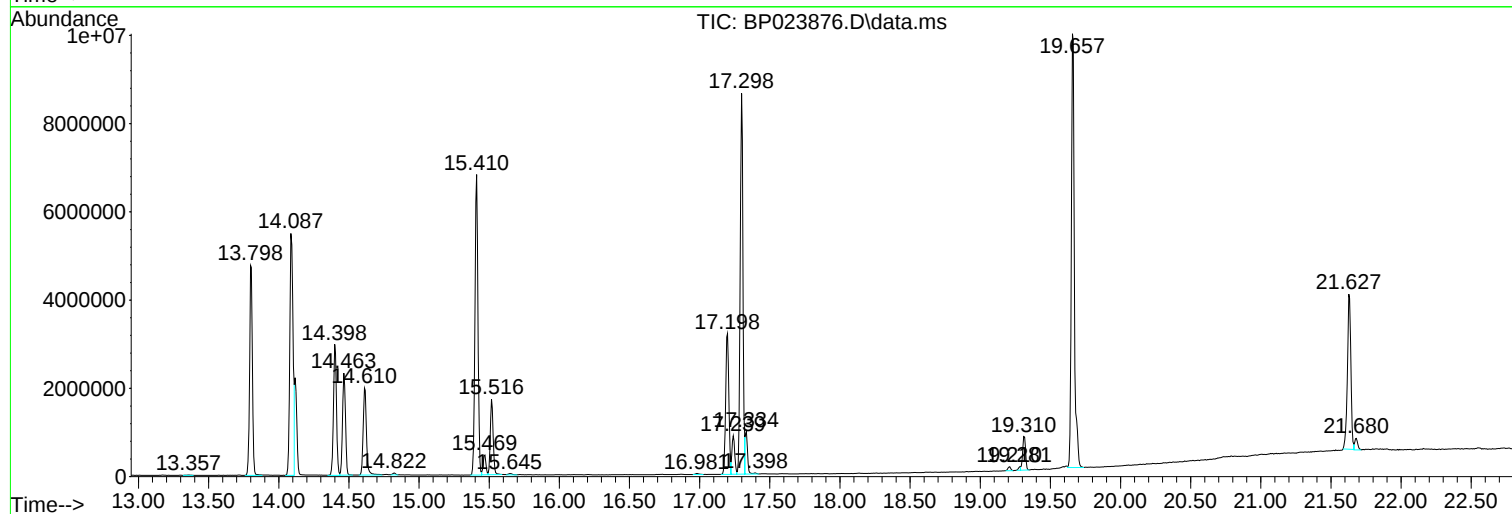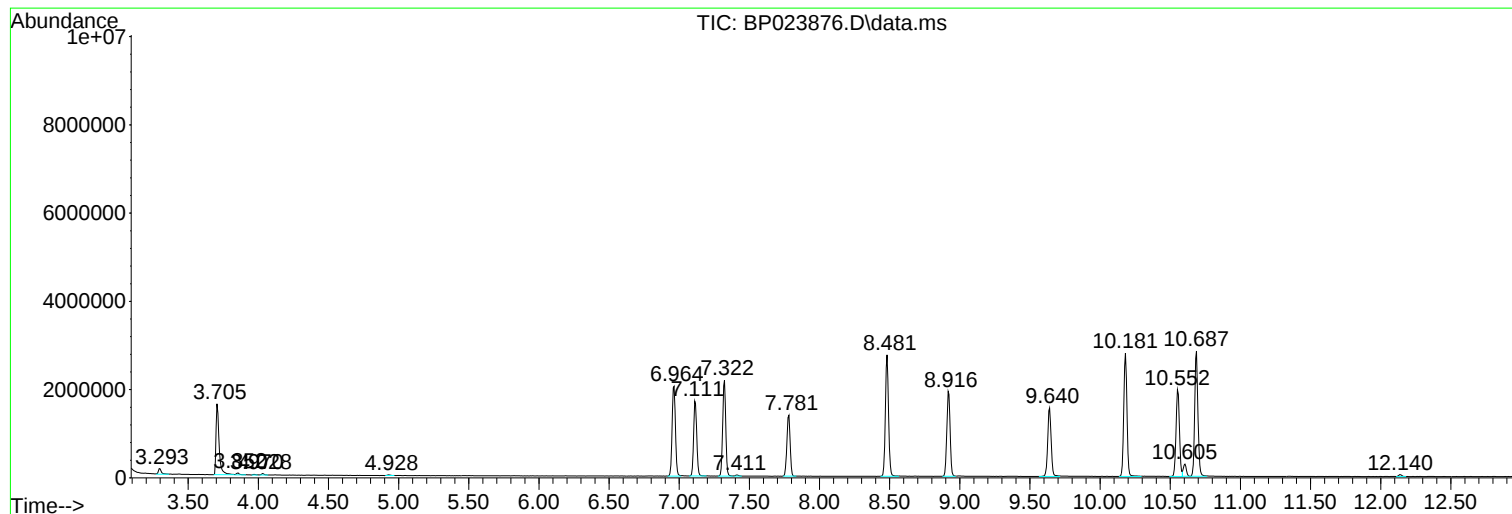

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020325\
Data File : BP023876.D
Acq On : 03 Feb 2025 12:32
Operator : RC/JU
Sample : Q1247-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A6317

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020325\
Data File : BP023876.D
Acq On : 03 Feb 2025 12:32
Operator : RC/JU
Sample : Q1247-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A6317

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------