

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020325\
 Data File : BP023884.D
 Acq On : 03 Feb 2025 17:55
 Operator : RC/JU
 Sample : PB166466BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK466

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP023884.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.299	32	36	46	rVB	116603	152636	1.47%	0.143%
2	3.711	102	106	125	rBV	1510398	2239011	21.52%	2.104%
3	4.034	157	161	167	rVB	29181	39181	0.38%	0.037%
4	6.964	652	659	677	rBV	1871549	2954771	28.40%	2.776%
5	7.117	678	685	696	rVV	1414261	2182155	20.98%	2.050%
6	7.328	713	721	728	rBV	1977122	2953829	28.39%	2.775%
7	7.781	790	798	811	rBV	1378341	2066641	19.87%	1.942%
8	8.481	909	917	929	rBV	2386983	3726345	35.82%	3.501%
9	8.922	985	992	1004	rBV	1619589	2599845	24.99%	2.443%
10	9.052	1009	1014	1019	rVV2	16366	24167	0.23%	0.023%
11	9.640	1106	1114	1131	rBV	1225317	2059418	19.80%	1.935%
12	10.181	1197	1206	1223	rBV	2313099	3678088	35.36%	3.456%
13	10.558	1261	1270	1280	rBV	1848501	3084408	29.65%	2.898%
14	10.687	1284	1292	1311	rVV	2166518	3668693	35.27%	3.447%
15	12.140	1532	1539	1544	rBV	33801	58370	0.56%	0.055%
16	13.363	1744	1747	1753	rVB6	7376	13933	0.13%	0.013%
17	13.804	1815	1822	1838	rBV	4062090	5217704	50.16%	4.903%
18	14.093	1863	1871	1884	rBV2	4389028	6543449	62.90%	6.148%
19	14.404	1916	1924	1934	rBV	2776493	4238629	40.75%	3.983%
20	14.610	1952	1959	1973	rBV	1591500	2504453	24.08%	2.353%
21	15.410	2087	2095	2108	rBV	5392144	8121522	78.07%	7.631%
22	15.522	2108	2114	2126	rBV	1332981	1803202	17.33%	1.694%
23	15.651	2132	2136	2142	rVB2	24519	38251	0.37%	0.036%
24	16.981	2358	2362	2369	rVB	14840	23981	0.23%	0.023%
25	17.198	2392	2399	2407	rBV2	3401751	5103174	49.06%	4.795%
26	17.298	2410	2416	2427	rBV	6859766	9007680	86.59%	8.464%
27	17.892	2514	2517	2521	rVB5	10303	11295	0.11%	0.011%
28	18.134	2555	2558	2562	rBV5	12035	16853	0.16%	0.016%
29	19.210	2737	2741	2748	rBV2	63131	91426	0.88%	0.086%
30	19.281	2749	2753	2759	rBV	59454	92809	0.89%	0.087%
31	19.663	2812	2818	2826	rBV	7615101	10363902	99.63%	9.738%
32	21.633	3147	3153	3161	rBV	3455890	5483861	52.72%	5.153%
33	24.786	3679	3689	3703	rVB	3721839	10402692	100.00%	9.774%
34	25.004	3719	3726	3742	rVB	2266930	5862627	56.36%	5.508%

Sum of corrected areas: 106429001




Instrument :
BNA_P
ClientSampleId :
SBLK466

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020325\
Data File : BP023884.D
Acq On : 03 Feb 2025 17:55
Operator : RC/JU
Sample : PB166466BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK466

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

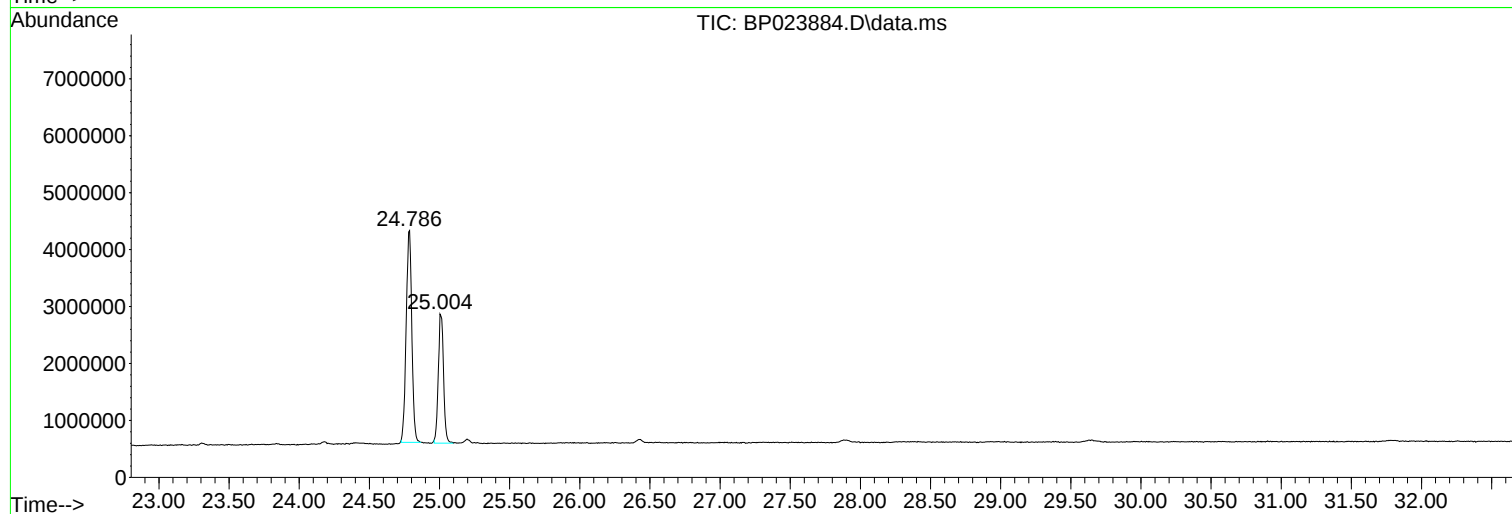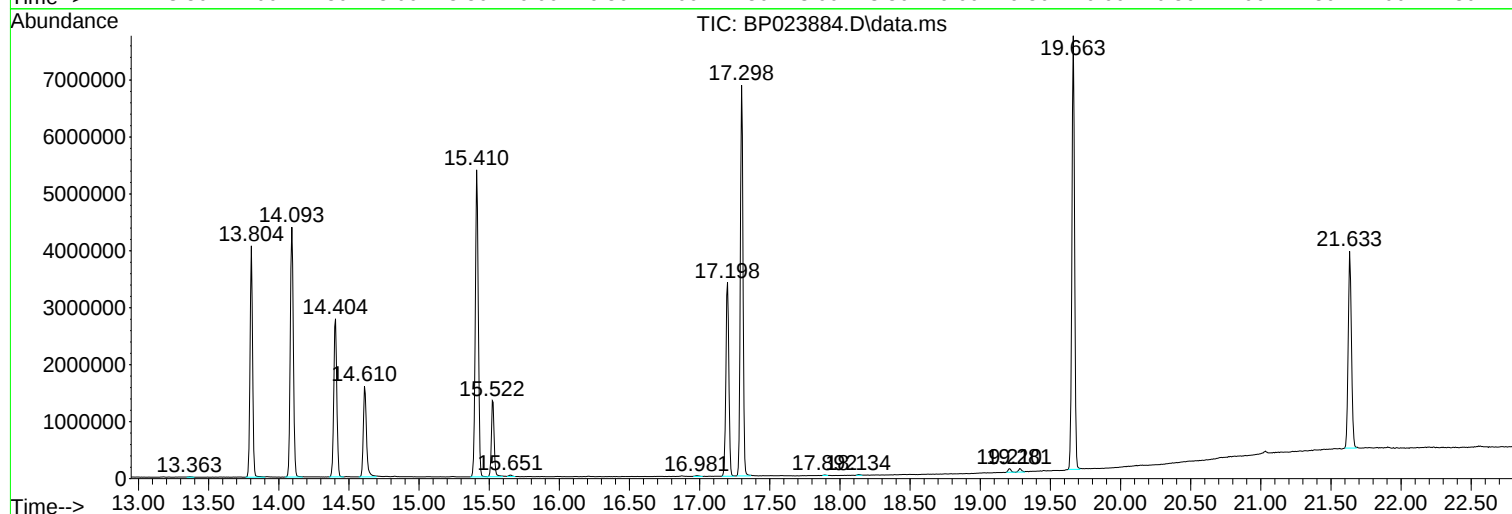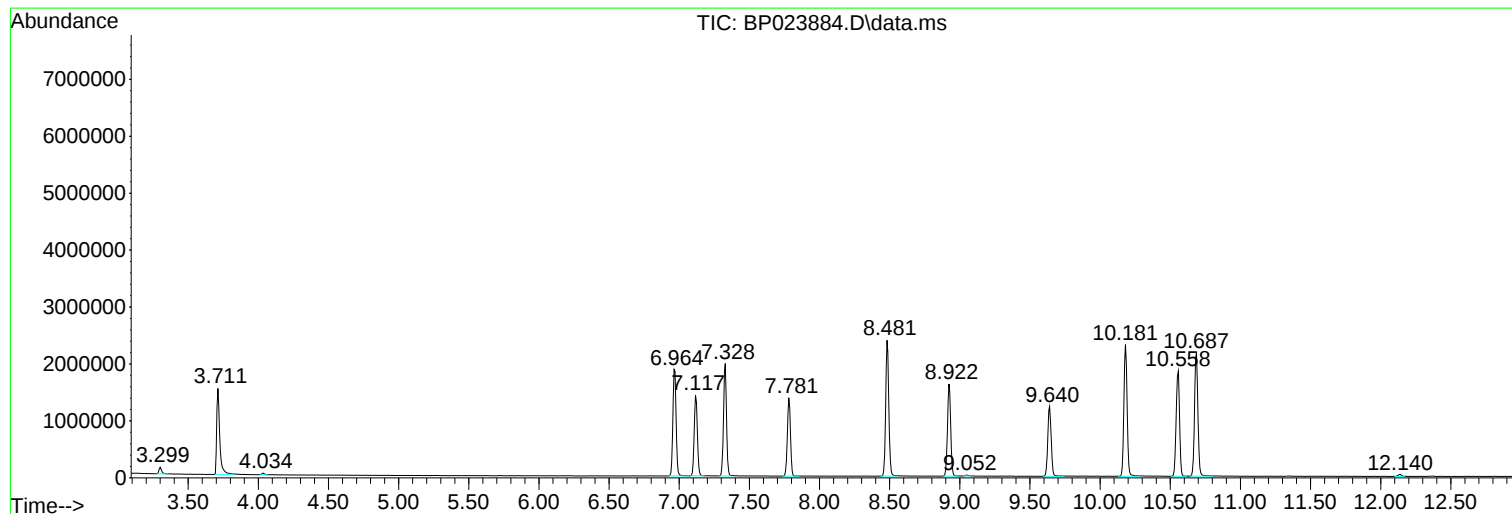

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020325\
Data File : BP023884.D
Acq On : 03 Feb 2025 17:55
Operator : RC/JU
Sample : PB166466BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK466

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020325\
Data File : BP023884.D
Acq On : 03 Feb 2025 17:55
Operator : RC/JU
Sample : PB166466BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK466

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc