

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020325\
 Data File : BP023885.D
 Acq On : 03 Feb 2025 18:35
 Operator : RC/JU
 Sample : PB166441BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK441

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP023885.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.293	32	35	42	rVB	116582	150693	1.24%	0.119%
2	3.705	101	105	134	rBV	1617260	2632180	21.68%	2.075%
3	4.028	156	160	165	rBV	27842	37435	0.31%	0.030%
4	6.963	651	659	669	rBV	2146498	3496801	28.80%	2.756%
5	7.111	678	684	698	rBV	1609786	2599829	21.41%	2.049%
6	7.322	712	720	738	rBV	2174791	3503665	28.86%	2.761%
7	7.775	790	797	808	rBV	1616908	2614944	21.54%	2.061%
8	8.481	910	917	933	rBV	2631281	4441003	36.58%	3.500%
9	8.916	984	991	1005	rBV	1893700	3083424	25.40%	2.430%
10	9.046	1009	1013	1020	rBV3	20400	34536	0.28%	0.027%
11	9.634	1106	1113	1130	rBV	1529535	2437631	20.08%	1.921%
12	10.175	1198	1205	1228	rBV	2625092	4378727	36.07%	3.451%
13	10.552	1261	1269	1277	rBV	2444745	3915681	32.25%	3.086%
14	10.681	1283	1291	1307	rBV	2685687	4371312	36.01%	3.445%
15	11.346	1398	1404	1407	rBV8	6952	13289	0.11%	0.010%
16	12.134	1532	1538	1545	rVB	42655	70133	0.58%	0.055%
17	13.363	1742	1747	1754	rVB6	8818	17866	0.15%	0.014%
18	13.804	1814	1822	1837	rBV	4555008	6271400	51.66%	4.943%
19	14.087	1863	1870	1887	rBV	5674221	7815563	64.37%	6.160%
20	14.398	1916	1923	1933	rBV	3757259	5490489	45.22%	4.327%
21	14.610	1950	1959	1977	rBV	1846886	2937590	24.20%	2.315%
22	14.816	1990	1994	1997	rVB5	11932	17902	0.15%	0.014%
23	15.404	2087	2094	2103	rBV	7027164	9727279	80.12%	7.666%
24	15.516	2106	2113	2128	rVV	1619710	2157985	17.77%	1.701%
25	15.651	2131	2136	2142	rVB	31103	51421	0.42%	0.041%
26	15.981	2187	2192	2197	rBV6	6979	13269	0.11%	0.010%
27	16.969	2356	2360	2365	rBV	18193	26281	0.22%	0.021%
28	17.186	2391	2397	2407	rBV2	4987263	6547295	53.93%	5.160%
29	17.292	2408	2415	2433	rVV	8087969	10862517	89.47%	8.561%
30	17.886	2514	2516	2521	rVB5	11951	13020	0.11%	0.010%
31	18.122	2553	2556	2563	rVB8	12484	18435	0.15%	0.015%
32	19.204	2736	2740	2746	rBV	78545	116511	0.96%	0.092%
33	19.275	2749	2752	2758	rVB	75278	104441	0.86%	0.082%
34	19.651	2811	2816	2827	rBV2	8621701	12140730	100.00%	9.569%
35	21.627	3146	3152	3163	rVB	4063536	6662895	54.88%	5.251%
36	24.768	3676	3686	3706	rVB	4335525	11345597	93.45%	8.942%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020325\
Data File : BP023885.D
Acq On : 03 Feb 2025 18:35
Operator : RC/JU
Sample : PB166441BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK441

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Title : SVOA CALIBRATION

37	24.998	3716	3725	3741	rVB	2349073	6760586	55.69%	5.328%
----	--------	------	------	------	-----	---------	---------	--------	--------




Sum of corrected areas: 126880355

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020325\
Data File : BP023885.D
Acq On : 03 Feb 2025 18:35
Operator : RC/JU
Sample : PB166441BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK441

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

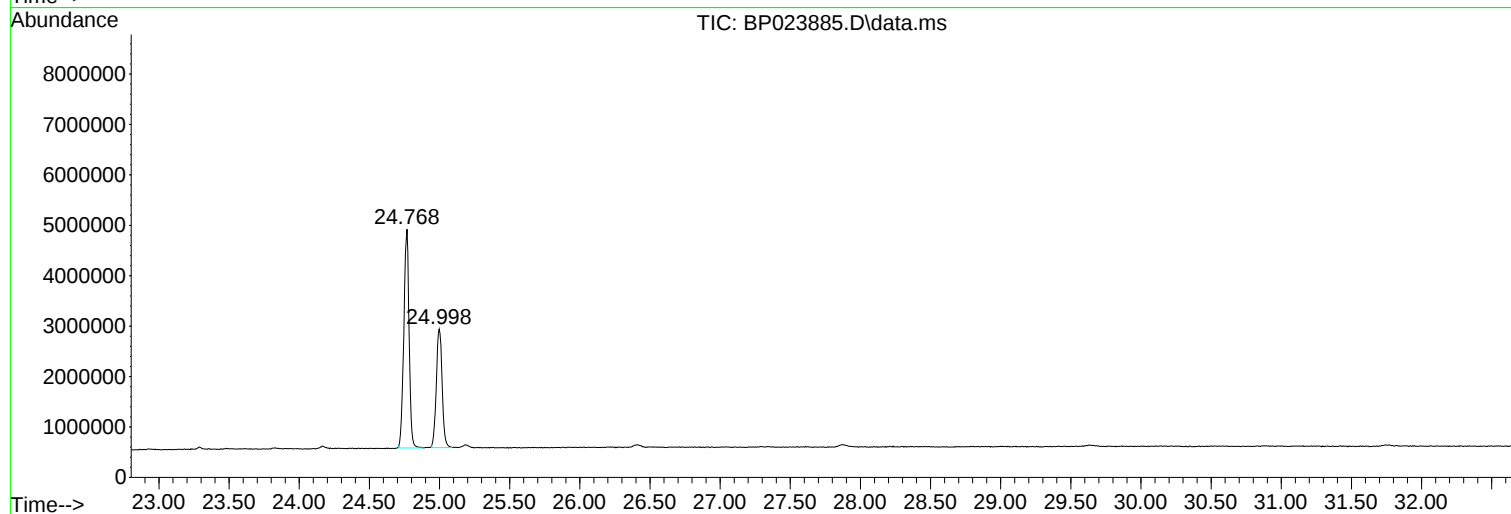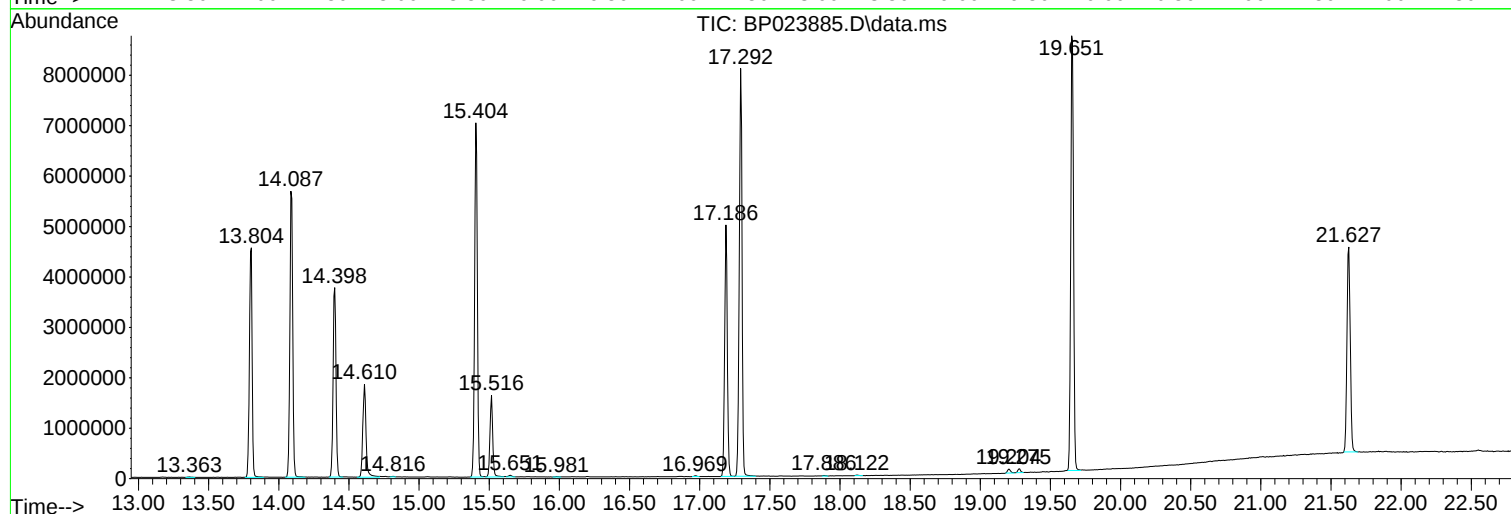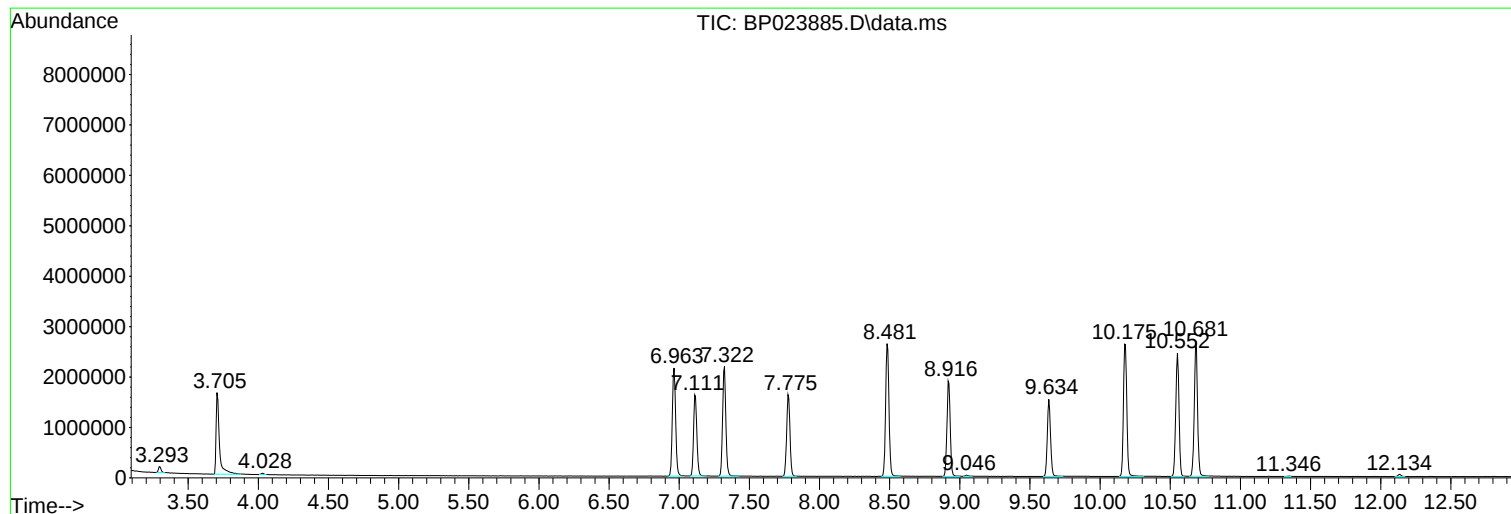

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020325\
Data File : BP023885.D
Acq On : 03 Feb 2025 18:35
Operator : RC/JU
Sample : PB166441BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK441

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020325\
Data File : BP023885.D
Acq On : 03 Feb 2025 18:35
Operator : RC/JU
Sample : PB166441BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK441

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc