

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020325\
 Data File : BP023900.D
 Acq On : 04 Feb 2025 05:25
 Operator : RC/JU
 Sample : PB166438BL
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK438

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP023900.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.293	30	35	45	rVB	125530	177018	1.41%	0.139%
2	3.699	100	104	126	rBV	1695973	2602793	20.71%	2.044%
3	4.022	155	159	167	rVB	34989	53098	0.42%	0.042%
4	6.957	650	658	670	rBV	2188605	3372696	26.84%	2.648%
5	7.104	677	683	696	rVB	1640493	2507761	19.96%	1.969%
6	7.316	712	719	730	rBV	2257568	3412059	27.15%	2.679%
7	7.769	789	796	806	rBV	1566136	2542739	20.23%	1.997%
8	8.475	908	916	933	rBV	2588108	4267008	33.95%	3.351%
9	8.916	983	991	1006	rBV	1811098	2995991	23.84%	2.353%
10	9.045	1008	1013	1017	rBV	19419	29147	0.23%	0.023%
11	9.634	1105	1113	1128	rBV	1486490	2399368	19.09%	1.884%
12	10.175	1197	1205	1218	rBV	2660583	4209318	33.50%	3.305%
13	10.551	1261	1269	1278	rBV	2446574	3777760	30.06%	2.967%
14	10.687	1284	1292	1305	rBV	2618266	4237418	33.72%	3.328%
15	11.351	1399	1405	1412	rBV8	7730	14073	0.11%	0.011%
16	12.139	1532	1539	1546	rBV2	39820	67038	0.53%	0.053%
17	13.357	1740	1746	1757	rVB6	8863	23000	0.18%	0.018%
18	13.804	1815	1822	1831	rBV	4622483	5984505	47.62%	4.699%
19	14.086	1863	1870	1884	rBV	5393050	7574488	60.27%	5.948%
20	14.398	1915	1923	1933	rBV	3542958	5242646	41.72%	4.117%
21	14.604	1952	1958	1980	rBV	1767238	3007988	23.94%	2.362%
22	14.816	1989	1994	2000	rVB9	10317	18897	0.15%	0.015%
23	15.404	2087	2094	2103	rBV	7280738	9446275	75.17%	7.418%
24	15.522	2107	2114	2130	rVV	1585774	2226190	17.71%	1.748%
25	15.645	2130	2135	2141	rVB2	27870	48131	0.38%	0.038%
26	16.969	2355	2360	2367	rVB	17542	30168	0.24%	0.024%
27	17.186	2390	2397	2407	rBV	4455676	6488589	51.63%	5.095%
28	17.292	2407	2415	2428	rBV	7367241	10568003	84.09%	8.299%
29	17.880	2513	2515	2521	rVB6	10006	15286	0.12%	0.012%
30	18.121	2552	2556	2560	rBV7	10199	18330	0.15%	0.014%
31	19.210	2737	2741	2747	rVB2	68947	102745	0.82%	0.081%
32	19.286	2750	2754	2758	rVB	67466	93362	0.74%	0.073%
33	19.663	2812	2818	2827	rBV	9380758	12566836	100.00%	9.868%
34	21.633	3148	3153	3162	rBV	5098023	7140108	56.82%	5.607%
35	24.774	3678	3687	3703	rVB	4737990	12551437	99.88%	9.856%
36	25.009	3718	3727	3750	rVB	2866731	7531996	59.94%	5.915%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020325\
Data File : BP023900.D
Acq On : 04 Feb 2025 05:25
Operator : RC/JU
Sample : PB166438BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK438

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 127344265

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020325\
Data File : BP023900.D
Acq On : 04 Feb 2025 05:25
Operator : RC/JU
Sample : PB166438BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK438

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

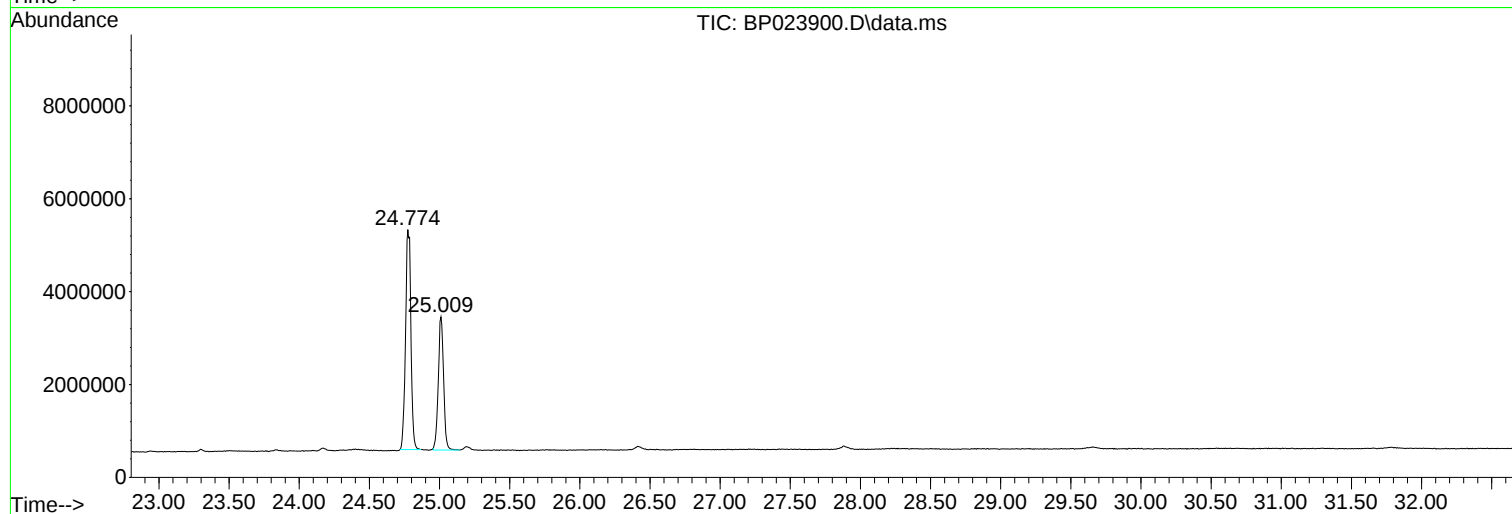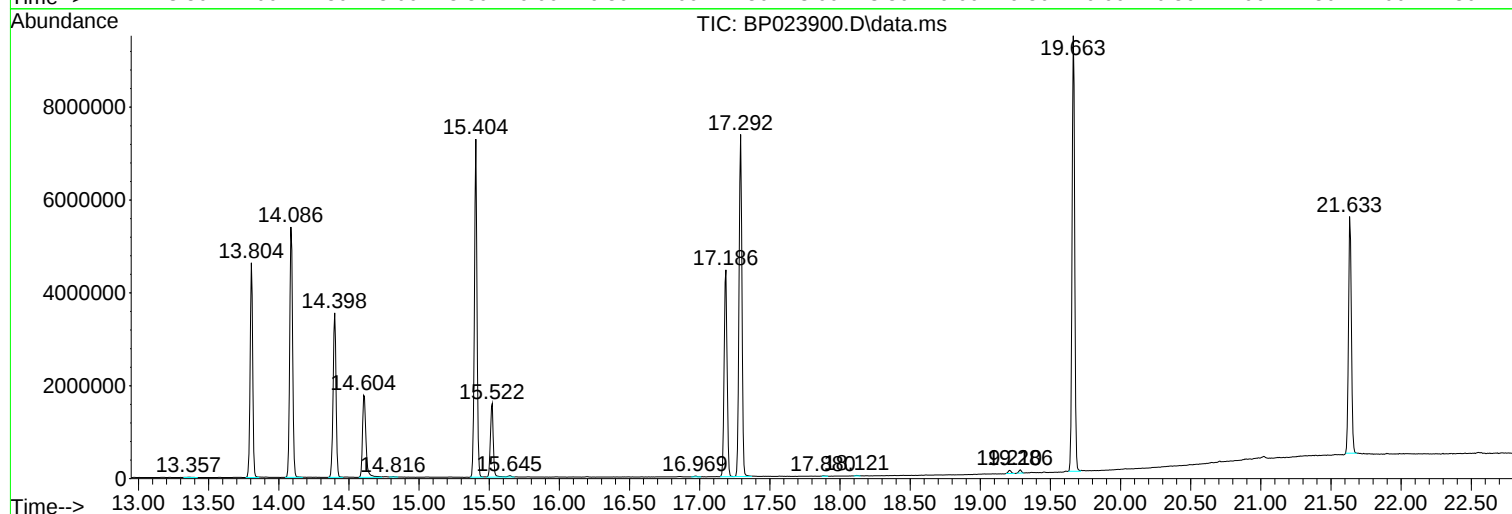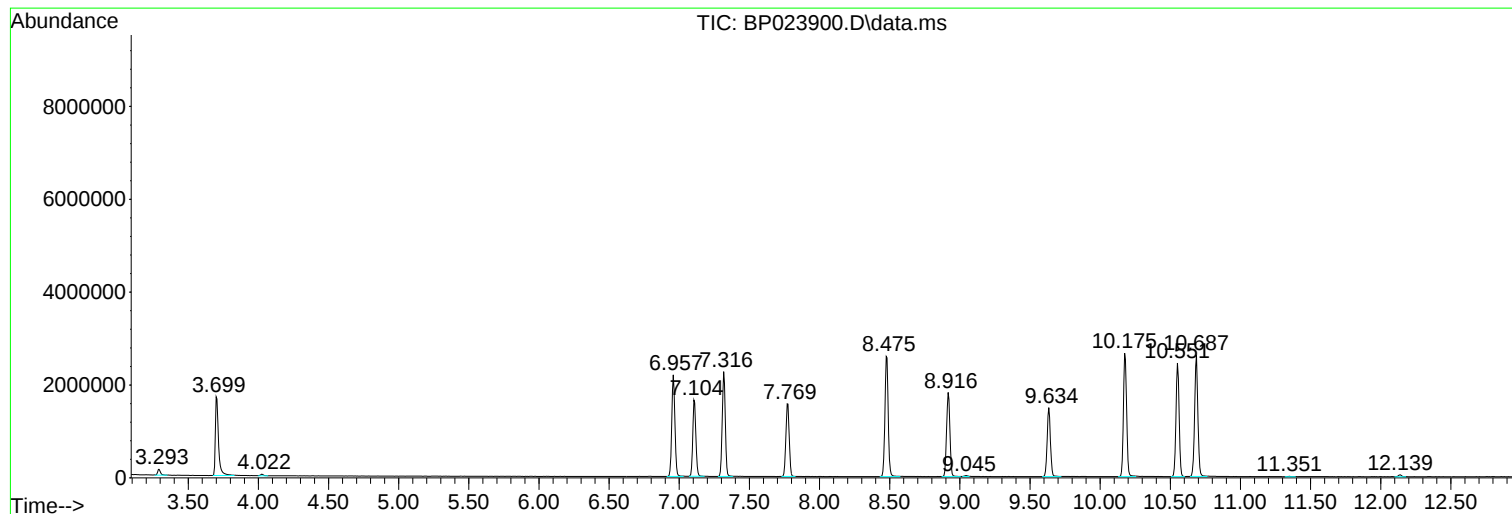

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020325\
Data File : BP023900.D
Acq On : 04 Feb 2025 05:25
Operator : RC/JU
Sample : PB166438BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK438

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020325\
Data File : BP023900.D
Acq On : 04 Feb 2025 05:25
Operator : RC/JU
Sample : PB166438BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK438

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc