

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020325\
 Data File : BP023901.D
 Acq On : 04 Feb 2025 06:05
 Operator : RC/JU
 Sample : PB166444BL
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK444

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP023901.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.293	31	35	45	rVB	149163	197057	1.50%	0.144%
2	3.705	101	105	129	rBV	1943589	2912092	22.23%	2.134%
3	4.028	156	160	168	rVB	34052	53595	0.41%	0.039%
4	6.958	650	658	674	rBV	2588706	3801728	29.02%	2.786%
5	7.111	677	684	696	rVB	1838680	2773007	21.17%	2.032%
6	7.316	712	719	733	rBV	2647691	3807318	29.06%	2.791%
7	7.775	790	797	808	rBV	1823941	2796969	21.35%	2.050%
8	8.481	905	917	930	rBV	3146553	4821527	36.80%	3.534%
9	8.916	981	991	1004	rBV	2035448	3348753	25.56%	2.454%
10	9.052	1009	1014	1018	rVV2	20112	32223	0.25%	0.024%
11	9.640	1105	1114	1123	rBV	1604413	2652942	20.25%	1.944%
12	10.175	1198	1205	1221	rBV	2950400	4701019	35.88%	3.446%
13	10.552	1261	1269	1277	rBV	2589079	4172271	31.85%	3.058%
14	10.681	1284	1291	1309	rBV	2763977	4726258	36.07%	3.464%
15	11.346	1399	1404	1408	rBV7	8288	15292	0.12%	0.011%
16	12.134	1531	1538	1545	rBV	44803	81834	0.62%	0.060%
17	13.363	1739	1747	1754	rVB6	9799	22932	0.18%	0.017%
18	13.798	1815	1821	1838	rBV	4887349	6490895	49.54%	4.757%
19	14.087	1863	1870	1882	rBV	6143894	8278079	63.19%	6.067%
20	14.398	1916	1923	1933	rBV	4188370	5796995	44.25%	4.249%
21	14.610	1952	1959	1981	rBV	1986426	3234847	24.69%	2.371%
22	14.816	1991	1994	2004	rVB8	11386	18936	0.14%	0.014%
23	15.398	2085	2093	2106	rBV	6988788	10300416	78.62%	7.550%
24	15.510	2106	2112	2125	rBV	1653433	2285228	17.44%	1.675%
25	15.640	2130	2134	2143	rVB2	31990	55985	0.43%	0.041%
26	15.981	2187	2192	2196	rBV5	6593	13428	0.10%	0.010%
27	16.969	2354	2360	2365	rVB	18109	30218	0.23%	0.022%
28	17.187	2389	2397	2407	rBV2	4583126	6784491	51.79%	4.973%
29	17.287	2408	2414	2429	rVV	8509506	11380809	86.87%	8.341%
30	17.881	2512	2515	2520	rVB7	13685	20260	0.15%	0.015%
31	18.122	2552	2556	2561	rBV8	15119	23742	0.18%	0.017%
32	19.198	2735	2739	2744	rBV3	77603	114924	0.88%	0.084%
33	19.269	2747	2751	2758	rBV	72919	112571	0.86%	0.083%
34	19.651	2810	2816	2827	rBV	10338319	13101254	100.00%	9.602%
35	21.627	3145	3152	3163	rBV	4586957	7361306	56.19%	5.395%
36	24.768	3676	3686	3702	rVB	4796419	12638375	96.47%	9.263%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020325\
Data File : BP023901.D
Acq On : 04 Feb 2025 06:05
Operator : RC/JU
Sample : PB166444BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK444

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Title : SVOA CALIBRATION

37 24.992 3716 3724 3740 rVB 2895323 7477958 57.08% 5.481%




Sum of corrected areas: 136437534

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020325\
Data File : BP023901.D
Acq On : 04 Feb 2025 06:05
Operator : RC/JU
Sample : PB166444BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK444

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

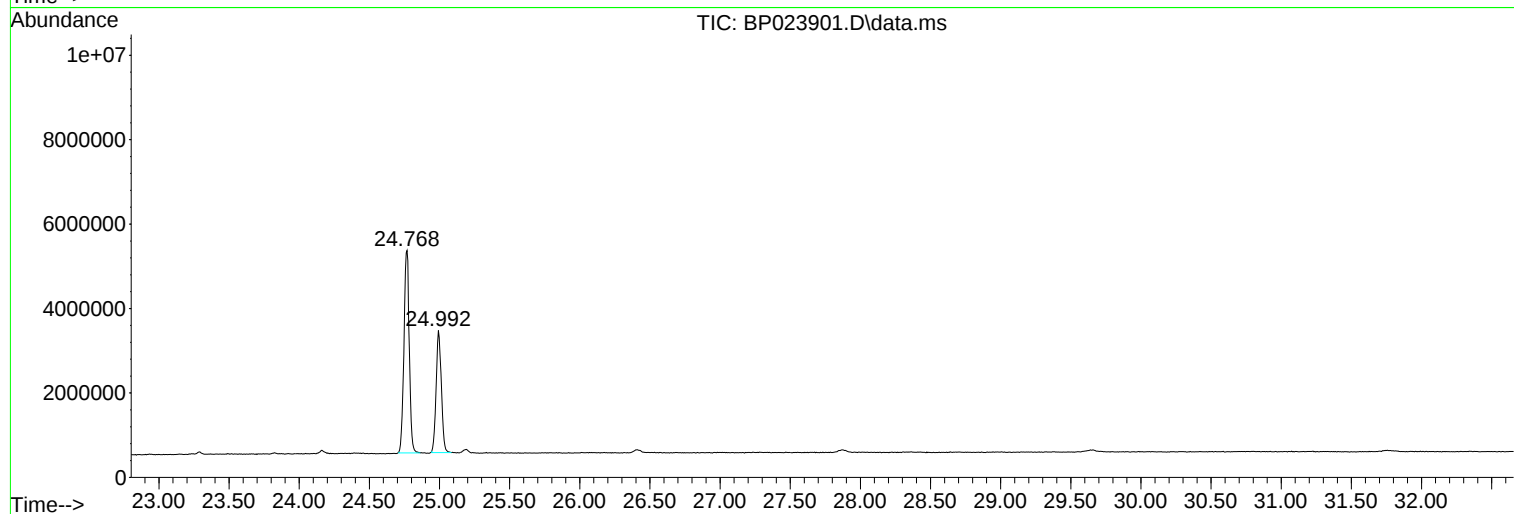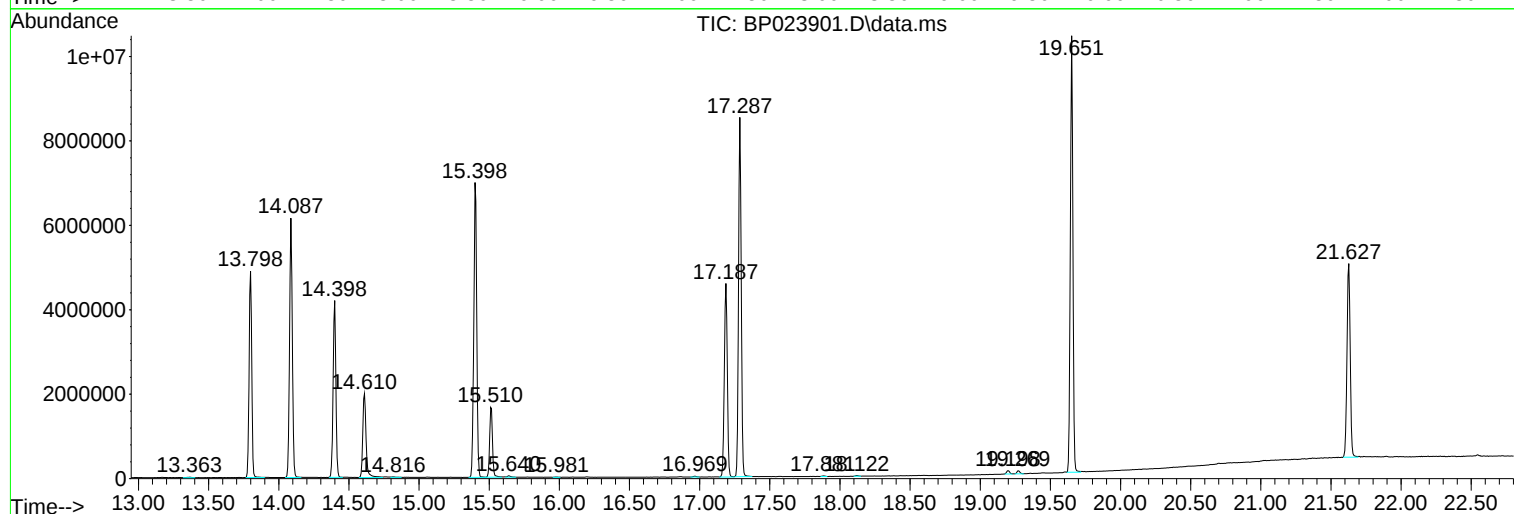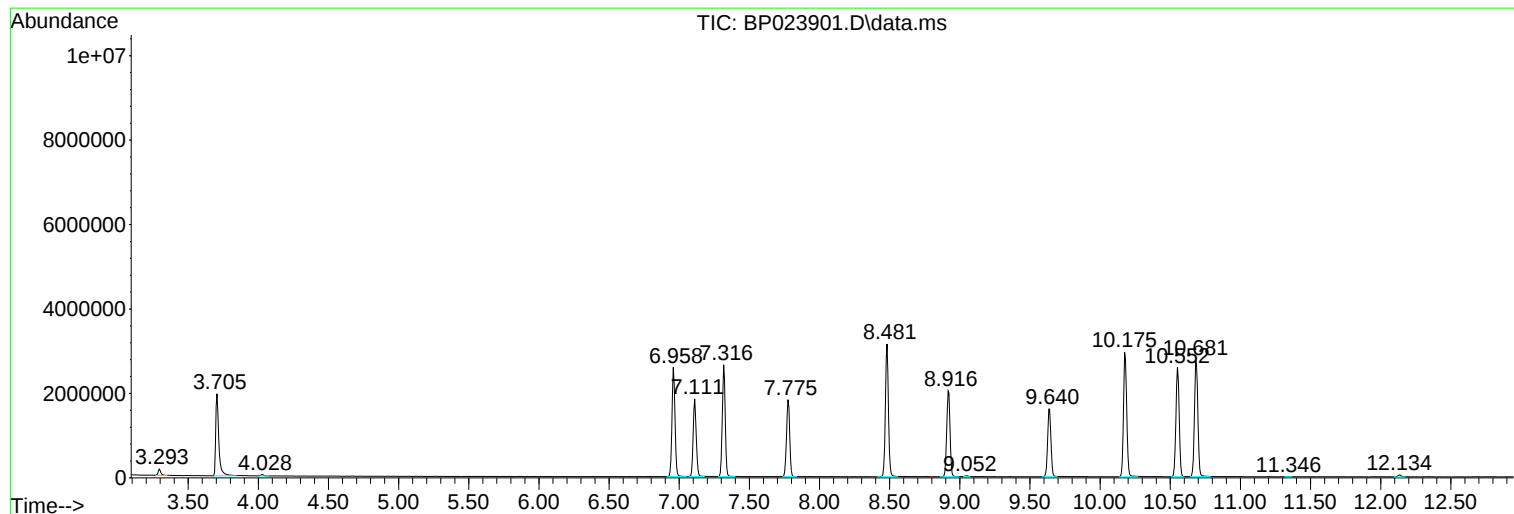

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020325\
Data File : BP023901.D
Acq On : 04 Feb 2025 06:05
Operator : RC/JU
Sample : PB166444BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK444

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020325\
Data File : BP023901.D
Acq On : 04 Feb 2025 06:05
Operator : RC/JU
Sample : PB166444BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK444

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc