

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP023907\
 Data File : BP023907.D
 Acq On : 04 Feb 2025 10:09
 Operator : RC/JU
 Sample : Q1202-04
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E2978

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP023907.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.299	32	36	46	rVB	130141	183087	1.17%	0.131%
2	3.711	102	106	127	rVB	635975	1018837	6.52%	0.727%
3	4.028	156	160	168	rVB	48767	68217	0.44%	0.049%
4	4.123	172	176	181	rVB2	35696	49550	0.32%	0.035%
5	4.470	232	235	239	rVB	11597	15677	0.10%	0.011%
6	4.934	310	314	321	rVB3	30864	50861	0.33%	0.036%
7	6.181	522	526	533	rBV	34671	46882	0.30%	0.033%
8	6.958	649	658	668	rBV	793576	1250428	8.00%	0.892%
9	7.111	675	684	694	rBV	1868177	2843967	18.19%	2.028%
10	7.316	712	719	731	rBV	2302066	3450668	22.07%	2.461%
11	7.411	732	735	741	rVB6	10869	16493	0.11%	0.012%
12	7.775	789	797	805	rBV	1872025	2906864	18.59%	2.073%
13	8.481	908	917	928	rBV	2105301	3420560	21.87%	2.439%
14	8.922	983	992	1001	rBV	2151687	3472303	22.20%	2.476%
15	9.352	1062	1065	1070	rVB	15348	21613	0.14%	0.015%
16	9.640	1106	1114	1121	rBV	1787553	2904738	18.58%	2.072%
17	10.181	1197	1206	1217	rBV	2991107	4945664	31.63%	3.527%
18	10.552	1261	1269	1282	rVB	2784203	4368512	27.94%	3.115%
19	10.681	1283	1291	1307	rBV	2694372	4486617	28.69%	3.200%
20	11.346	1396	1404	1410	rBV6	10713	24499	0.16%	0.017%
21	12.075	1523	1528	1533	rBV	15109	23923	0.15%	0.017%
22	12.134	1533	1538	1546	rVB	41048	76043	0.49%	0.054%
23	13.804	1815	1822	1834	rBV	5155494	7409379	47.38%	5.284%
24	14.087	1861	1870	1884	rBV	5688892	8841803	56.54%	6.306%
25	14.398	1914	1923	1933	rBV	3853858	5894924	37.70%	4.204%
26	14.481	1933	1937	1943	rVB9	7491	17345	0.11%	0.012%
27	14.610	1953	1959	1975	rBV	828233	1214572	7.77%	0.866%
28	14.757	1979	1984	1988	rVV8	12202	23686	0.15%	0.017%
29	14.822	1991	1995	2000	rVB8	10293	16792	0.11%	0.012%
30	14.951	2012	2017	2022	rBV2	13135	21939	0.14%	0.016%
31	15.228	2059	2064	2069	rVB2	11876	19020	0.12%	0.014%
32	15.404	2087	2094	2102	rBV	8247844	11558632	73.92%	8.243%
33	15.516	2107	2113	2130	rVV	2366438	3056059	19.54%	2.179%
34	15.645	2131	2135	2141	rVB	33906	55683	0.36%	0.040%
35	15.769	2151	2156	2161	rBV	126988	172664	1.10%	0.123%
36	16.969	2358	2360	2364	rVB	20247	21946	0.14%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020325\
Data File : BP023907.D
Acq On : 04 Feb 2025 10:09
Operator : RC/JU
Sample : Q1202-04
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E2978

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Title : SVOA CALIBRATION

37	17.187	2390	2397	2408	rBV2	4251692	6709923	42.91%	4.785%
38	17.292	2408	2415	2427	rBV	9828367	13097327	83.76%	9.341%
39	18.122	2552	2556	2564	rBV	54403	97116	0.62%	0.069%
40	19.210	2737	2741	2745	rBV	108117	135628	0.87%	0.097%
41	19.275	2749	2752	2758	rBV	110777	154034	0.99%	0.110%
42	19.663	2812	2818	2826	rBV2	10281087	15359212	98.22%	10.954%
43	21.627	3146	3152	3160	rBV2	4622966	7230682	46.24%	5.157%
44	24.774	3677	3687	3703	rBV	6620029	15637500	100.00%	11.152%
45	25.004	3718	3726	3743	rVB	2954309	7827996	50.06%	5.583%




Sum of corrected areas: 140219865

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020325\
Data File : BP023907.D
Acq On : 04 Feb 2025 10:09
Operator : RC/JU
Sample : Q1202-04
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E2978

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

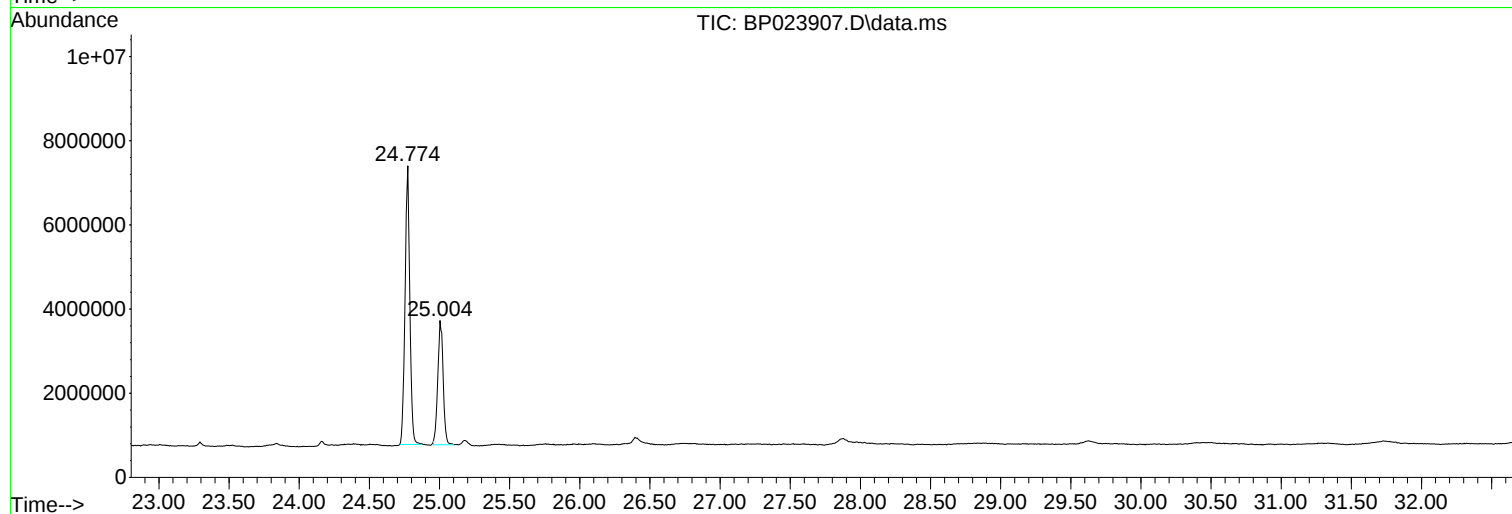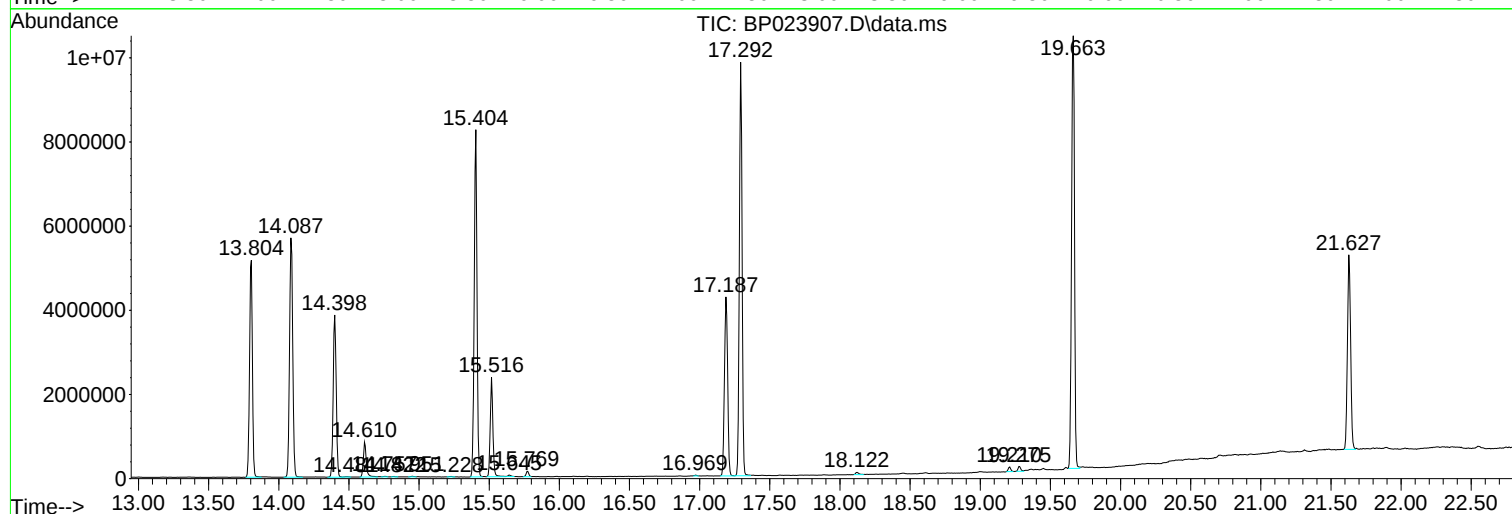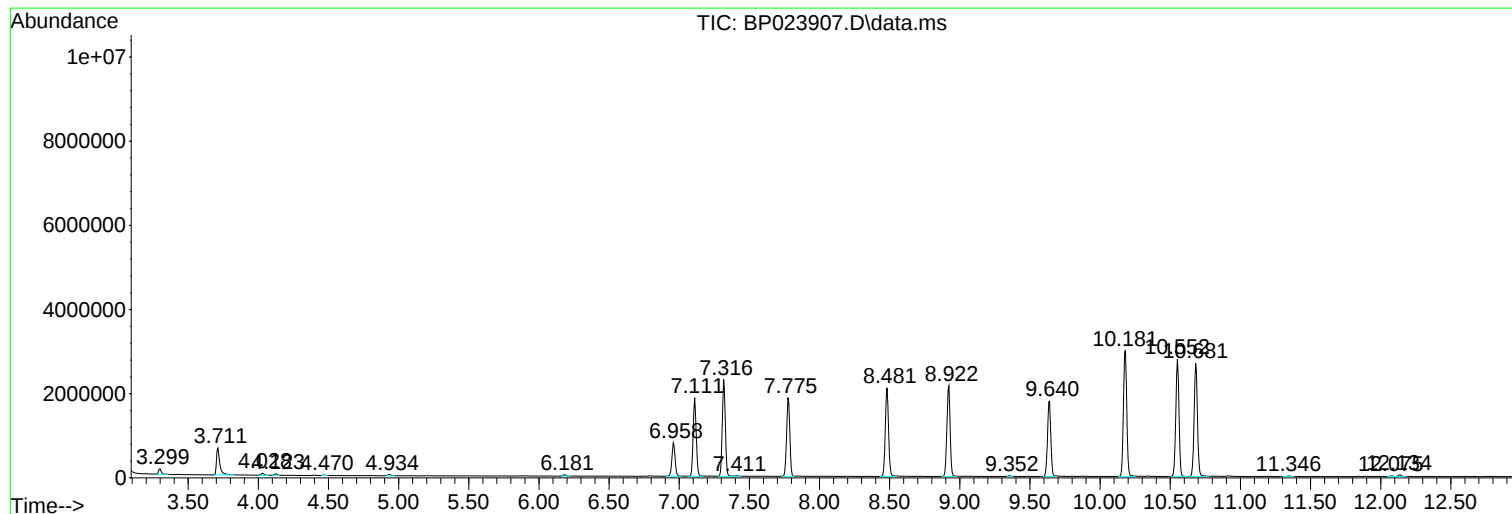

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020325\
Data File : BP023907.D
Acq On : 04 Feb 2025 10:09
Operator : RC/JU
Sample : Q1202-04
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E2978

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020325\
Data File : BP023907.D
Acq On : 04 Feb 2025 10:09
Operator : RC/JU
Sample : Q1202-04
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E2978

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc