

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020325\
 Data File : BP023908.D
 Acq On : 04 Feb 2025 10:49
 Operator : RC/JU
 Sample : Q1202-05
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E2979

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP023908.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.293	31	35	45	rVB	126643	171754	1.07%	0.118%
2	3.705	101	105	126	rBV	619360	1003381	6.25%	0.691%
3	4.028	156	160	169	rVB	49369	68171	0.42%	0.047%
4	4.123	172	176	180	rBV	32917	44782	0.28%	0.031%
5	4.470	231	235	238	rBV	14435	20305	0.13%	0.014%
6	4.934	309	314	321	rVB3	29971	55575	0.35%	0.038%
7	6.181	521	526	532	rVB	31128	45418	0.28%	0.031%
8	6.958	650	658	668	rBV	736583	1153508	7.19%	0.795%
9	7.111	677	684	696	rBV	2047106	2960674	18.44%	2.039%
10	7.316	712	719	730	rBV	2302985	3486113	21.72%	2.401%
11	7.405	731	734	742	rVB7	9753	16076	0.10%	0.011%
12	7.775	790	797	805	rBV	1864785	2865314	17.85%	1.974%
13	8.481	907	917	927	rBV	1978418	3320997	20.69%	2.287%
14	8.916	983	991	1004	rBV	2262258	3650497	22.74%	2.514%
15	9.052	1009	1014	1022	rVB2	30669	53905	0.34%	0.037%
16	9.358	1060	1066	1076	rVB3	17928	34963	0.22%	0.024%
17	9.487	1081	1088	1091	rBV8	8070	16649	0.10%	0.011%
18	9.634	1104	1113	1121	rBV	1760123	3045584	18.97%	2.098%
19	10.175	1196	1205	1220	rBV	2830449	5022430	31.29%	3.459%
20	10.552	1261	1269	1282	rVB	2740438	4373669	27.25%	3.013%
21	10.681	1282	1291	1307	rBV	2785336	4668792	29.08%	3.216%
22	10.916	1326	1331	1336	rBV4	14041	30108	0.19%	0.021%
23	11.340	1398	1403	1408	rBV6	10853	21061	0.13%	0.015%
24	11.893	1491	1497	1503	rBV	99599	148689	0.93%	0.102%
25	12.081	1524	1529	1532	rBV	13913	20687	0.13%	0.014%
26	12.134	1533	1538	1544	rVB	47985	71940	0.45%	0.050%
27	13.234	1720	1725	1733	rVB	40511	57517	0.36%	0.040%
28	13.798	1814	1821	1836	rBV	5573560	7697755	47.95%	5.302%
29	14.087	1860	1870	1879	rBV	6294503	9205898	57.35%	6.341%
30	14.398	1915	1923	1932	rBV	4405955	6058062	37.74%	4.173%
31	14.475	1932	1936	1944	rVB9	12625	24052	0.15%	0.017%
32	14.616	1952	1960	1979	rBV	764493	1177612	7.34%	0.811%
33	14.751	1979	1983	1988	rVV8	15746	32302	0.20%	0.022%
34	14.810	1988	1993	1999	rVB10	11905	22358	0.14%	0.015%
35	14.957	2013	2018	2024	rBV3	22511	40551	0.25%	0.028%
36	15.222	2058	2063	2069	rVB3	11356	21119	0.13%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020325\
Data File : BP023908.D
Acq On : 04 Feb 2025 10:49
Operator : RC/JU
Sample : Q1202-05
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E2979

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Title : SVOA CALIBRATION

37	15.404	2087	2094	2105	rBV	8382600	12043111	75.02%	8.295%
38	15.522	2107	2114	2127	rVV	2223232	3205730	19.97%	2.208%
39	15.651	2131	2136	2142	rVB2	39918	70790	0.44%	0.049%
40	15.775	2151	2157	2163	rBV	228946	348290	2.17%	0.240%
41	16.351	2249	2255	2264	rVB	94002	139355	0.87%	0.096%
42	16.863	2339	2342	2347	rVB5	11406	16635	0.10%	0.011%
43	16.969	2356	2360	2365	rVB2	18862	31298	0.19%	0.022%
44	17.192	2392	2398	2409	rBV2	5100465	6840209	42.61%	4.712%
45	17.298	2409	2416	2429	rVV	9629464	13858102	86.33%	9.545%
46	17.892	2515	2517	2522	rVB6	14892	16946	0.11%	0.012%
47	18.128	2553	2557	2567	rBV2	113056	184006	1.15%	0.127%
48	18.457	2609	2613	2618	rVB4	32598	57182	0.36%	0.039%
49	19.010	2703	2707	2711	rVB3	39084	60207	0.38%	0.041%
50	19.216	2737	2742	2748	rBV	117849	155521	0.97%	0.107%
51	19.286	2750	2754	2759	rBV	107133	142049	0.88%	0.098%
52	19.457	2779	2783	2790	rBV5	54564	106486	0.66%	0.073%
53	19.669	2812	2819	2828	rBV	12002902	15898407	99.04%	10.951%
54	21.633	3147	3153	3166	rVB	4738645	7382559	45.99%	5.085%
55	24.780	3678	3688	3700	rVB	5631119	16052805	100.00%	11.057%
56	25.016	3718	3728	3743	rVB	2982368	7862480	48.98%	5.416%




Sum of corrected areas: 145180436

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020325\
Data File : BP023908.D
Acq On : 04 Feb 2025 10:49
Operator : RC/JU
Sample : Q1202-05
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E2979

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

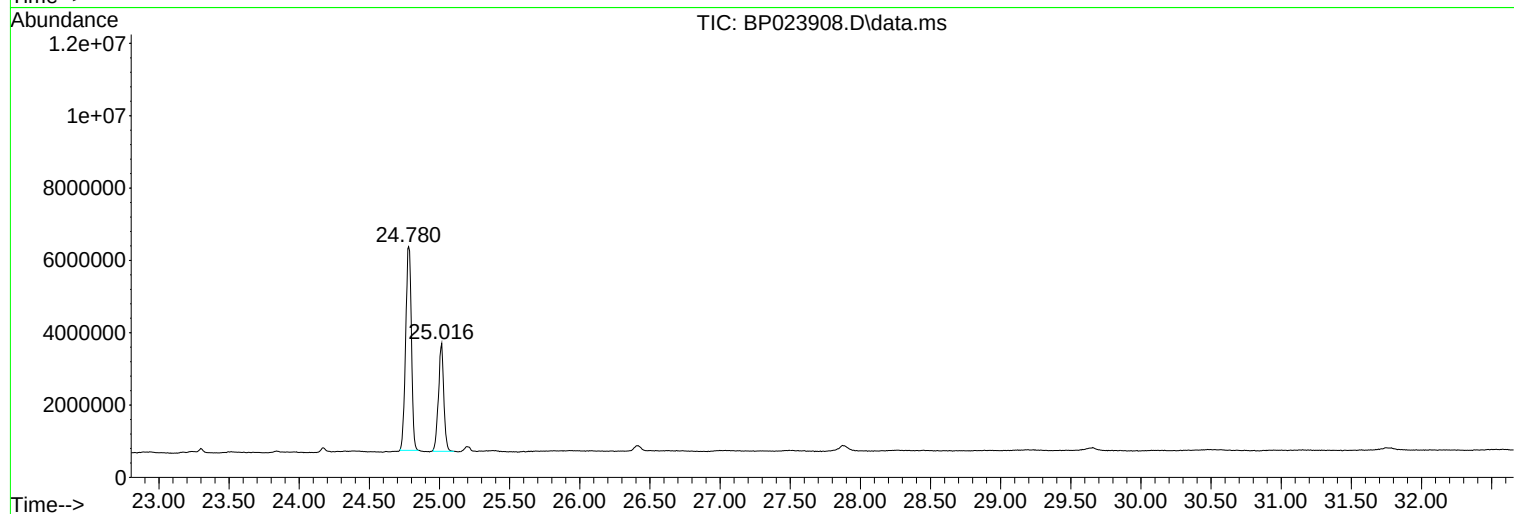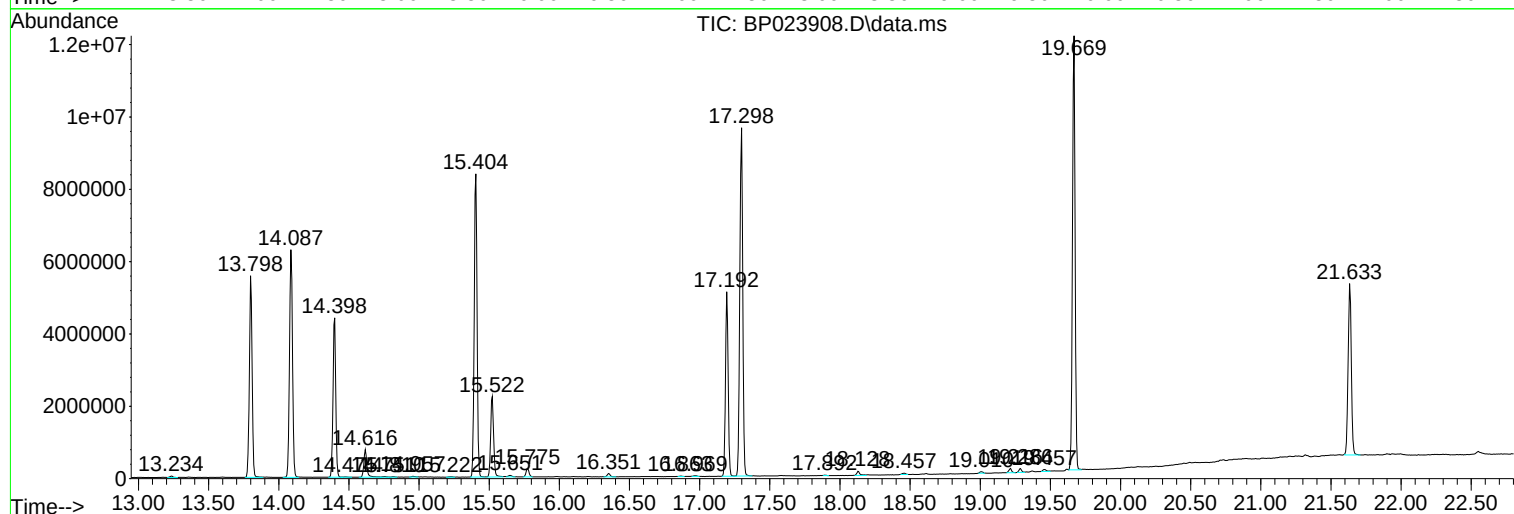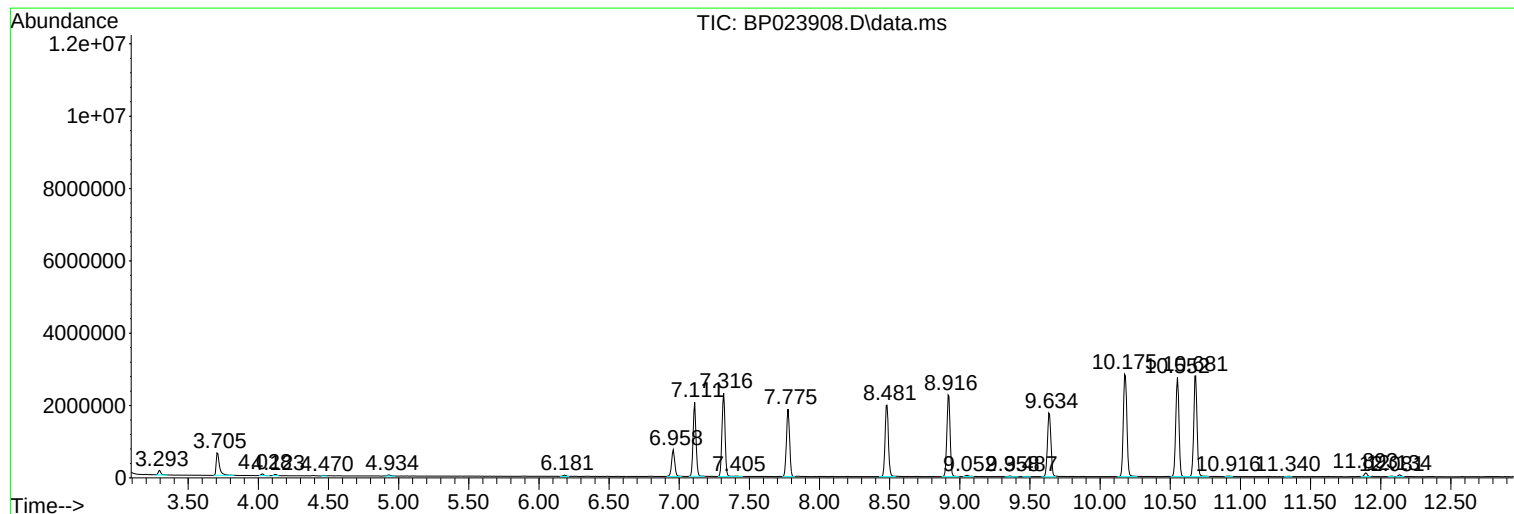

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020325\
Data File : BP023908.D
Acq On : 04 Feb 2025 10:49
Operator : RC/JU
Sample : Q1202-05
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E2979

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020325\
Data File : BP023908.D
Acq On : 04 Feb 2025 10:49
Operator : RC/JU
Sample : Q1202-05
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E2979

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
