

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020325\
 Data File : BP023914.D
 Acq On : 04 Feb 2025 15:59
 Operator : RC/JU
 Sample : PB166453BL
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK453

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP023914.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.287	30	34	46	rVB	130227	179794	1.51%	0.140%
2	3.699	100	104	118	rBV	1820015	2673799	22.47%	2.085%
3	4.022	155	159	166	rVB	36389	50987	0.43%	0.040%
4	6.952	650	657	668	rBV	2328596	3596979	30.23%	2.805%
5	7.105	676	683	695	rVB	1751264	2632728	22.13%	2.053%
6	7.310	710	718	732	rBV	2365959	3652271	30.69%	2.849%
7	7.763	788	795	805	rBV	1694523	2671817	22.45%	2.084%
8	8.475	908	916	930	rBV	2774142	4553522	38.27%	3.551%
9	8.910	982	990	1003	rBV	1935508	3201568	26.91%	2.497%
10	9.040	1007	1012	1022	rVB2	20360	39277	0.33%	0.031%
11	9.628	1105	1112	1125	rBV	1659406	2613203	21.96%	2.038%
12	10.175	1197	1205	1223	rBV	2747507	4532969	38.10%	3.535%
13	10.546	1259	1268	1278	rBV	2479089	4025909	33.84%	3.140%
14	10.675	1281	1290	1310	rBV	2650087	4504994	37.86%	3.514%
15	12.122	1528	1536	1543	rBV2	41195	74702	0.63%	0.058%
16	13.351	1743	1745	1752	rVB4	8735	14775	0.12%	0.012%
17	13.792	1813	1820	1830	rBV	4397124	6146723	51.66%	4.794%
18	14.081	1862	1869	1885	rBV	5331212	7854138	66.01%	6.126%
19	14.392	1914	1922	1932	rBV	3730968	5509631	46.30%	4.297%
20	14.475	1933	1936	1942	rVB7	7133	12185	0.10%	0.010%
21	14.604	1952	1958	1979	rBV	1898132	2979425	25.04%	2.324%
22	14.757	1982	1984	1990	rVV7	10039	15599	0.13%	0.012%
23	14.816	1990	1994	1998	rVB7	8200	12280	0.10%	0.010%
24	15.392	2085	2092	2107	rBV	6292561	9645077	81.06%	7.522%
25	15.516	2107	2113	2129	rVV	1766760	2225119	18.70%	1.735%
26	15.639	2129	2134	2140	rVB2	31976	51409	0.43%	0.040%
27	16.869	2337	2343	2348	rBV9	9261	17843	0.15%	0.014%
28	16.975	2356	2361	2367	rBV2	15949	25628	0.22%	0.020%
29	17.198	2392	2399	2409	rBV2	4637311	6439333	54.12%	5.022%
30	17.298	2409	2416	2434	rVB	8997800	10626094	89.31%	8.288%
31	19.210	2737	2741	2746	rBV3	73295	108261	0.91%	0.084%
32	19.280	2749	2753	2759	rVV2	67650	104683	0.88%	0.082%
33	19.663	2811	2818	2824	rBV	8679643	11792290	99.11%	9.197%
34	21.621	3145	3151	3166	rBV2	4204495	6738027	56.63%	5.255%
35	24.757	3674	3684	3700	rVB	4452745	11898618	100.00%	9.280%
36	24.998	3716	3725	3739	rVB	2435472	6995327	58.79%	5.456%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020325\
Data File : BP023914.D
Acq On : 04 Feb 2025 15:59
Operator : RC/JU
Sample : PB166453BL
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK453

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 128216984

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020325\
Data File : BP023914.D
Acq On : 04 Feb 2025 15:59
Operator : RC/JU
Sample : PB166453BL
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK453

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

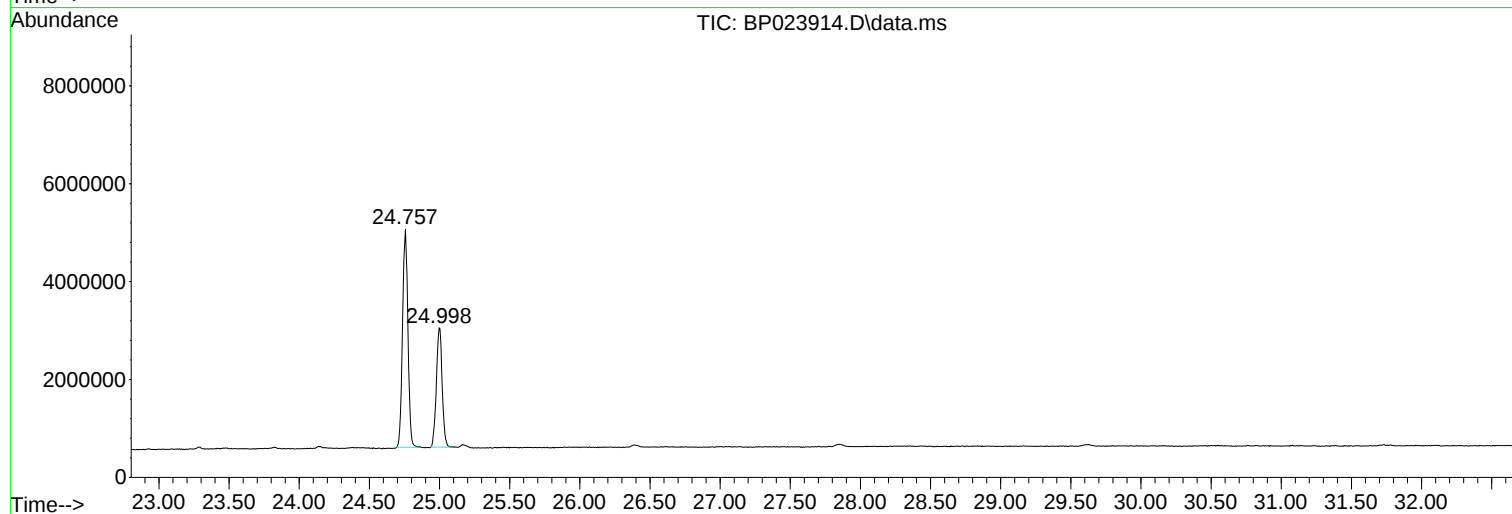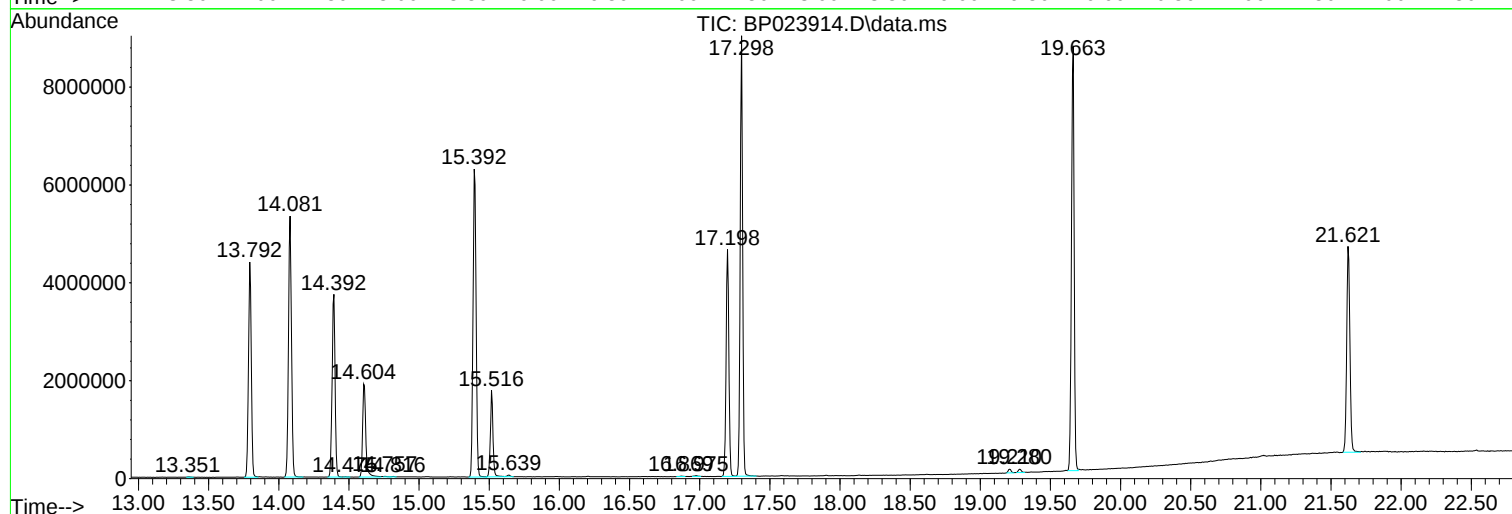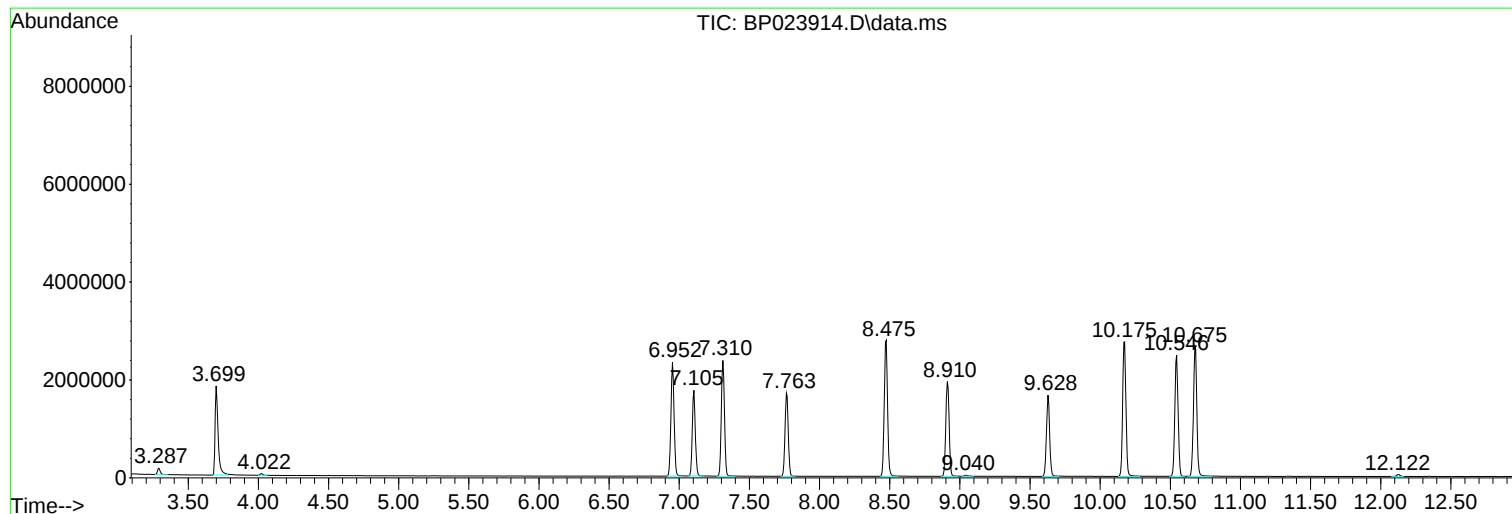

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020325\
Data File : BP023914.D
Acq On : 04 Feb 2025 15:59
Operator : RC/JU
Sample : PB166453BL
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK453

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020325\
Data File : BP023914.D
Acq On : 04 Feb 2025 15:59
Operator : RC/JU
Sample : PB166453BL
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK453

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------