

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020325\
 Data File : BP023915.D
 Acq On : 04 Feb 2025 16:46
 Operator : RC/JU
 Sample : Q1202-09
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E29A0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP023915.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.281	29	33	41	rVB	124977	160971	1.36%	0.150%
2	3.693	99	103	124	rVB	531780	829364	7.03%	0.772%
3	4.011	154	157	163	rVB	21658	28666	0.24%	0.027%
4	4.446	228	231	237	rVB2	11935	16025	0.14%	0.015%
5	4.917	305	311	320	rVB6	14507	29881	0.25%	0.028%
6	6.940	647	655	666	rBV	639629	961363	8.15%	0.895%
7	7.093	674	681	694	rVB	1468695	2125971	18.02%	1.980%
8	7.299	709	716	728	rBV	1630770	2564316	21.74%	2.388%
9	7.387	728	731	741	rVB10	10213	20057	0.17%	0.019%
10	7.758	786	794	803	rBV	1544800	2323941	19.70%	2.164%
11	8.464	907	914	925	rBV	1700863	2621390	22.22%	2.441%
12	8.905	981	989	1001	rBV	1531258	2499904	21.19%	2.328%
13	9.340	1058	1063	1070	rVB3	12459	21030	0.18%	0.020%
14	9.622	1103	1111	1126	rBV	1292324	2041965	17.31%	1.901%
15	10.163	1194	1203	1221	rBV	2091681	3417444	28.97%	3.182%
16	10.534	1259	1266	1275	rVB	2033583	3428447	29.06%	3.192%
17	10.669	1280	1289	1300	rBV	2432665	3968427	33.64%	3.695%
18	11.334	1396	1402	1405	rBV8	7384	12852	0.11%	0.012%
19	12.122	1531	1536	1544	rVB	30780	55465	0.47%	0.052%
20	13.210	1718	1721	1729	rVB10	7059	14135	0.12%	0.013%
21	13.352	1740	1745	1750	rVB8	6757	13417	0.11%	0.012%
22	13.557	1775	1780	1784	rBV3	8224	12557	0.11%	0.012%
23	13.787	1812	1819	1831	rBV	3706126	5121022	43.41%	4.768%
24	14.075	1860	1868	1885	rBV	4206713	6289982	53.32%	5.857%
25	14.387	1914	1921	1931	rBV	3084253	4637618	39.31%	4.318%
26	14.469	1932	1935	1941	rVB8	7792	12627	0.11%	0.012%
27	14.604	1951	1958	1977	rBV	513463	933932	7.92%	0.870%
28	14.746	1978	1982	1989	rVV10	8606	21428	0.18%	0.020%
29	14.816	1989	1994	1998	rVB7	13777	20046	0.17%	0.019%
30	15.398	2084	2093	2105	rBV	5385387	7981843	67.66%	7.432%
31	15.510	2106	2112	2129	rVV	1547792	2127883	18.04%	1.981%
32	15.634	2129	2133	2141	rVB2	24534	46118	0.39%	0.043%
33	15.769	2151	2156	2160	rBV	24485	31352	0.27%	0.029%
34	15.975	2186	2191	2196	rVB9	8629	15164	0.13%	0.014%
35	16.963	2355	2359	2363	rVB2	11772	17185	0.15%	0.016%
36	17.187	2390	2397	2407	rBV	3915936	5488749	46.53%	5.111%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020325\
Data File : BP023915.D
Acq On : 04 Feb 2025 16:46
Operator : RC/JU
Sample : Q1202-09
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E29A0

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Title : SVOA CALIBRATION

37	17.287	2407	2414	2428	rBV2	6635432	9491350	80.46%	8.838%
38	18.122	2552	2556	2564	rBV2	85313	144063	1.22%	0.134%
39	19.204	2736	2740	2746	rBV2	74044	110352	0.94%	0.103%
40	19.281	2749	2753	2757	rBV	62770	97240	0.82%	0.091%
41	19.451	2779	2782	2787	rBV4	45639	60639	0.51%	0.056%
42	19.663	2812	2818	2827	rBV	8160417	11351440	96.22%	10.570%
43	21.557	3137	3140	3145	rVB	286331	376370	3.19%	0.350%
44	21.639	3147	3154	3166	rVB2	3626431	6129352	51.96%	5.707%
45	22.945	3370	3376	3386	rVB	752910	1469926	12.46%	1.369%
46	24.786	3678	3689	3710	rVB	4430540	11796788	100.00%	10.985%
47	25.010	3719	3727	3743	rVB	2435269	6454647	54.72%	6.010%




Sum of corrected areas: 107394704

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020325\
Data File : BP023915.D
Acq On : 04 Feb 2025 16:46
Operator : RC/JU
Sample : Q1202-09
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E29A0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

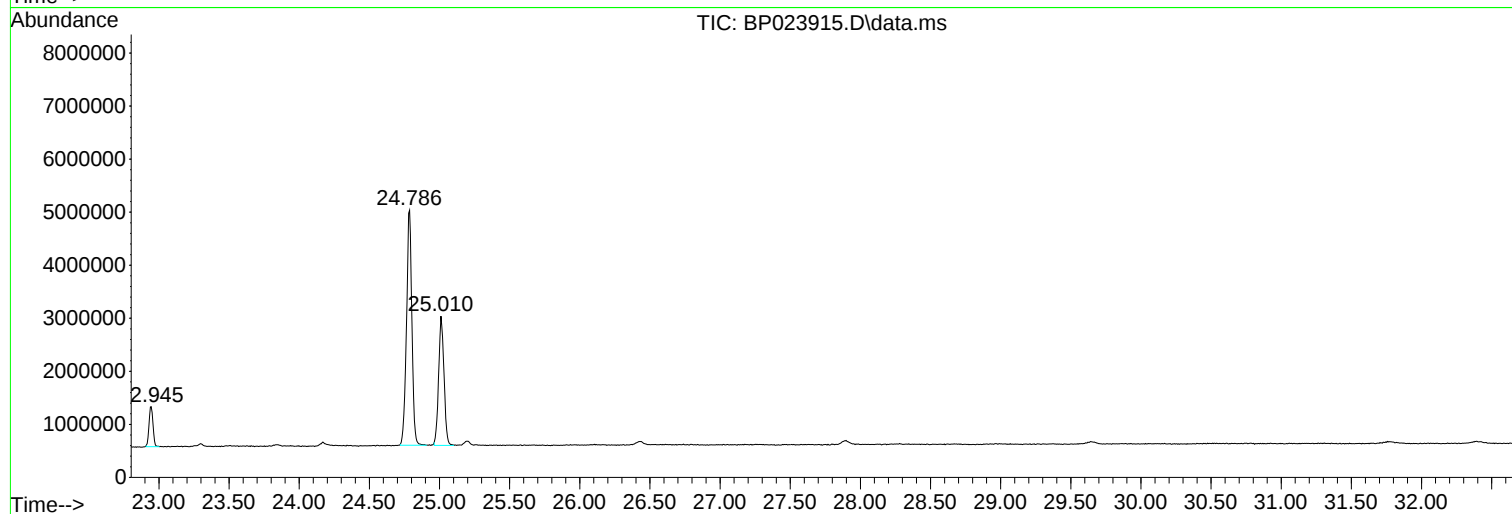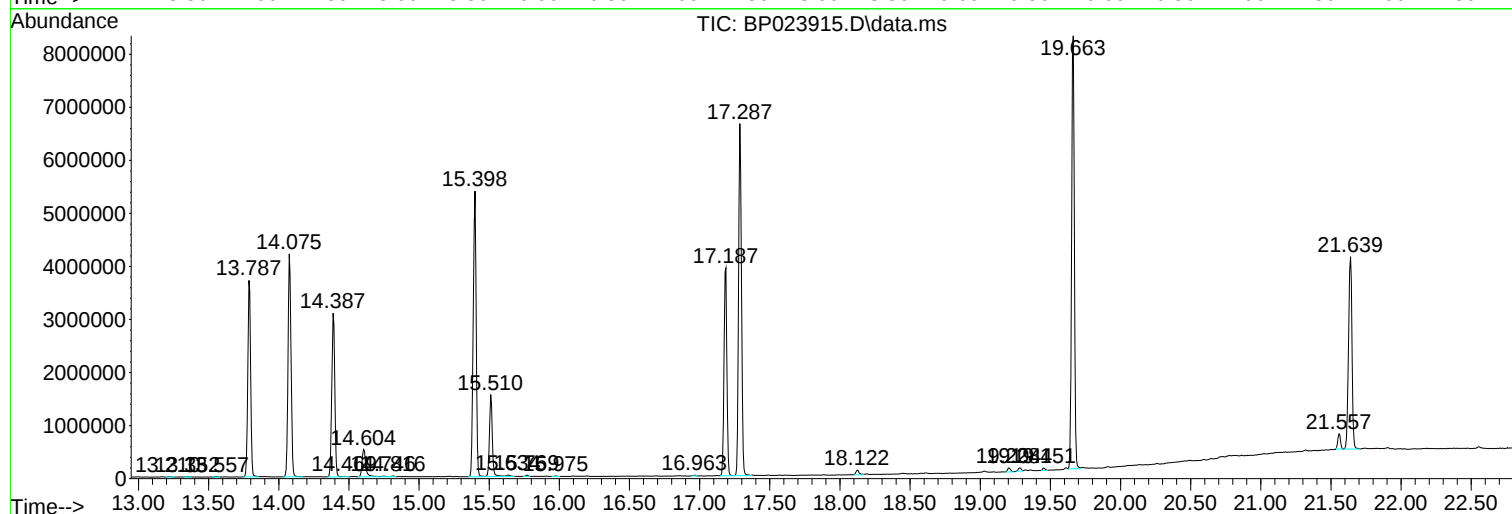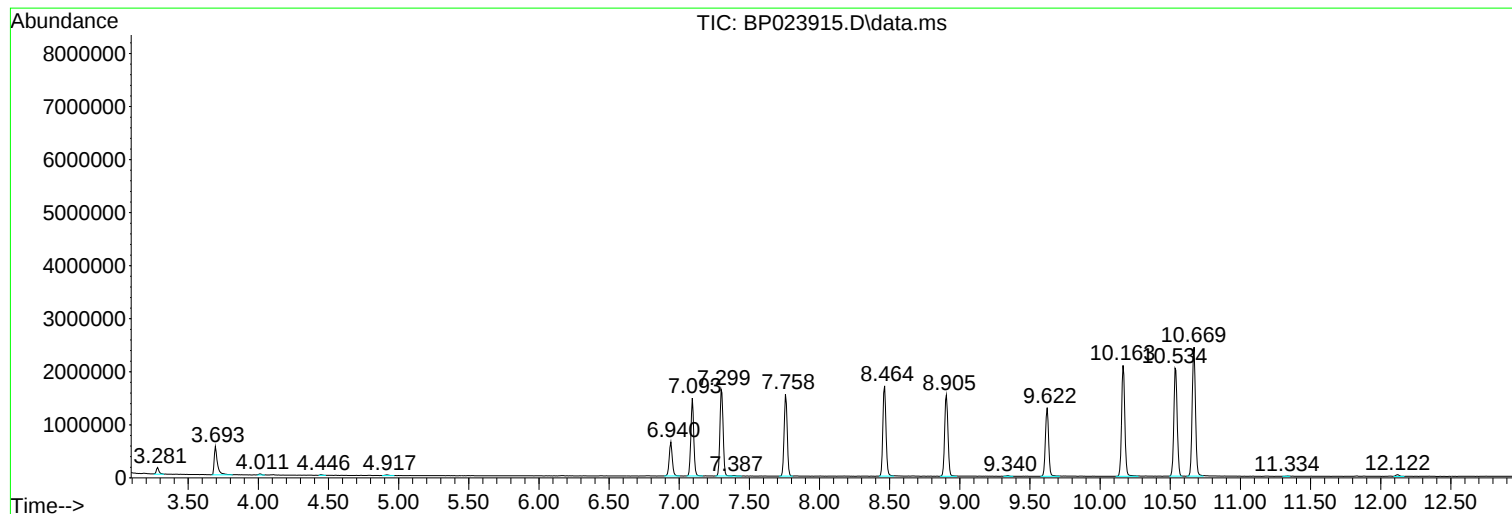

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020325\
Data File : BP023915.D
Acq On : 04 Feb 2025 16:46
Operator : RC/JU
Sample : Q1202-09
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E29A0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020325\
Data File : BP023915.D
Acq On : 04 Feb 2025 16:46
Operator : RC/JU
Sample : Q1202-09
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E29A0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
