

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020325\
 Data File : BP023918.D
 Acq On : 04 Feb 2025 18:47
 Operator : RC/JU
 Sample : Q1202-14
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E29A5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP023918.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.293	31	35	41	rVB	111118	137190	0.99%	0.117%
2	3.716	104	107	119	rBV	87303	148047	1.06%	0.126%
3	4.028	156	160	164	rVB	23165	31620	0.23%	0.027%
4	4.122	172	176	183	rVB7	9787	17065	0.12%	0.014%
5	4.469	231	235	241	rVB	17995	25895	0.19%	0.022%
6	4.940	309	315	319	rBV3	18734	30122	0.22%	0.026%
7	6.957	649	658	669	rBV	583333	969675	6.97%	0.824%
8	7.110	676	684	693	rBV	1633109	2531822	18.21%	2.151%
9	7.316	711	719	731	rBV	1877838	2904904	20.89%	2.468%
10	7.410	731	735	741	rVB6	10179	15271	0.11%	0.013%
11	7.775	788	797	804	rBV	1726156	2614283	18.80%	2.221%
12	8.475	907	916	928	rBV	1789917	2786831	20.04%	2.367%
13	8.916	983	991	999	rBV	1924070	3024221	21.75%	2.569%
14	9.351	1061	1065	1073	rVB	27713	40985	0.29%	0.035%
15	9.481	1082	1087	1093	rVB8	8183	14656	0.11%	0.012%
16	9.634	1104	1113	1128	rBV	1625986	2480559	17.84%	2.107%
17	10.175	1197	1205	1223	rBV	2585187	4049187	29.12%	3.440%
18	10.545	1260	1268	1277	rBV	2213823	3732895	26.85%	3.171%
19	10.675	1284	1290	1300	rBV	540555	903139	6.50%	0.767%
20	11.834	1481	1487	1492	rBV2	32606	48830	0.35%	0.041%
21	11.887	1492	1496	1502	rVB	18468	29001	0.21%	0.025%
22	12.128	1530	1537	1544	rBV	36762	63766	0.46%	0.054%
23	13.216	1718	1722	1729	rVB6	10163	16620	0.12%	0.014%
24	13.798	1813	1821	1833	rBV	4578761	6122846	44.04%	5.201%
25	14.081	1856	1869	1879	rBV	5047100	7356681	52.91%	6.249%
26	14.392	1913	1922	1932	rBV	3667236	5002571	35.98%	4.250%
27	14.610	1950	1959	1971	rBV	455866	821842	5.91%	0.698%
28	14.751	1979	1983	1989	rVB9	9668	16819	0.12%	0.014%
29	14.816	1989	1994	2004	rBV4	32772	56864	0.41%	0.048%
30	15.398	2084	2093	2105	rBV	7115051	9723857	69.94%	8.260%
31	15.510	2106	2112	2126	rVV	1736210	2526236	18.17%	2.146%
32	15.645	2130	2135	2144	rVB	26728	55789	0.40%	0.047%
33	15.763	2150	2155	2160	rBV	210984	264850	1.90%	0.225%
34	16.186	2224	2227	2232	rVB3	9896	15557	0.11%	0.013%
35	16.339	2244	2253	2259	rBV	23079	48701	0.35%	0.041%
36	16.957	2354	2358	2365	rVB	16744	28024	0.20%	0.024%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020325\
Data File : BP023918.D
Acq On : 04 Feb 2025 18:47
Operator : RC/JU
Sample : Q1202-14
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E29A5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Title : SVOA CALIBRATION

37	17.186	2389	2397	2406	rBV2	3906062	5956603	42.84%	5.060%
38	17.280	2407	2413	2427	rVV	8293199	11080685	79.70%	9.413%
39	18.116	2551	2555	2564	rBV2	97044	159801	1.15%	0.136%
40	18.439	2606	2610	2617	rBV6	33456	65658	0.47%	0.056%
41	18.992	2699	2704	2709	rBV4	24206	49514	0.36%	0.042%
42	19.198	2735	2739	2746	rBV2	86345	134523	0.97%	0.114%
43	19.274	2748	2752	2758	rVB	77024	115822	0.83%	0.098%
44	19.651	2810	2816	2826	rBV	10557204	13792394	99.20%	11.716%
45	21.621	3145	3151	3160	rBV2	4335338	6763115	48.64%	5.745%
46	24.751	3674	3683	3700	rVB	5905793	13903305	100.00%	11.810%
47	24.986	3714	3723	3736	rVB2	2717733	7041684	50.65%	5.982%




Sum of corrected areas: 117720325

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020325\
Data File : BP023918.D
Acq On : 04 Feb 2025 18:47
Operator : RC/JU
Sample : Q1202-14
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E29A5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

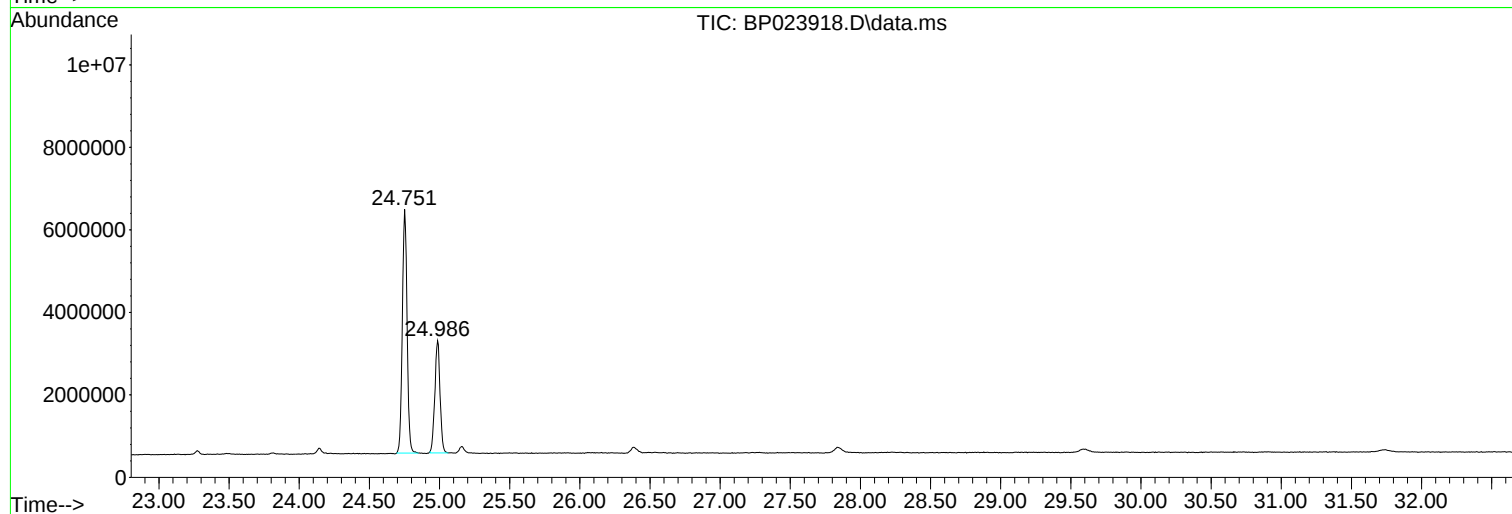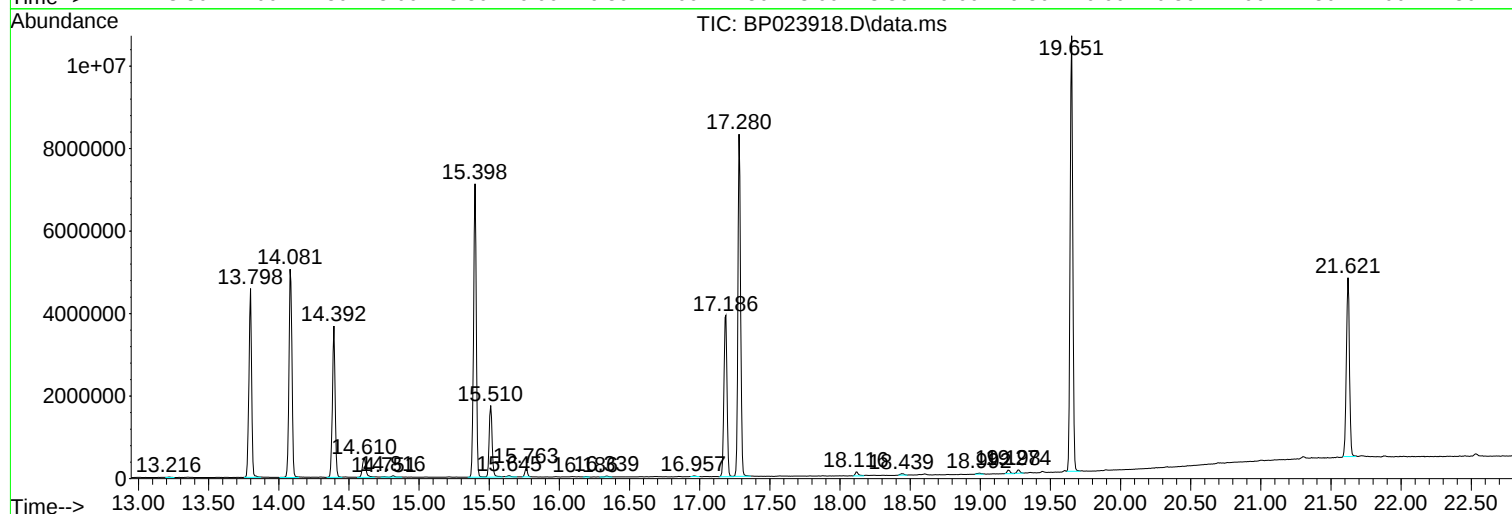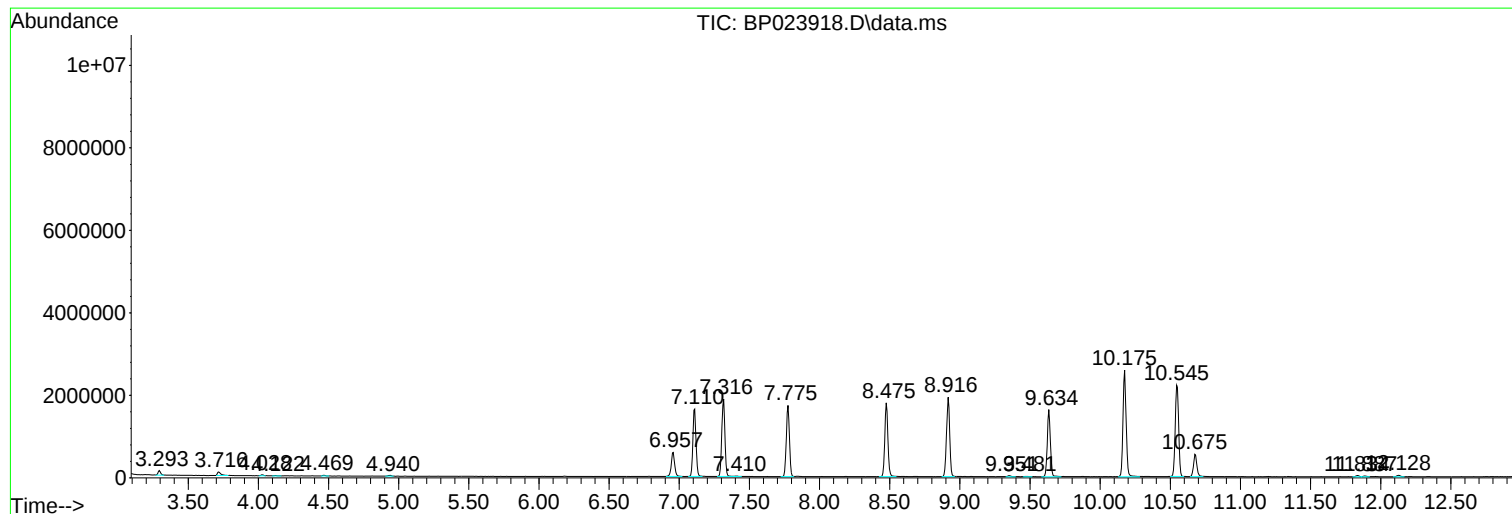

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020325\
Data File : BP023918.D
Acq On : 04 Feb 2025 18:47
Operator : RC/JU
Sample : Q1202-14
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E29A5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020325\
Data File : BP023918.D
Acq On : 04 Feb 2025 18:47
Operator : RC/JU
Sample : Q1202-14
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E29A5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc