

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020325\
 Data File : BP023919.D
 Acq On : 04 Feb 2025 19:28
 Operator : RC/JU
 Sample : Q1202-15
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E29A7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP023919.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.293	31	35	45	rVB	116705	152103	1.08%	0.120%
2	3.705	101	105	123	rBV	472241	794373	5.65%	0.626%
3	4.028	156	160	165	rVB	23467	33206	0.24%	0.026%
4	4.464	231	234	240	rVB2	15396	22922	0.16%	0.018%
5	4.934	309	314	319	rBV3	16797	30328	0.22%	0.024%
6	6.958	649	658	674	rVB	626329	1003395	7.13%	0.791%
7	7.110	677	684	693	rBV	1802920	2669750	18.97%	2.103%
8	7.316	711	719	728	rBV	2030590	3114547	22.13%	2.454%
9	7.775	789	797	805	rBV	1776480	2704831	19.22%	2.131%
10	8.475	909	916	928	rBV	1874051	2968946	21.10%	2.339%
11	8.916	983	991	1008	rBV	2007254	3270482	23.24%	2.577%
12	9.352	1060	1065	1070	rVB4	10175	17959	0.13%	0.014%
13	9.634	1103	1113	1126	rBV	1634559	2671147	18.98%	2.105%
14	10.175	1195	1205	1227	rBV	2707622	4518143	32.11%	3.560%
15	10.546	1260	1268	1276	rVB	2483572	4014385	28.53%	3.163%
16	10.675	1282	1290	1308	rBV	2388038	3932999	27.95%	3.099%
17	12.128	1532	1537	1545	rVV2	40512	63387	0.45%	0.050%
18	13.175	1708	1715	1720	rBV7	7966	15266	0.11%	0.012%
19	13.351	1742	1745	1756	rVB5	8064	16830	0.12%	0.013%
20	13.563	1776	1781	1785	rBV2	10072	16584	0.12%	0.013%
21	13.798	1812	1821	1837	rBV	5341522	6862240	48.77%	5.407%
22	14.081	1862	1869	1887	rBV	5903067	8305621	59.02%	6.544%
23	14.392	1915	1922	1931	rBV	3816072	5393377	38.33%	4.249%
24	14.469	1931	1935	1943	rVB	8475	17263	0.12%	0.014%
25	14.610	1952	1959	1972	rBV	502306	904475	6.43%	0.713%
26	14.751	1979	1983	1989	rVV8	10742	17048	0.12%	0.013%
27	14.816	1989	1994	1999	rVB7	13418	25084	0.18%	0.020%
28	15.228	2059	2064	2069	rVB4	12710	20703	0.15%	0.016%
29	15.398	2086	2093	2106	rBV	7535885	10754481	76.43%	8.473%
30	15.516	2106	2113	2130	rVV	1956982	2699425	19.18%	2.127%
31	15.639	2130	2134	2142	rVB2	30968	58690	0.42%	0.046%
32	15.975	2186	2191	2195	rBV8	7822	14457	0.10%	0.011%
33	16.198	2224	2229	2232	rBV7	10057	15088	0.11%	0.012%
34	16.963	2355	2359	2363	rVB2	16392	24470	0.17%	0.019%
35	17.181	2390	2396	2407	rBV2	4578517	6269117	44.55%	4.939%
36	17.281	2407	2413	2427	rVV	8177125	11882370	84.44%	9.362%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020325\
Data File : BP023919.D
Acq On : 04 Feb 2025 19:28
Operator : RC/JU
Sample : Q1202-15
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E29A7

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Title : SVOA CALIBRATION

37	17.875	2511	2514	2521	rBV8	11203	21479	0.15%	0.017%
38	18.116	2551	2555	2560	rBV4	34390	50622	0.36%	0.040%
39	18.445	2607	2611	2616	rBV5	17855	31920	0.23%	0.025%
40	18.598	2634	2637	2642	rVB4	21979	30101	0.21%	0.024%
41	19.198	2735	2739	2744	rVB	92116	119329	0.85%	0.094%
42	19.263	2746	2750	2754	rBV	92838	117789	0.84%	0.093%
43	19.645	2809	2815	2824	rBV	9480518	14071846	100.00%	11.087%
44	21.616	3144	3150	3161	rVB2	4047933	6692856	47.56%	5.273%
45	24.757	3673	3684	3698	rBV	5286574	13530083	96.15%	10.660%
46	24.992	3714	3724	3738	rVB	2393103	6960450	49.46%	5.484%




Sum of corrected areas: 126921967

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020325\
Data File : BP023919.D
Acq On : 04 Feb 2025 19:28
Operator : RC/JU
Sample : Q1202-15
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E29A7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

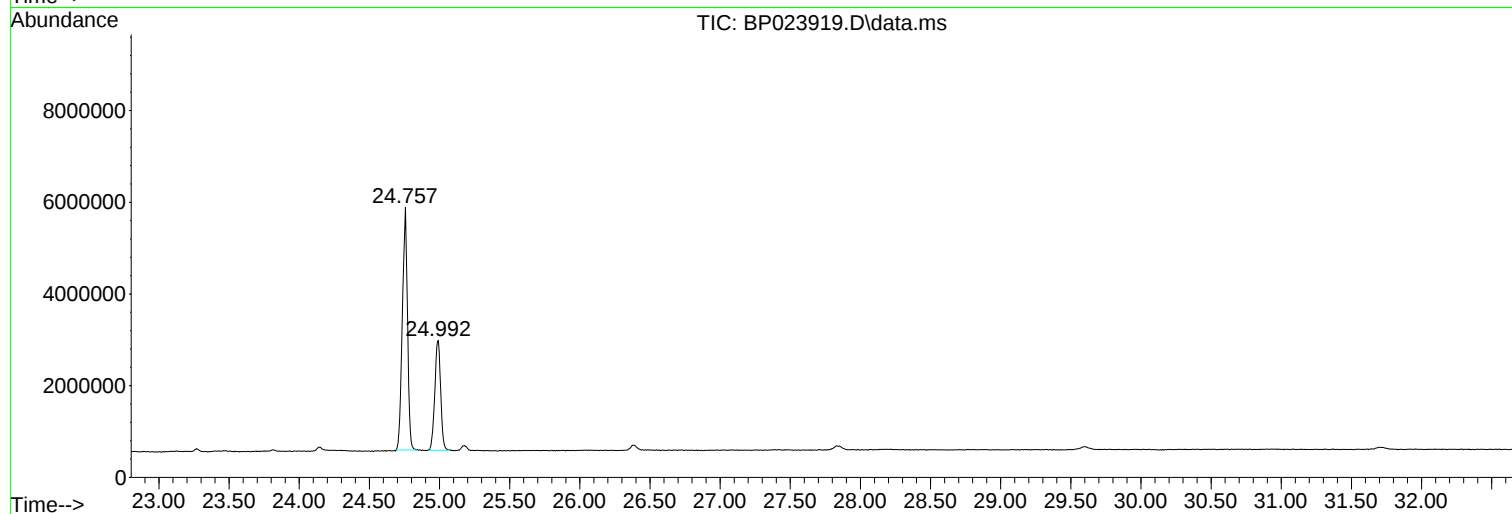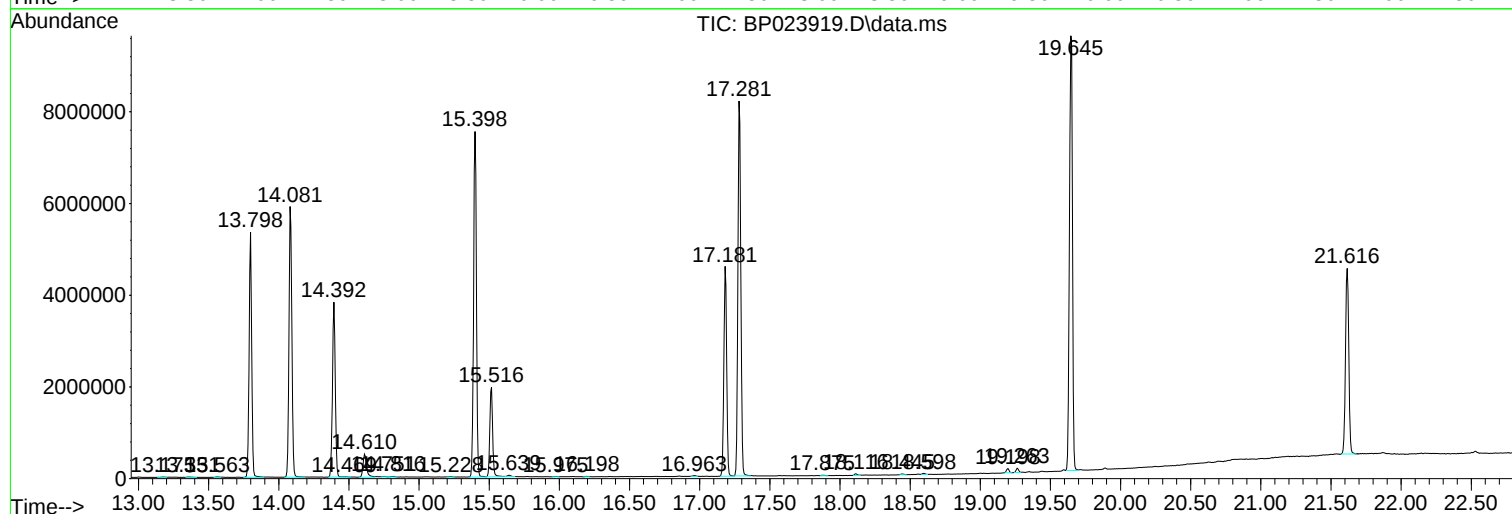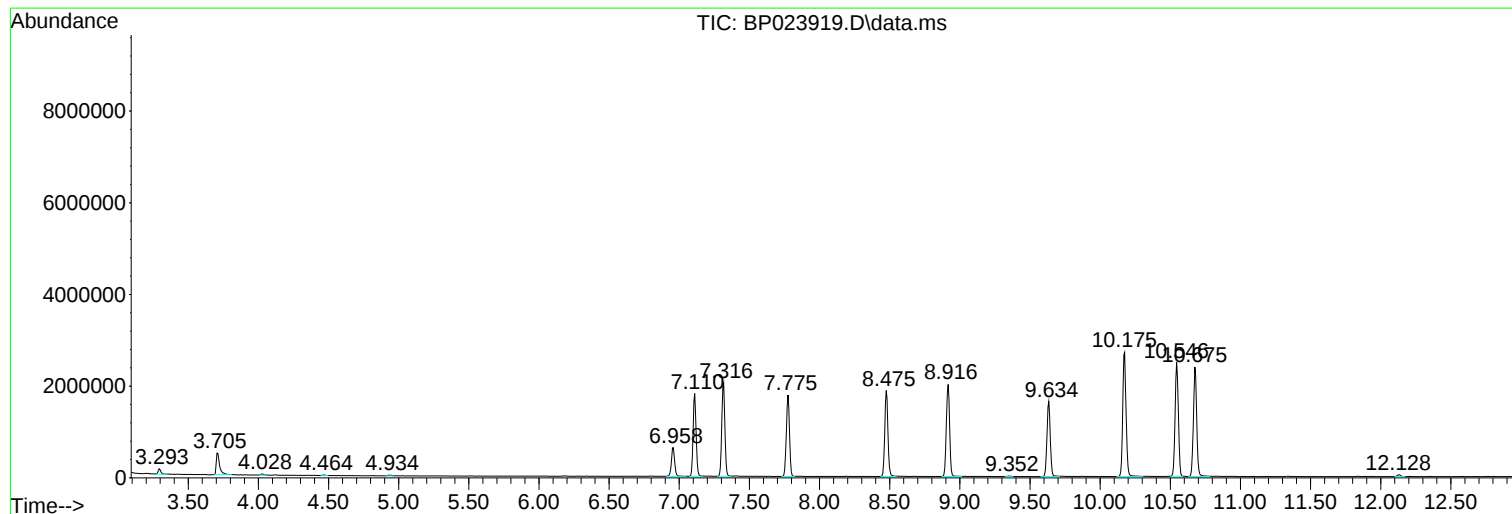

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020325\
Data File : BP023919.D
Acq On : 04 Feb 2025 19:28
Operator : RC/JU
Sample : Q1202-15
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E29A7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020325\
Data File : BP023919.D
Acq On : 04 Feb 2025 19:28
Operator : RC/JU
Sample : Q1202-15
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E29A7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------