

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020422\
Data File : BP009037.D
Acq On : 04 Feb 2022 15:02
Operator : CG/JU
Sample : PB142454BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB142454BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020422.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP009037.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.399	403	410	430	rBV	3019078	5019699	60.69%	11.088%
2	6.993	673	681	707	rBV	2949586	5201280	62.89%	11.489%
3	7.805	812	819	832	rBV	676357	1153778	13.95%	2.548%
4	8.969	1009	1017	1050	rBV	1856296	3410753	41.24%	7.534%
5	10.604	1287	1295	1319	rBV	738460	1542612	18.65%	3.407%
6	13.069	1707	1714	1746	rBV	5077944	8270710	100.00%	18.268%
7	14.451	1942	1949	1972	rBV	1205132	2040216	24.67%	4.506%
8	15.945	2194	2203	2237	rBV	3213807	5468735	66.12%	12.079%
9	17.210	2411	2418	2437	rBV	1197507	2112086	25.54%	4.665%
10	19.774	2848	2854	2868	rBV	6093243	8013745	96.89%	17.701%
11	21.304	3110	3114	3125	rBV	981727	1565240	18.93%	3.457%
12	23.704	3517	3522	3536	rVB2	669293	1474640	17.83%	3.257%




Sum of corrected areas: 45273494

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020422\
Data File : BP009037.D
Acq On : 04 Feb 2022 15:02
Operator : CG/JU
Sample : PB142454BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB142454BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

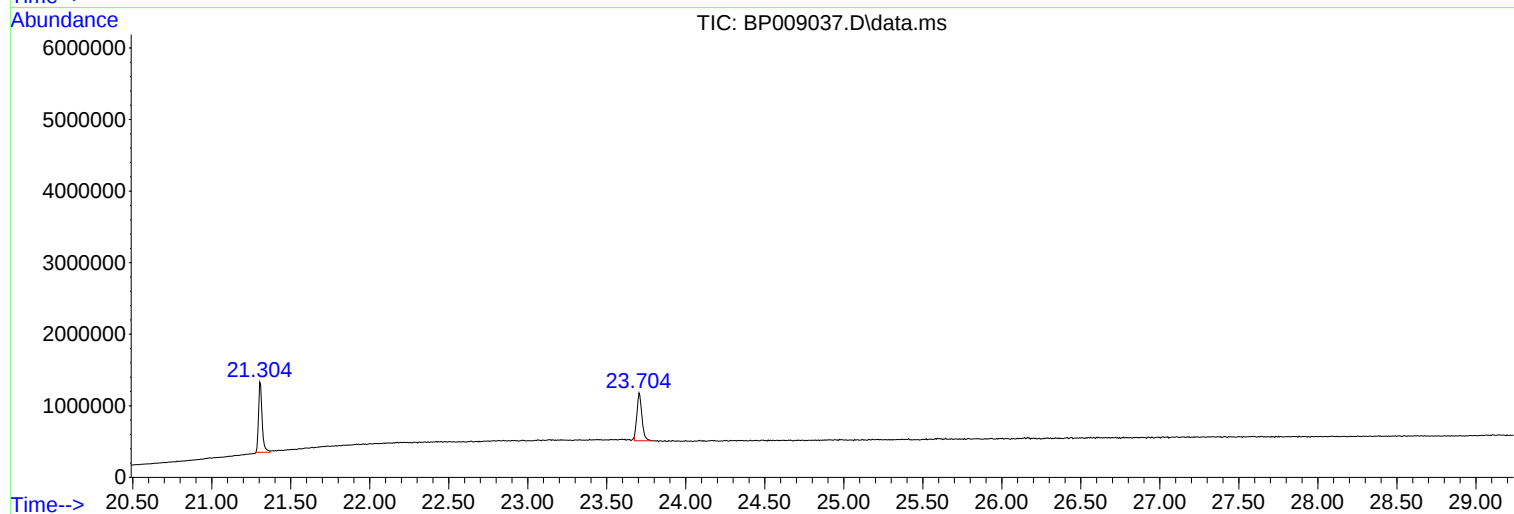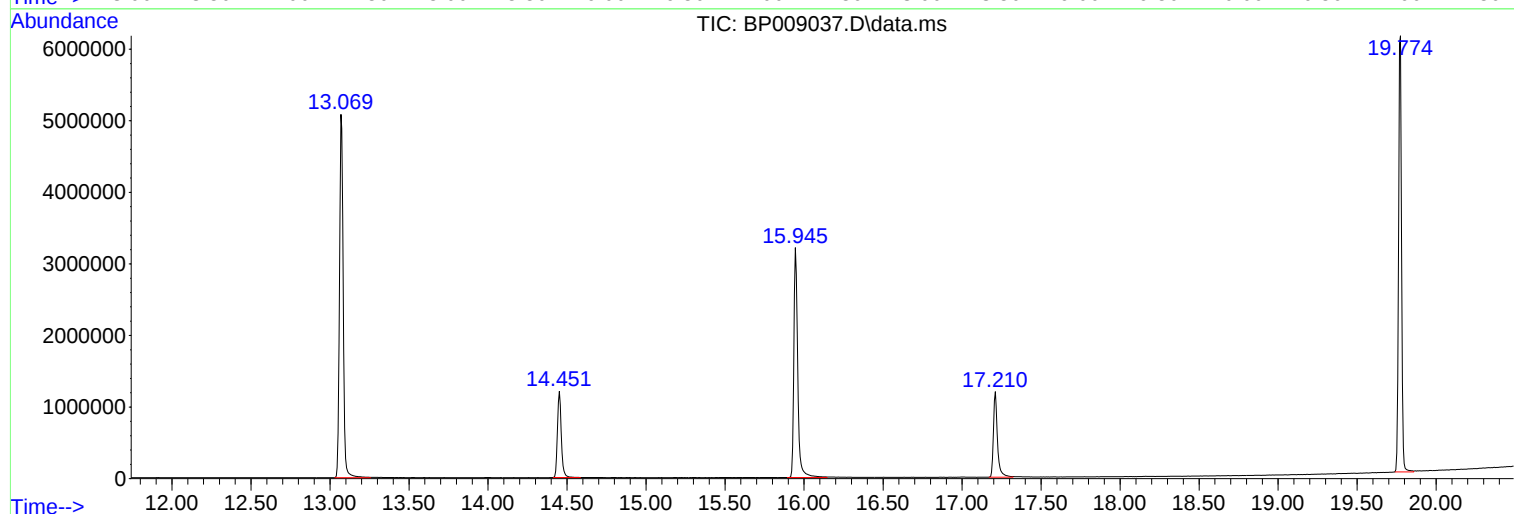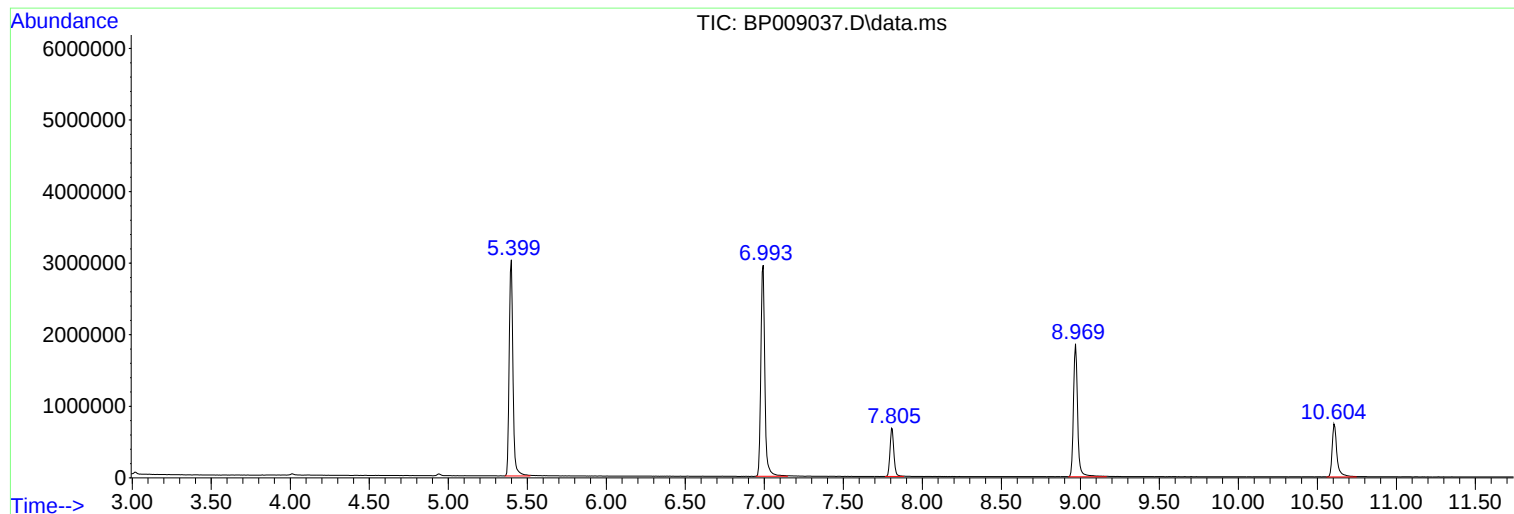

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020422\
Data File : BP009037.D
Acq On : 04 Feb 2022 15:02
Operator : CG/JU
Sample : PB142454BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB142454BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020422\
Data File : BP009037.D
Acq On : 04 Feb 2022 15:02
Operator : CG/JU
Sample : PB142454BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB142454BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------