


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020422\
 Data File : BP009028.D
 Acq On : 04 Feb 2022 08:44
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Feb 04 14:19:33 2022

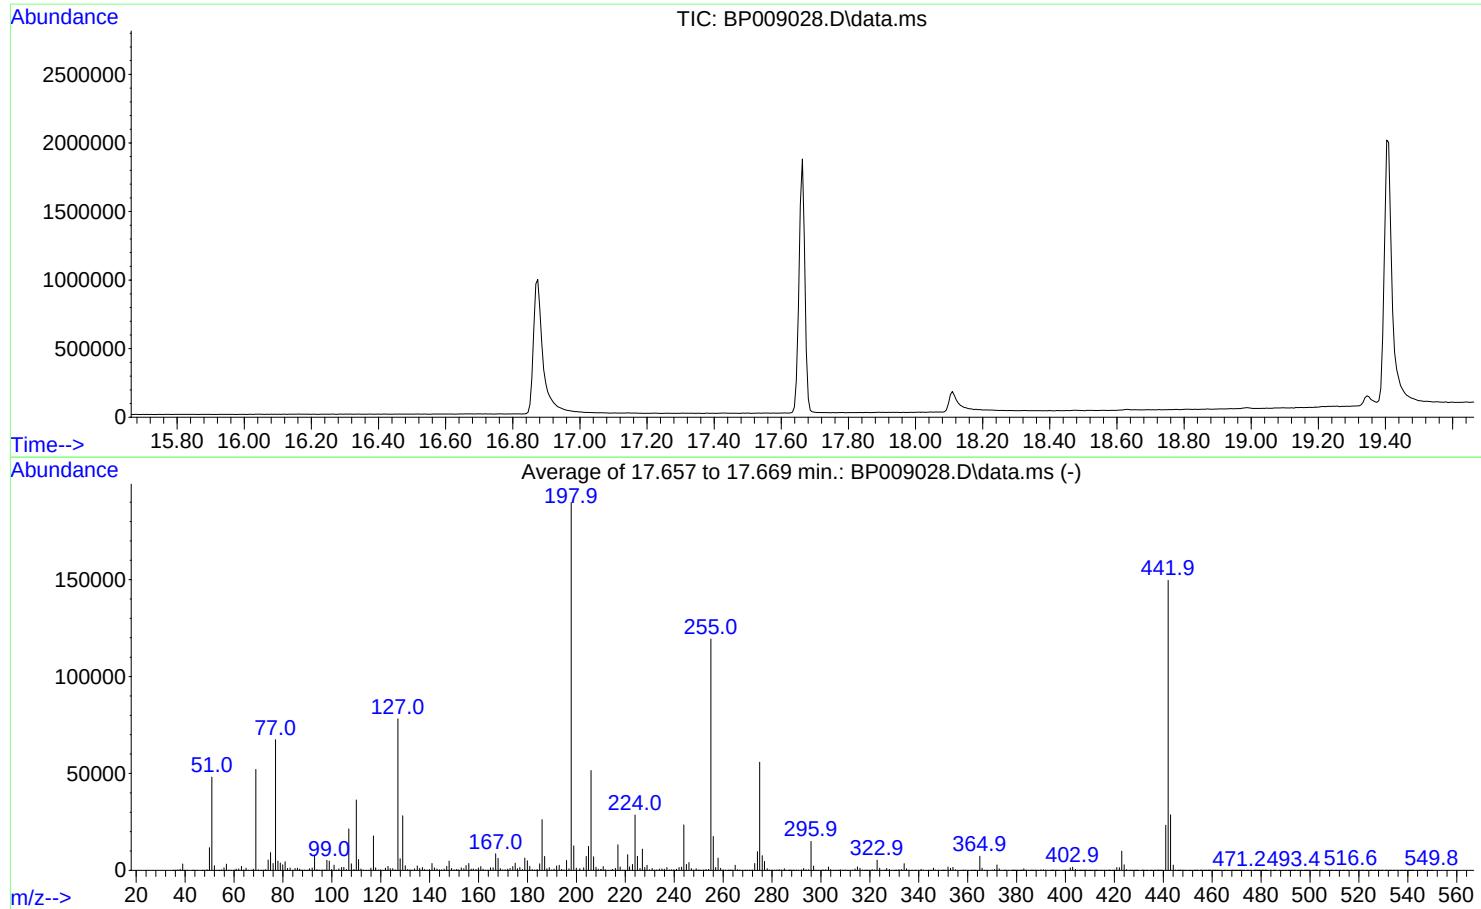

AutoFind: Scans 2494, 2495, 2496; Background Corrected with Scan 2484

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.3	48105	PASS
68	69	0.00	2	1.4	707	PASS
69	198	0.00	100	27.4	52064	PASS
70	69	0.00	2	0.6	288	PASS
127	198	10	80	41.2	78215	PASS
197	198	0.00	2	0.4	837	PASS
198	198	100	100	100.0	189805	PASS
199	198	5	9	6.7	12672	PASS
275	198	10	60	29.4	55785	PASS
365	198	1	100	3.8	7272	PASS
441	198	0.01	100	12.3	23285	PASS
442	442	100	100	100.0	149617	PASS
443	442	15	24	19.2	28676	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
2/4/2022	BNA_P	<u>BP009028.D</u>
Compound Name	Response	Retention Time
DDT	634205	20.61
DDD	2462	20.18
DDE	498	19.68
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2960	637165	0.46

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020422\
 Data File : BP009028.D
 Acq On : 04 Feb 2022 08:44
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Feb 04 13:23:14 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 04 13:16:05 2022
 Response via : Initial Calibration

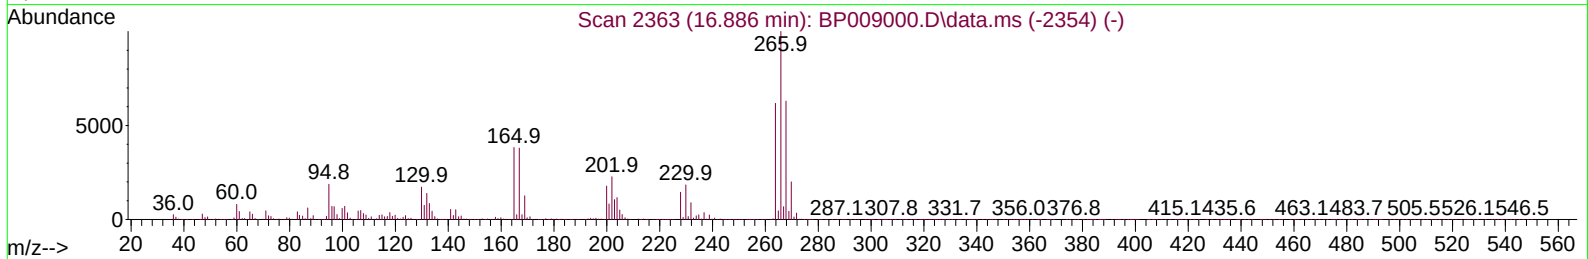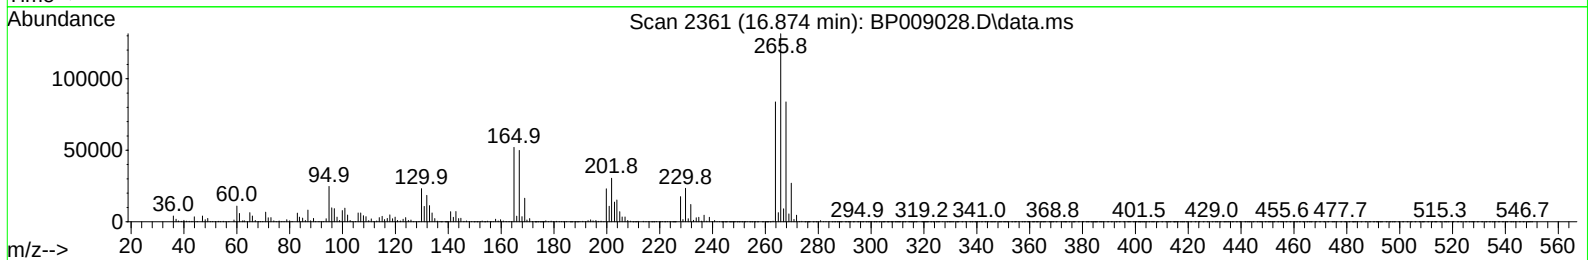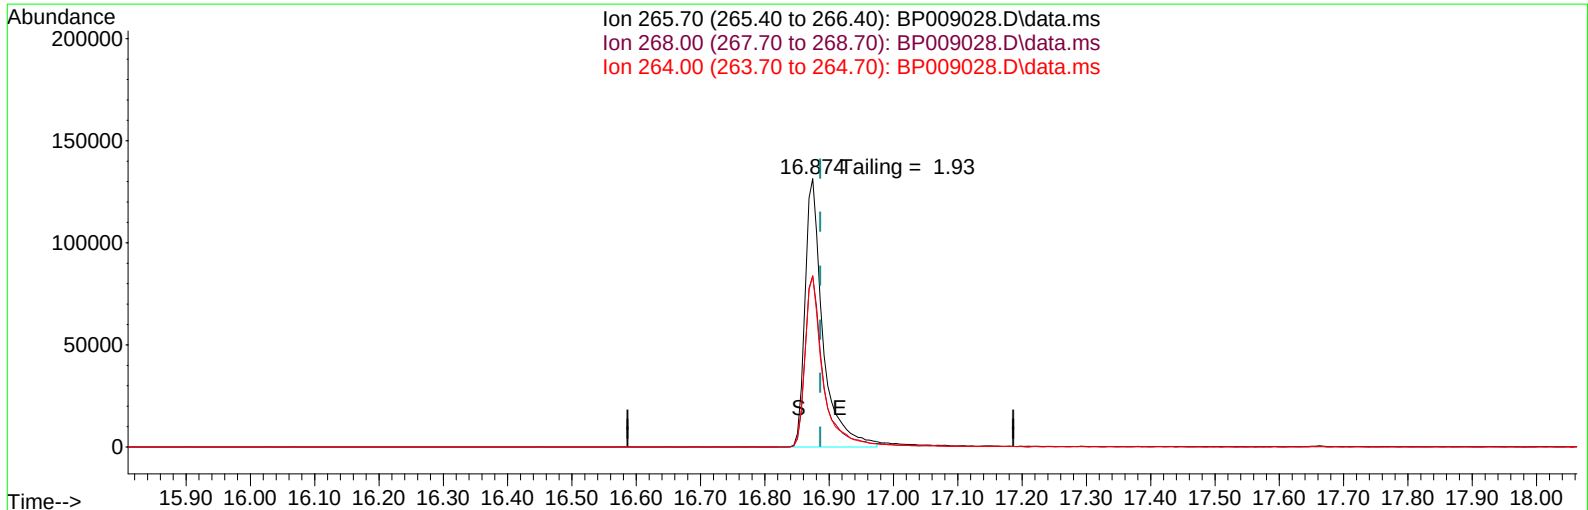

TIC: BP009028.D\data.ms

(70) Pentachlorophenol (C)

16.874min (-0.012) 747192.27 ng


response 261970

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	63.72
264.00	62.90	63.78
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020422\
 Data File : BP009028.D
 Acq On : 04 Feb 2022 08:44
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Feb 04 13:23:14 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 04 13:16:05 2022
 Response via : Initial Calibration

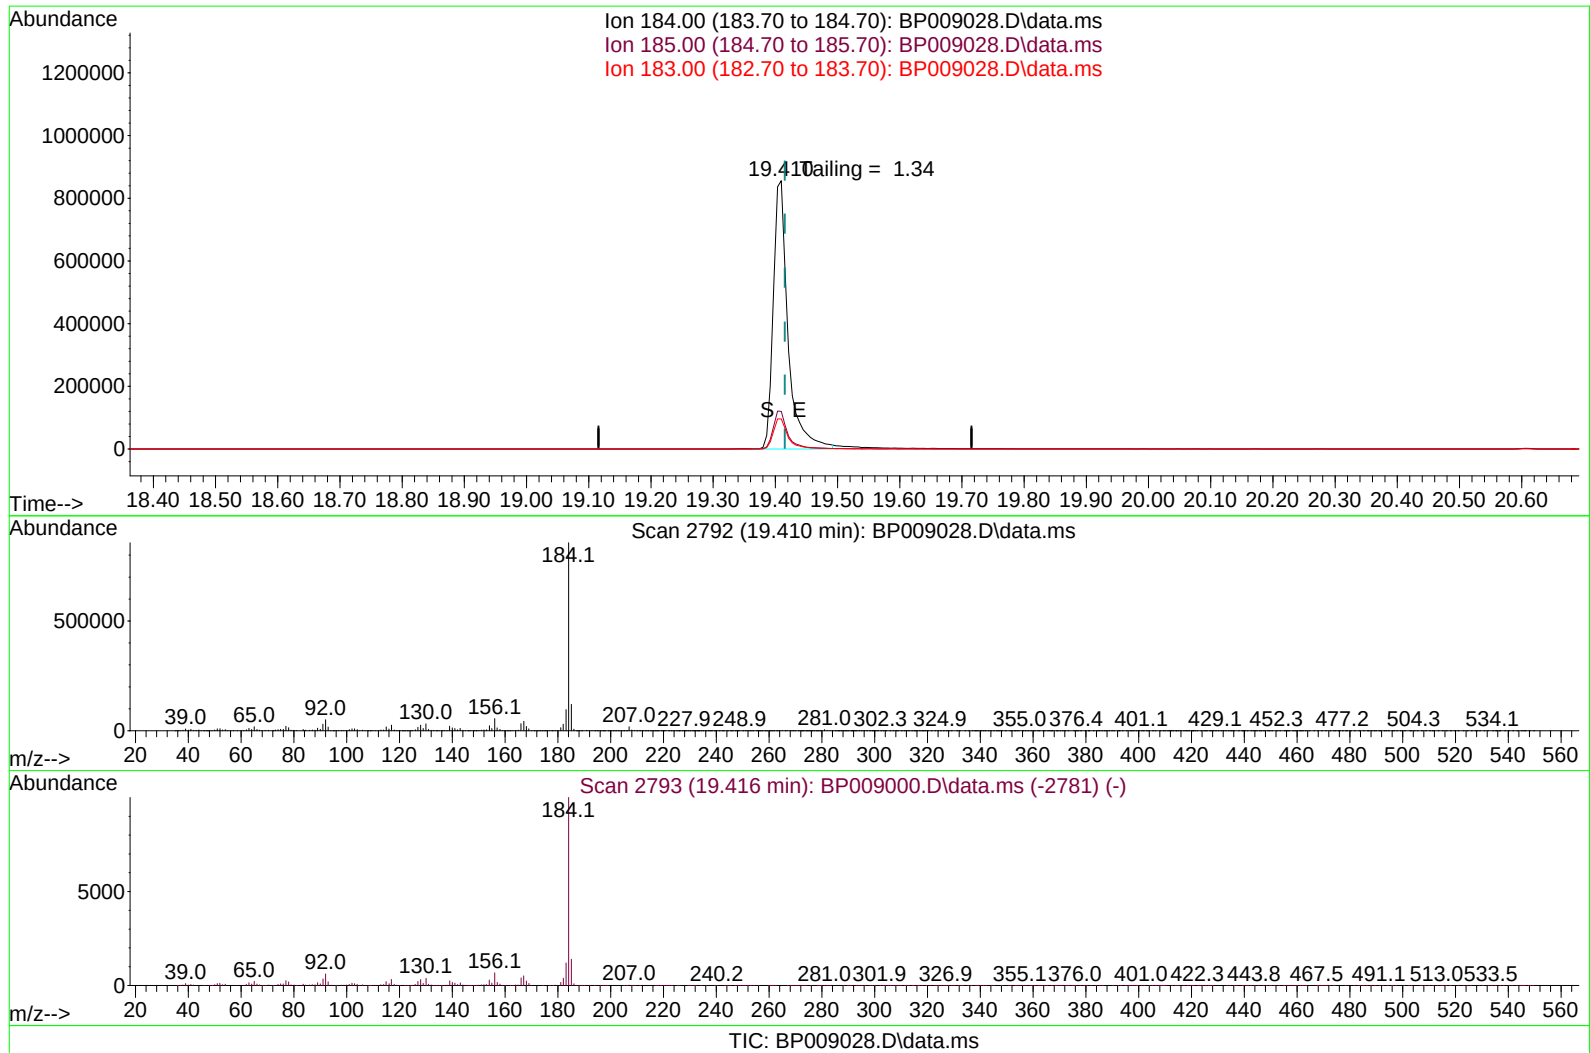**(77) Benzidine**

19.410min (-0.006) 550313.15 ng

response 1458101

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.04
183.00	11.90	11.22
0.00	0.00	0.00