


Benzoic acid

Response Ratio

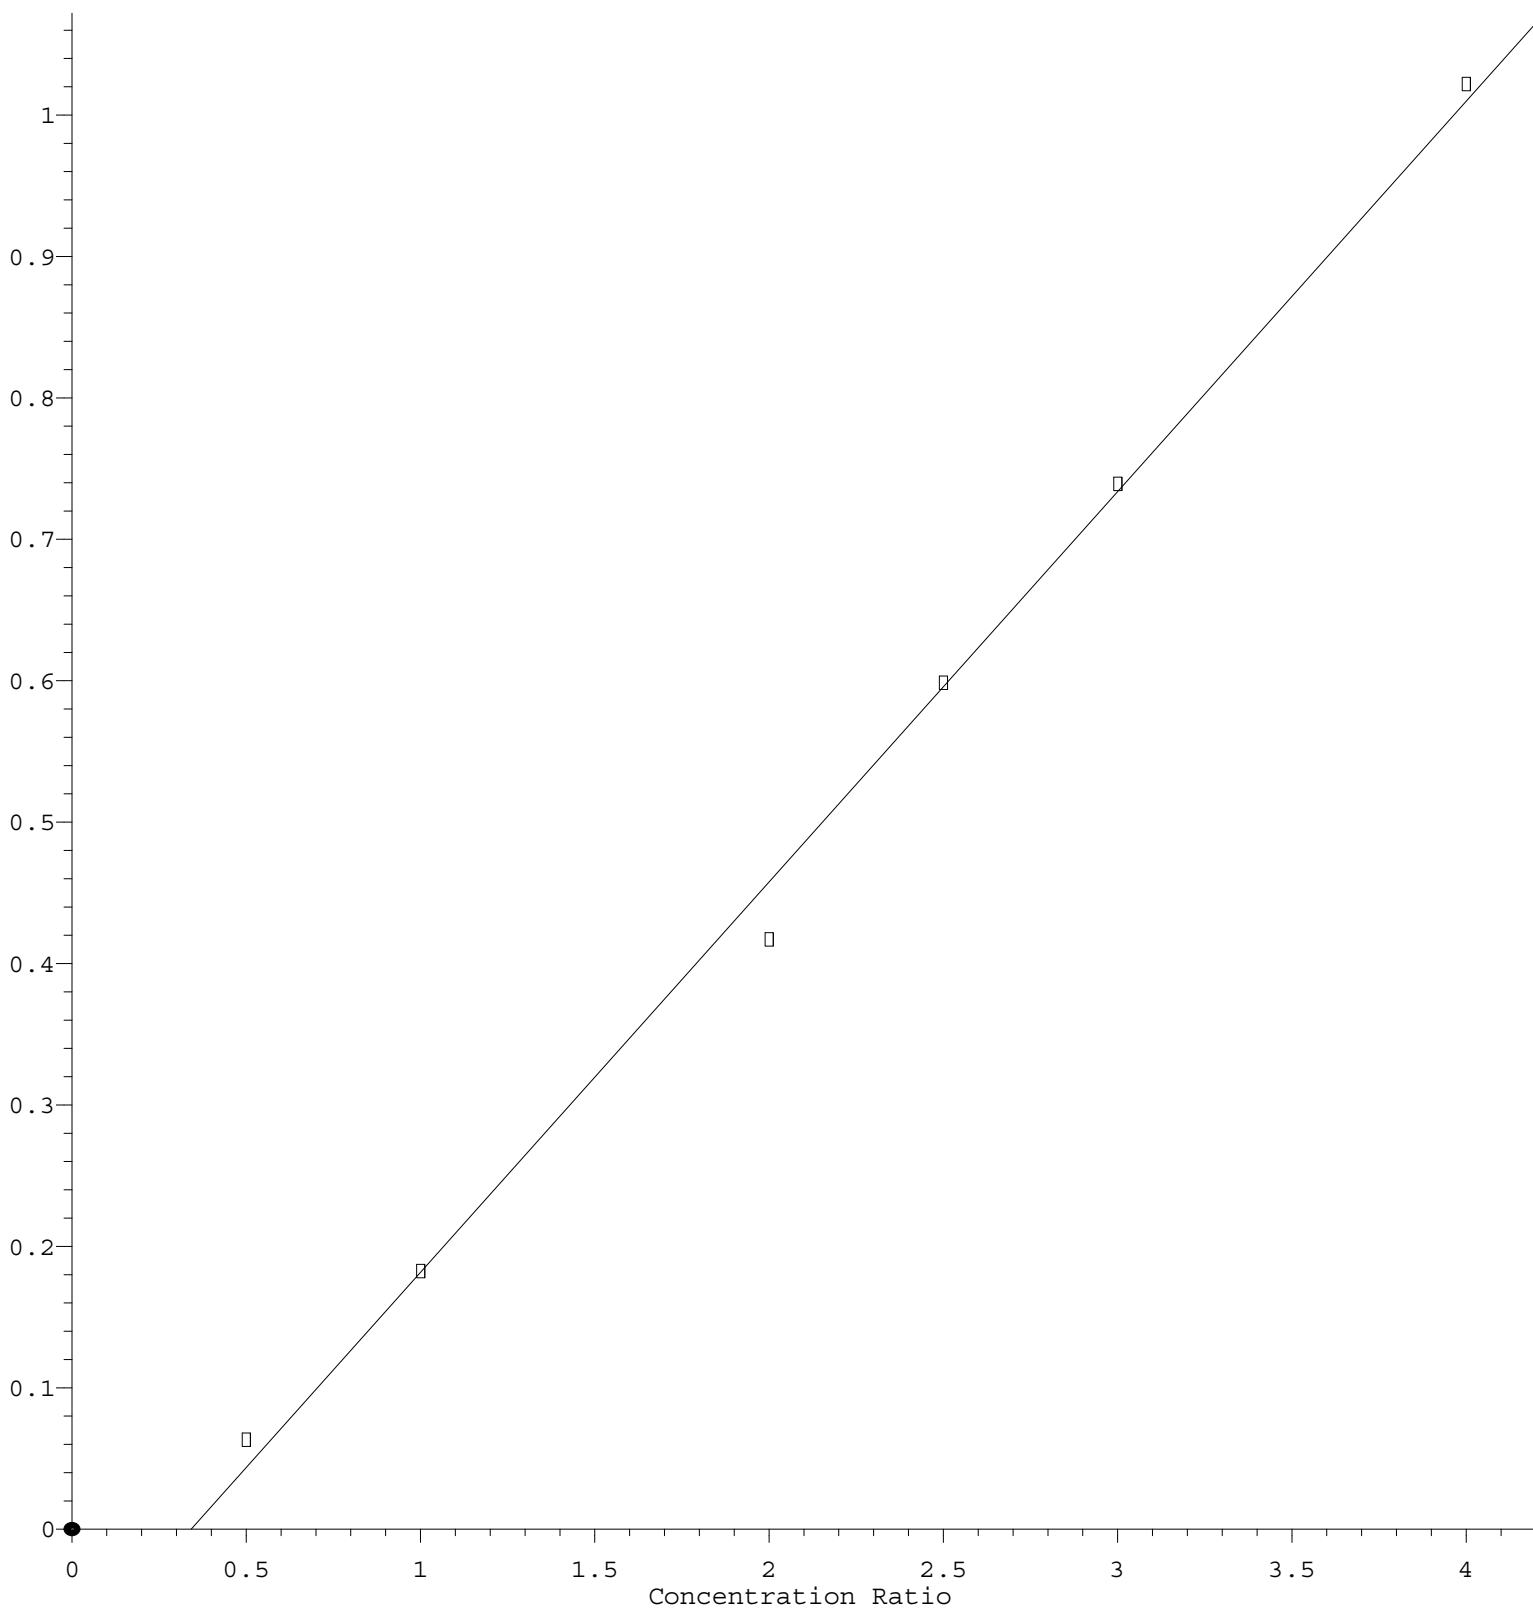

$$\text{Response} = 2.761\text{e-}001 * \text{Amt} - 9.457\text{e-}002$$


Coef of Det (r^2) = 0.996520 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270E-BP020521.M

Calibration Table Last Updated: Fri Feb 05 18:04:48 2021

Benzidine

Response Ratio

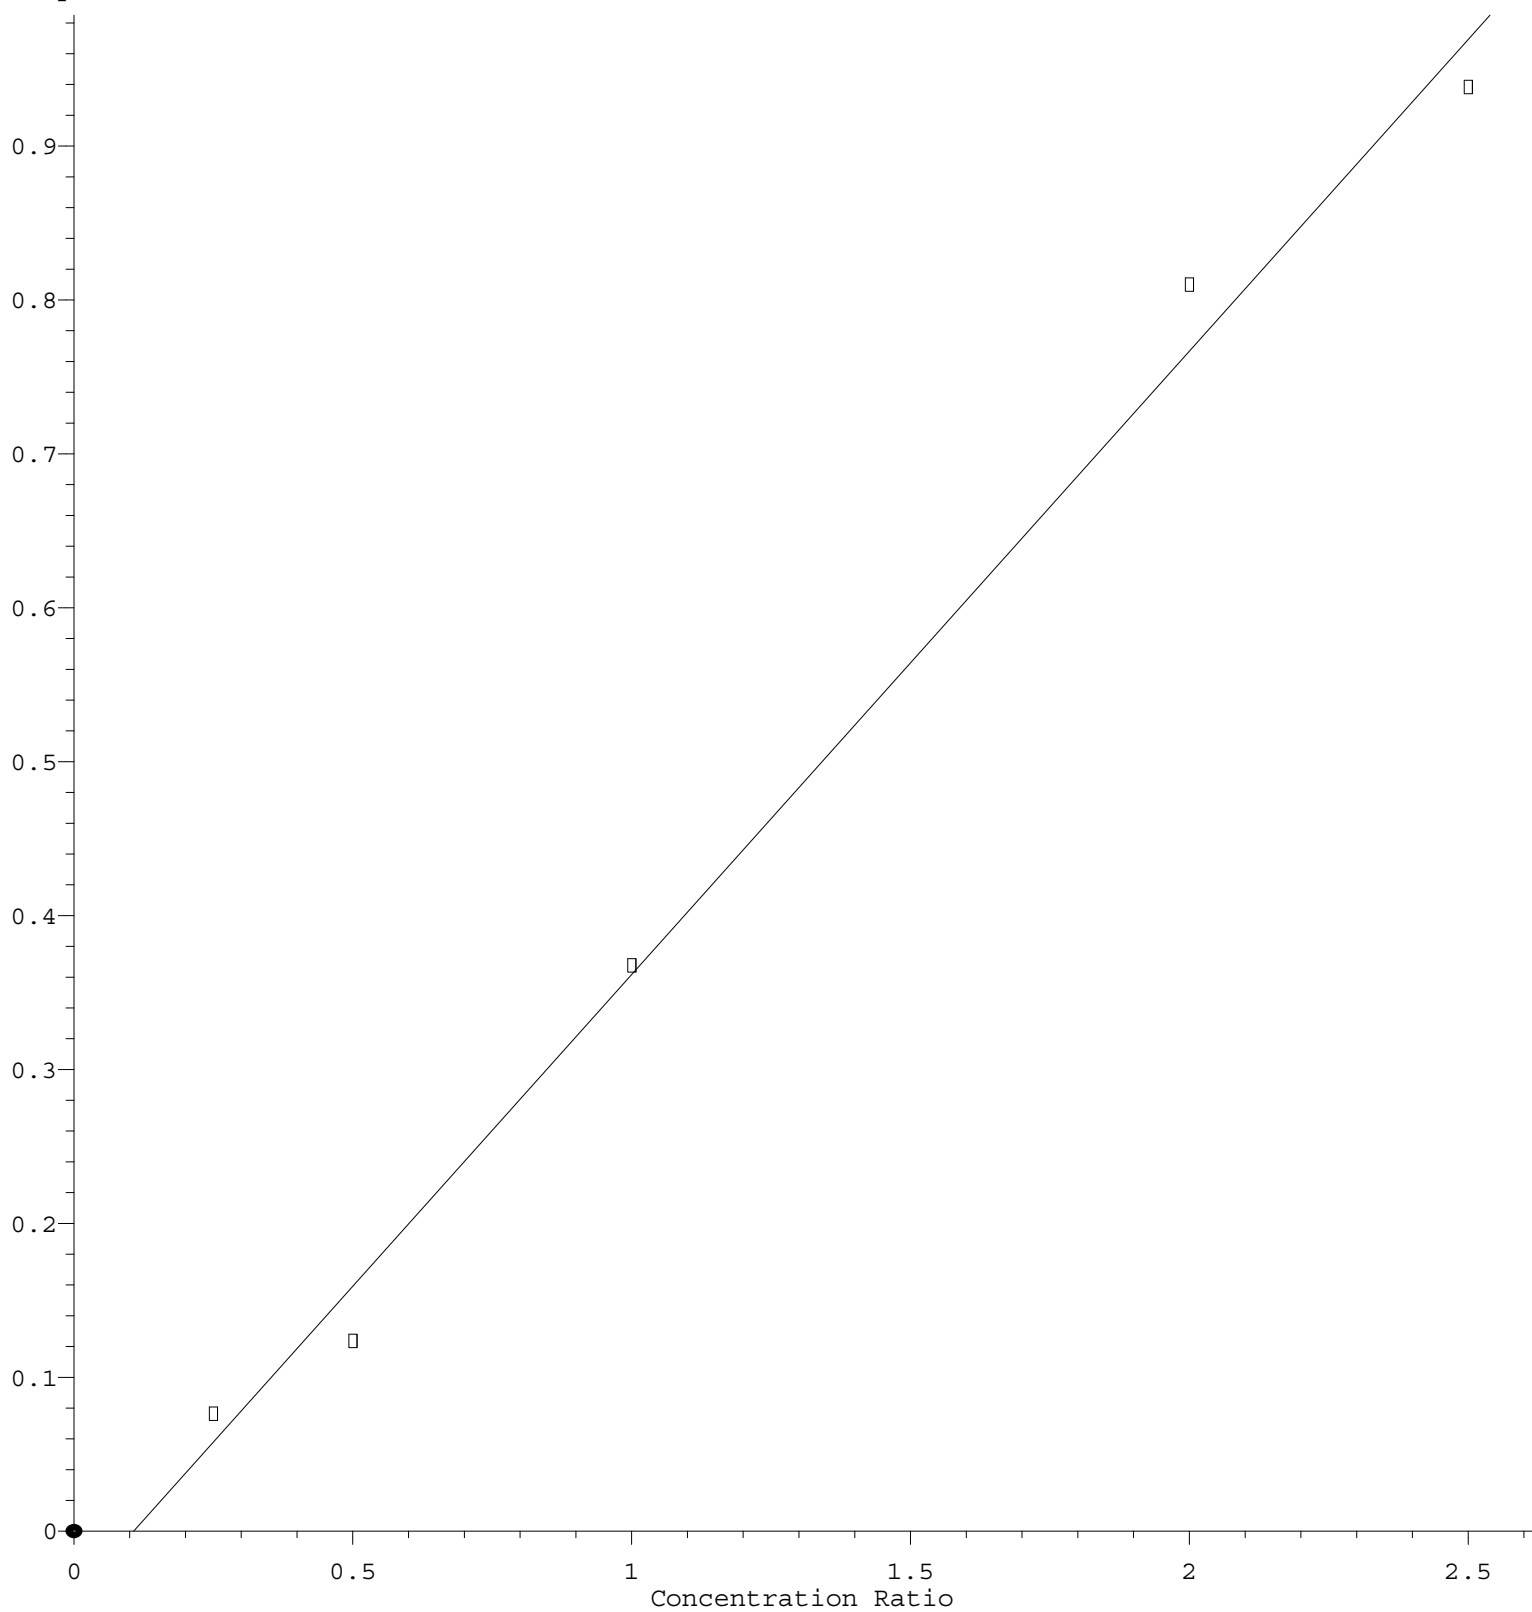

$$\text{Response} = 4.052\text{e-}001 * \text{Amt} - 4.330\text{e-}002$$

Coef of Det (r^2) = 0.992812 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270E-BP020521.M

Calibration Table Last Updated: Fri Feb 05 18:04:48 2021