
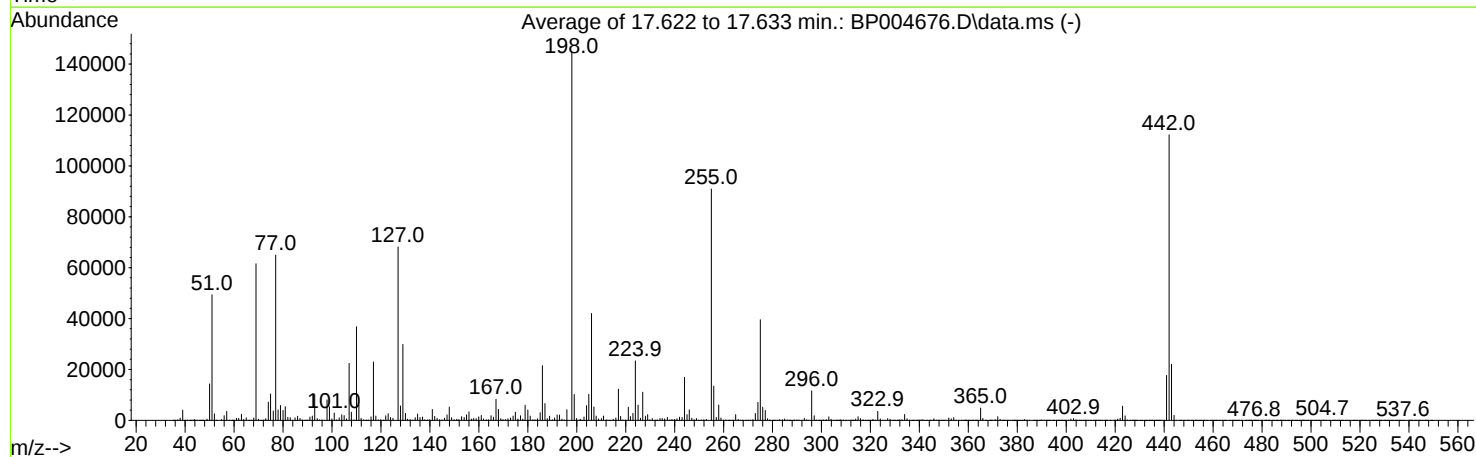


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020521\
 Data File : BP004676.D
 Acq On : 05 Feb 2021 12:58
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270E-BP020521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Feb 05 18:04:48 2021

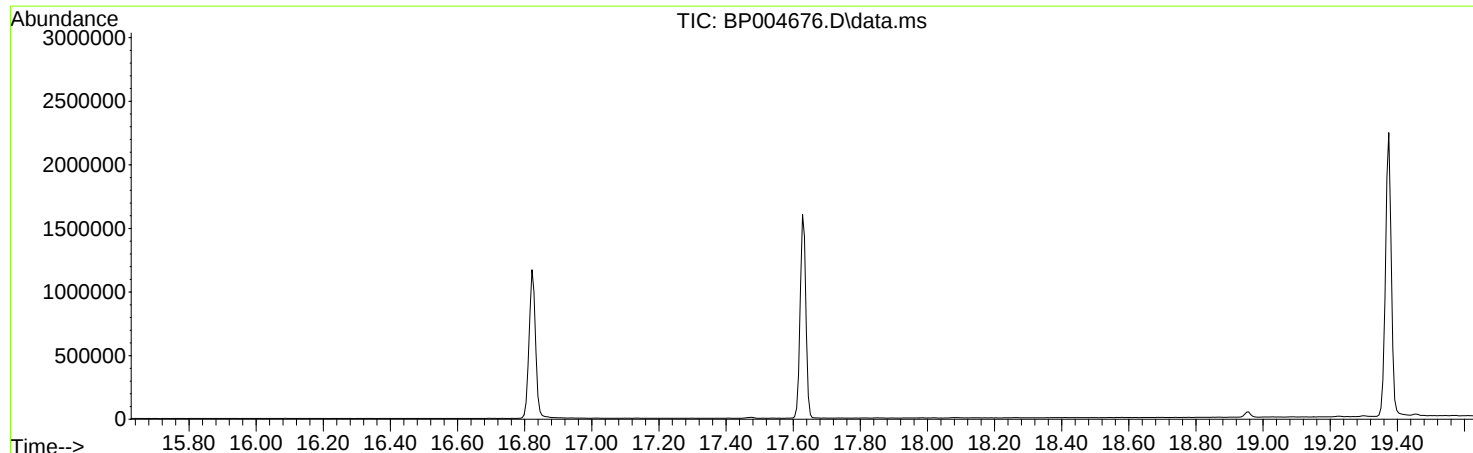

AutoFind: Scans 2454, 2455, 2456; Background Corrected with Scan 2443

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.2	49383	PASS
68	69	0.00	2	1.5	931	PASS
69	198	0.00	100	42.6	61591	PASS
70	69	0.00	2	0.7	451	PASS
127	198	10	80	47.2	68179	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	144560	PASS
199	198	5	9	7.0	10186	PASS
275	198	10	60	27.4	39573	PASS
365	198	1	100	3.3	4822	PASS
441	198	0.01	100	12.2	17663	PASS
442	442	100	100	100.0	112240	PASS
443	442	15	24	19.7	22078	PASS

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP




DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/5/2021	BNA_P	<u>BP004676.D</u>
Compound Name	Response	Retention Time
DDT	608090	20.574
DDD	2846	20.145
DDE	787	19.657
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3633	611723	0.59

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020521\
 Data File : BP004676.D
 Acq On : 05 Feb 2021 12:58
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Feb 06 03:59:49 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270E-BP020521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 05 18:04:48 2021
 Response via : Initial Calibration

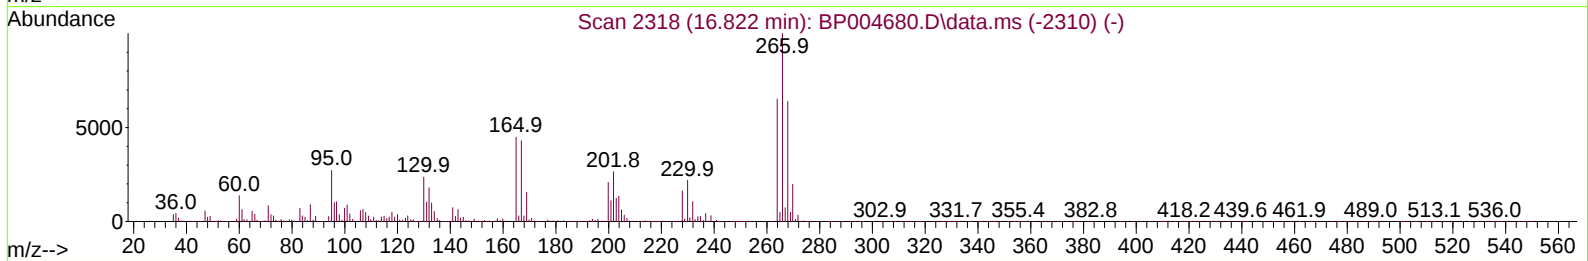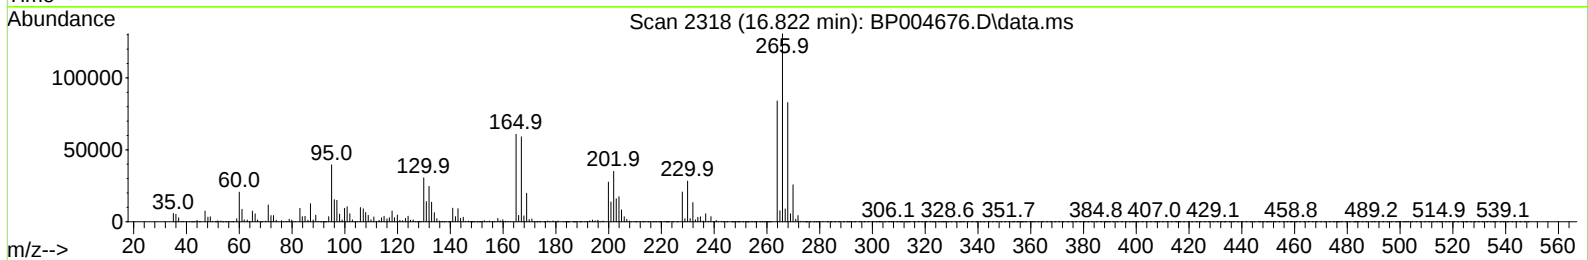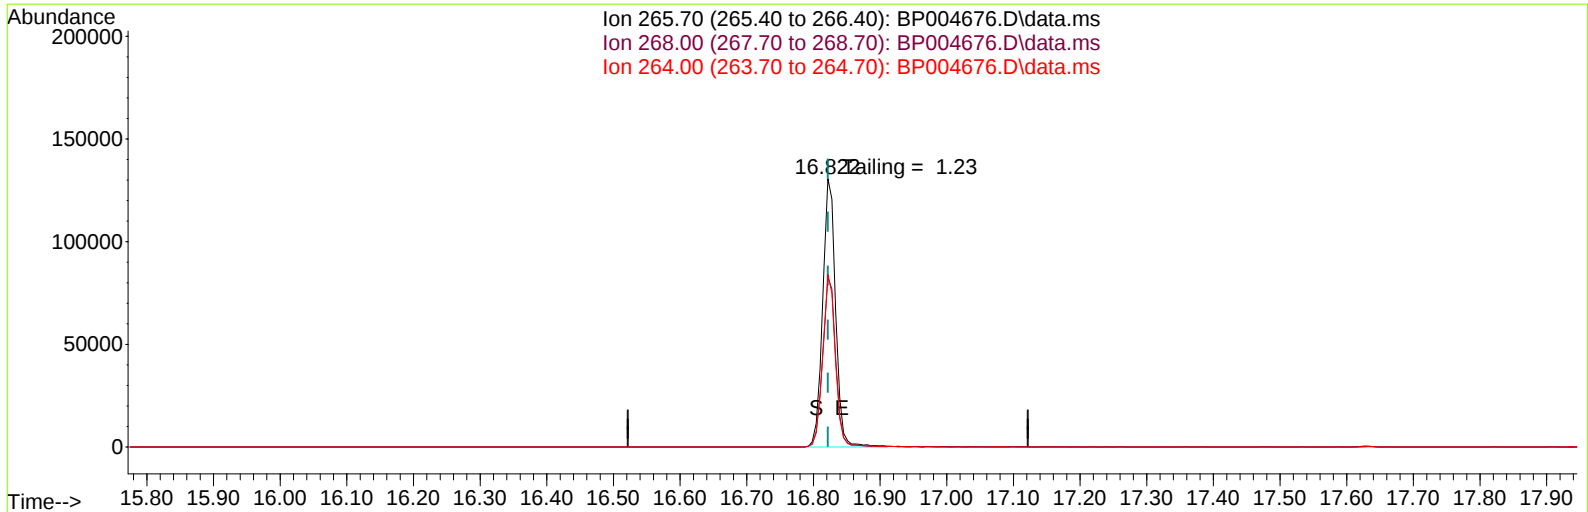

TIC: BP004676.D\data.ms

(70) Pentachlorophenol (C)

16.822min (-0.000) 644623.90 ng




response 177118

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	63.41
264.00	63.30	64.26
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020521\
Data File : BP004676.D
Acq On : 05 Feb 2021 12:58
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Feb 06 03:59:49 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270E-BP020521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 05 18:04:48 2021
Response via : Initial Calibration

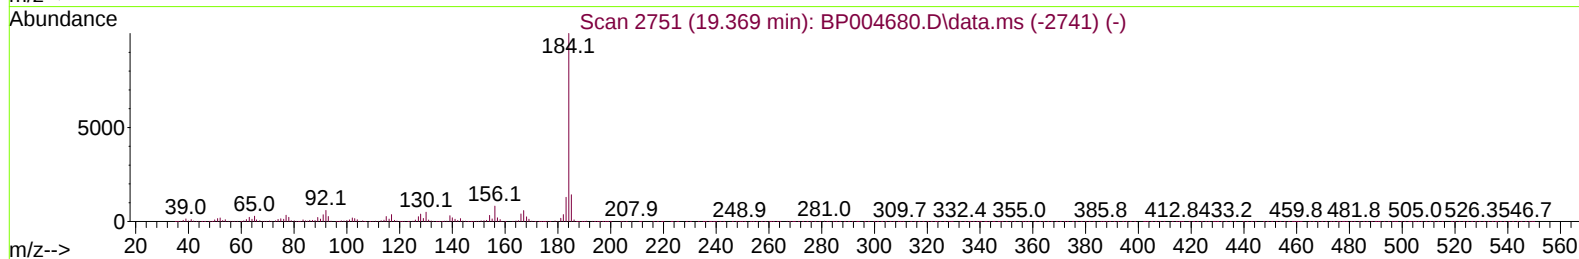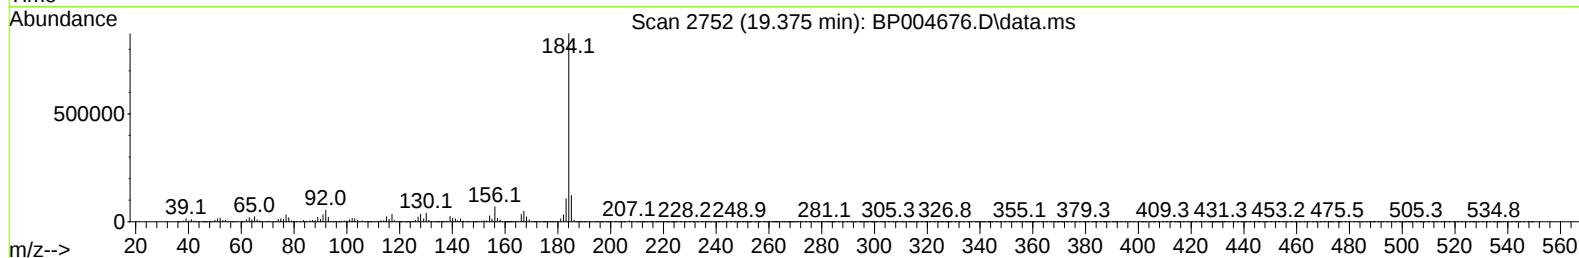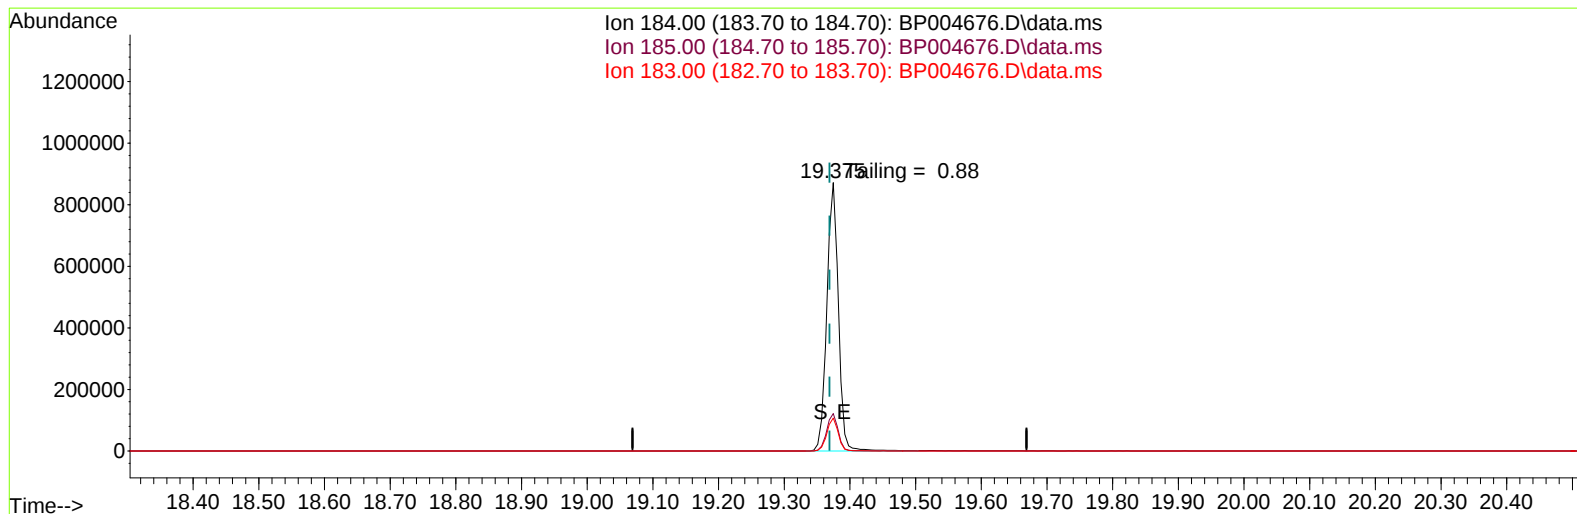

TIC: BP004676.D\data.ms

(77) Benzidine

19.375min (+ 0.006) 361193.39 ng

response 1061023

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.99
183.00	12.00	12.28
0.00	0.00	0.00