
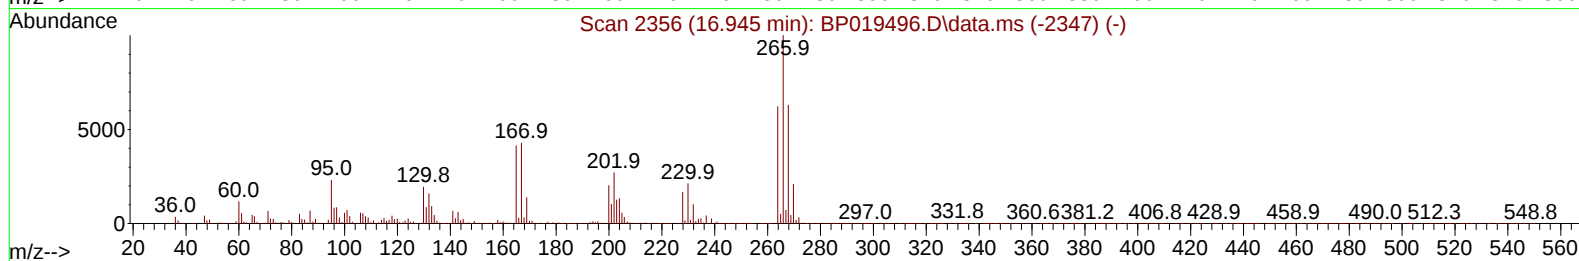
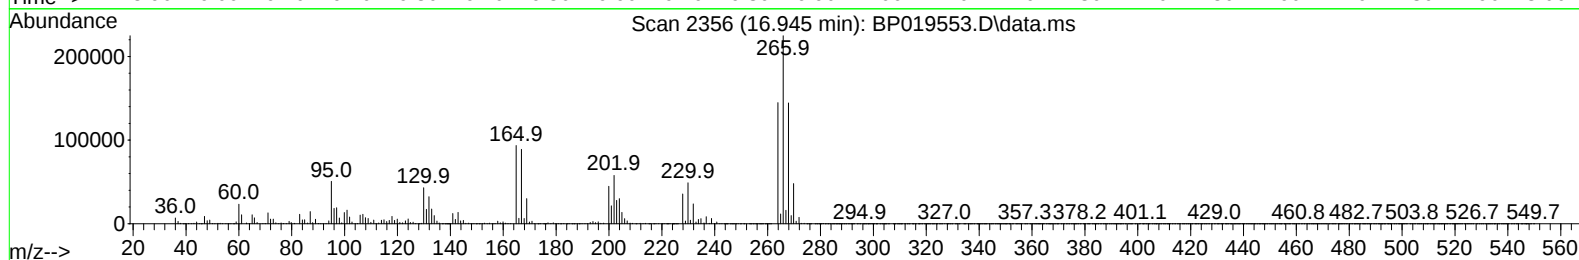


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020524\
Data File : BP019553.D
Acq On : 05 Feb 2024 09:31
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 06 18:49:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 01 00:51:48 2024
Response via : Initial Calibration

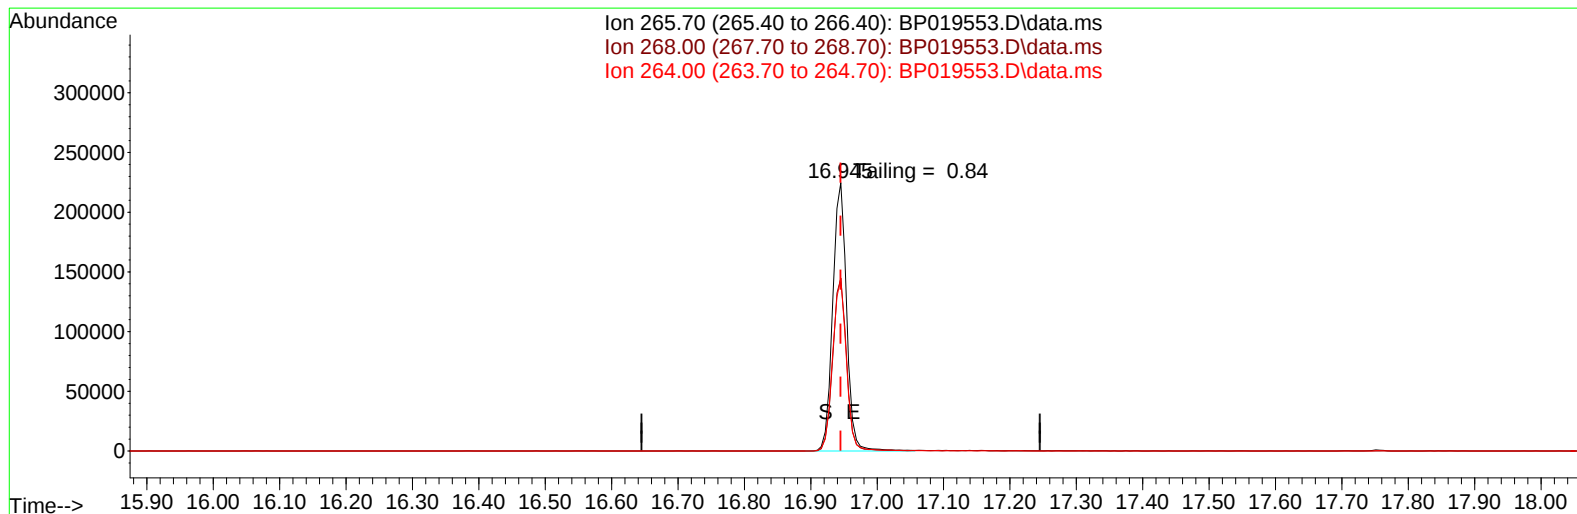

TIC: BP019553.D\data.ms

(70) Pentachlorophenol (C)




16.945min (+ 0.000) 304292.54 ng

response 326433

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	64.27
264.00	62.10	64.44
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020524\
Data File : BP019553.D
Acq On : 05 Feb 2024 09:31
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 06 18:49:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 01 00:51:48 2024
Response via : Initial Calibration

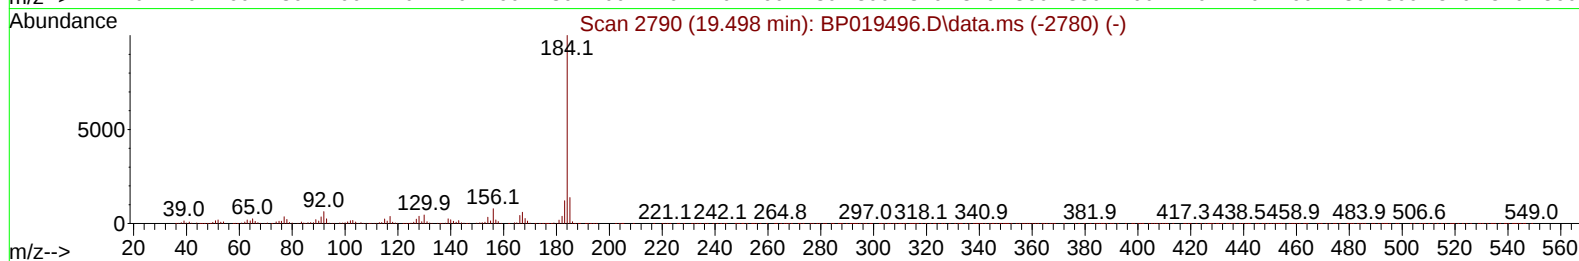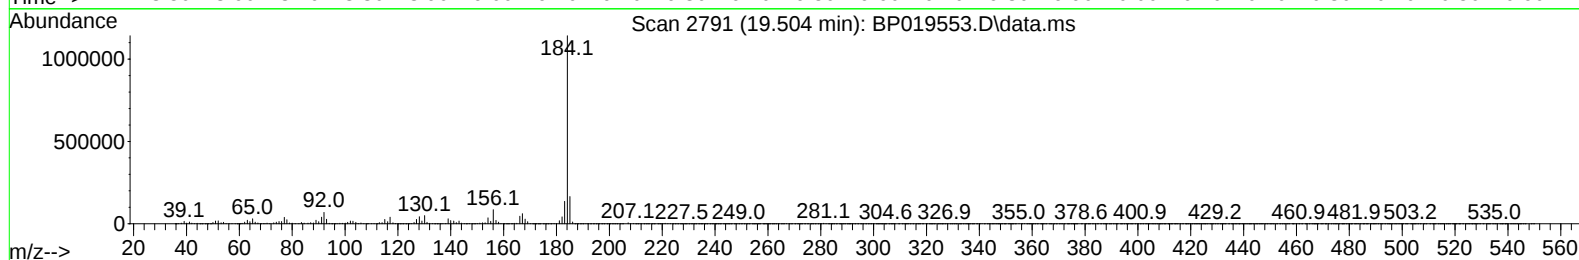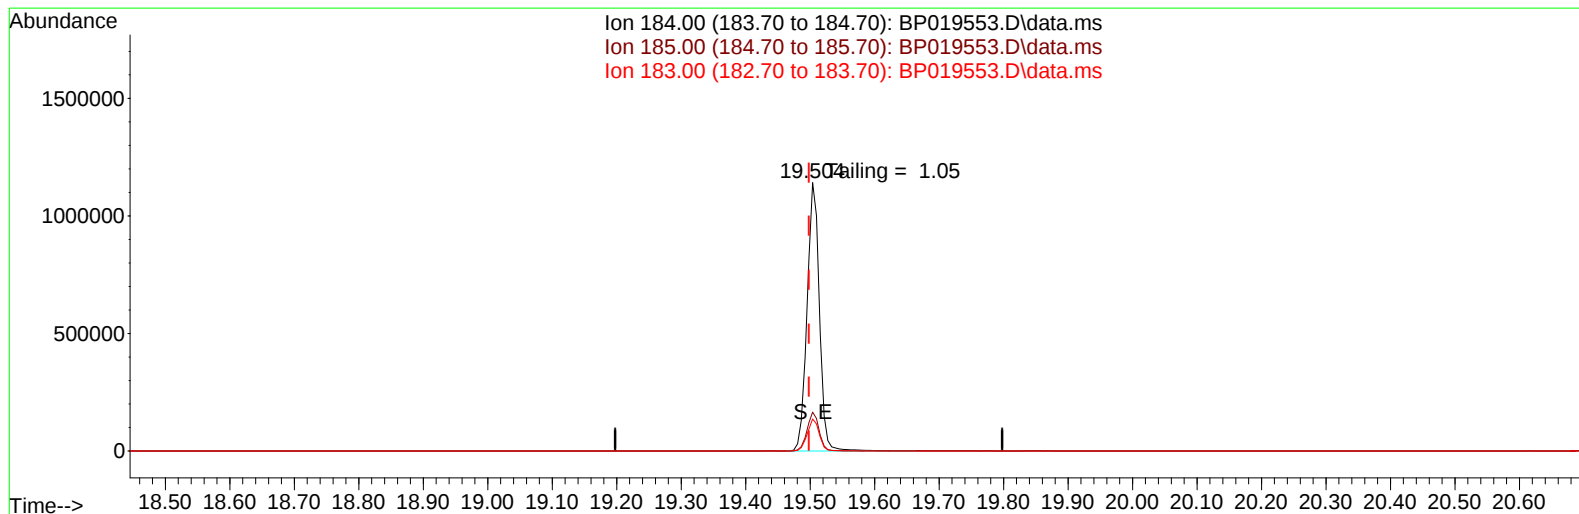

TIC: BP019553.D\data.ms

(77) Benzidine**19.504min (+ 0.006) 2105.64 ng****response 1523333**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.47
183.00	12.10	11.92
0.00	0.00	0.00