
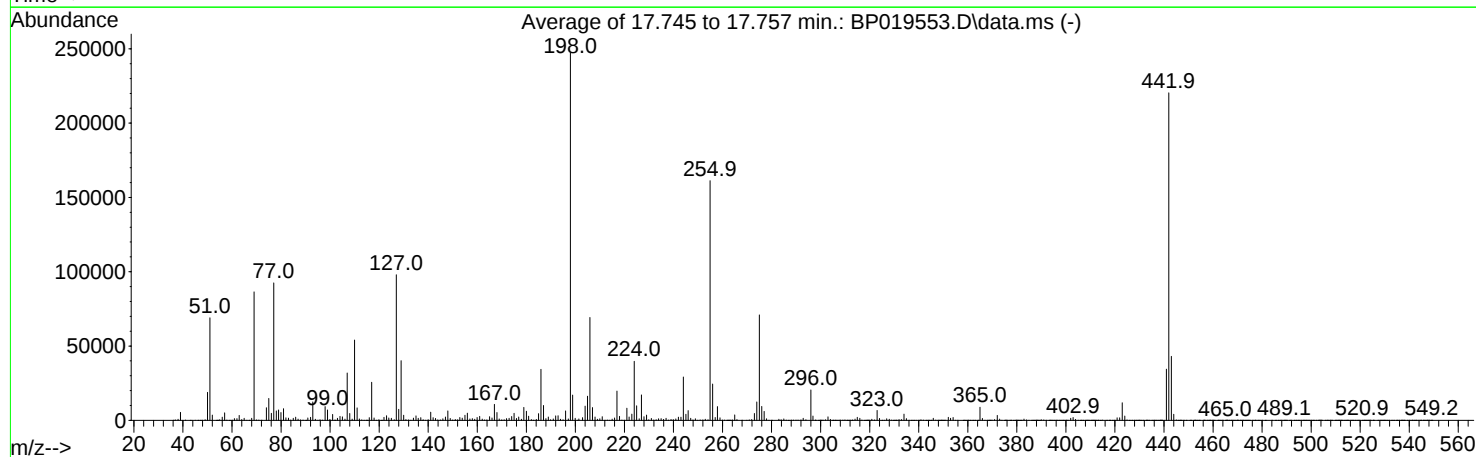


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020524\
Data File : BP019553.D
Acq On : 05 Feb 2024 09:31
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Feb 01 00:51:48 2024

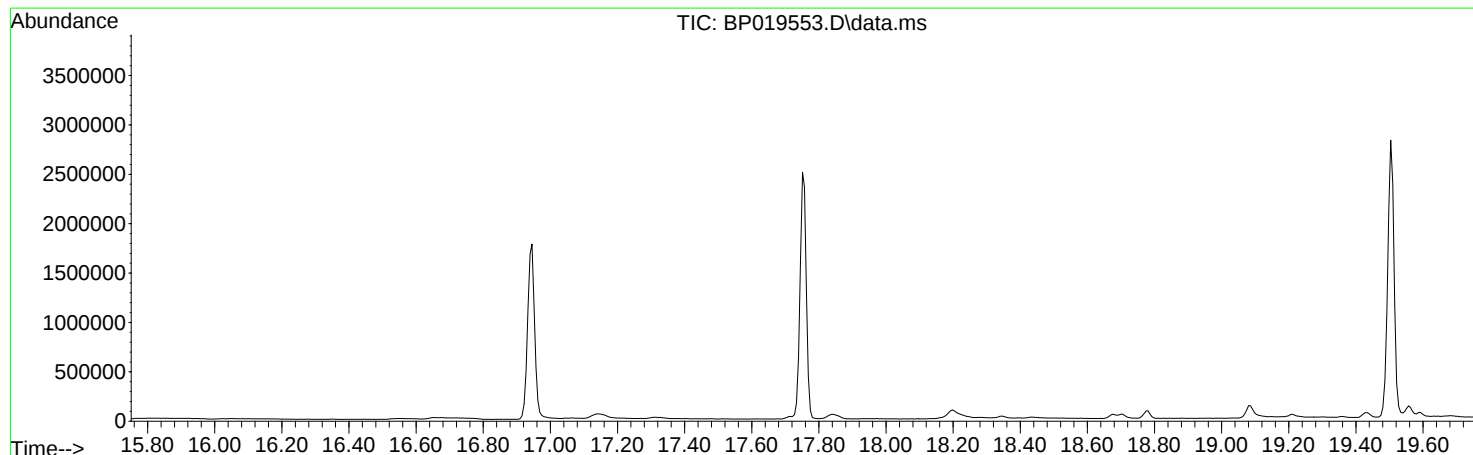




AutoFind: Scans 2492, 2493, 2494; Background Corrected with Scan 2485

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.9	68994	PASS
68	69	0.00	2	1.6	1397	PASS
69	198	0.00	100	34.9	86476	PASS
70	69	0.00	2	0.4	318	PASS
127	198	10	80	39.6	97985	PASS
197	198	0.00	2	0.4	956	PASS
198	198	100	100	100.0	247520	PASS
199	198	5	9	6.9	17057	PASS
275	198	10	60	28.7	70979	PASS
365	198	1	100	3.6	8822	PASS
441	198	0.01	100	13.9	34509	PASS
442	442	100	100	100.0	220427	PASS
443	442	15	24	19.5	43033	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020524\
Data File : BP019553.D
Acq On : 05 Feb 2024 09:31
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Feb 06 18:49:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 01 00:51:48 2024
Response via : Initial Calibration

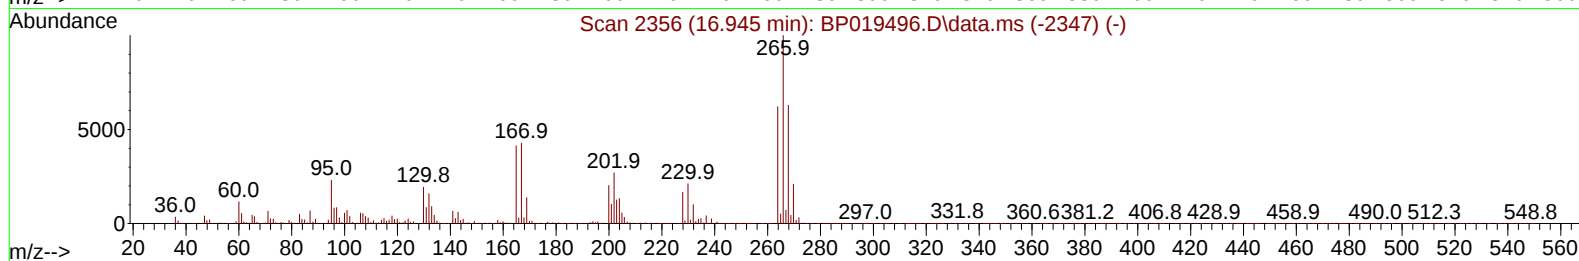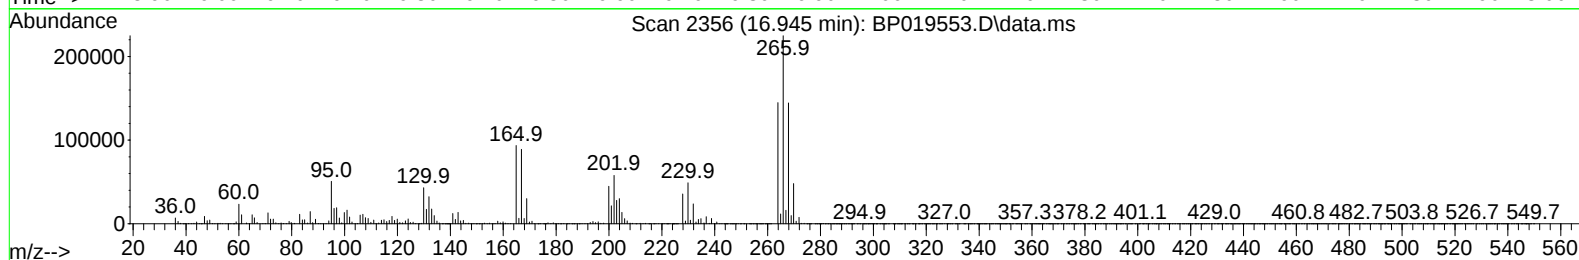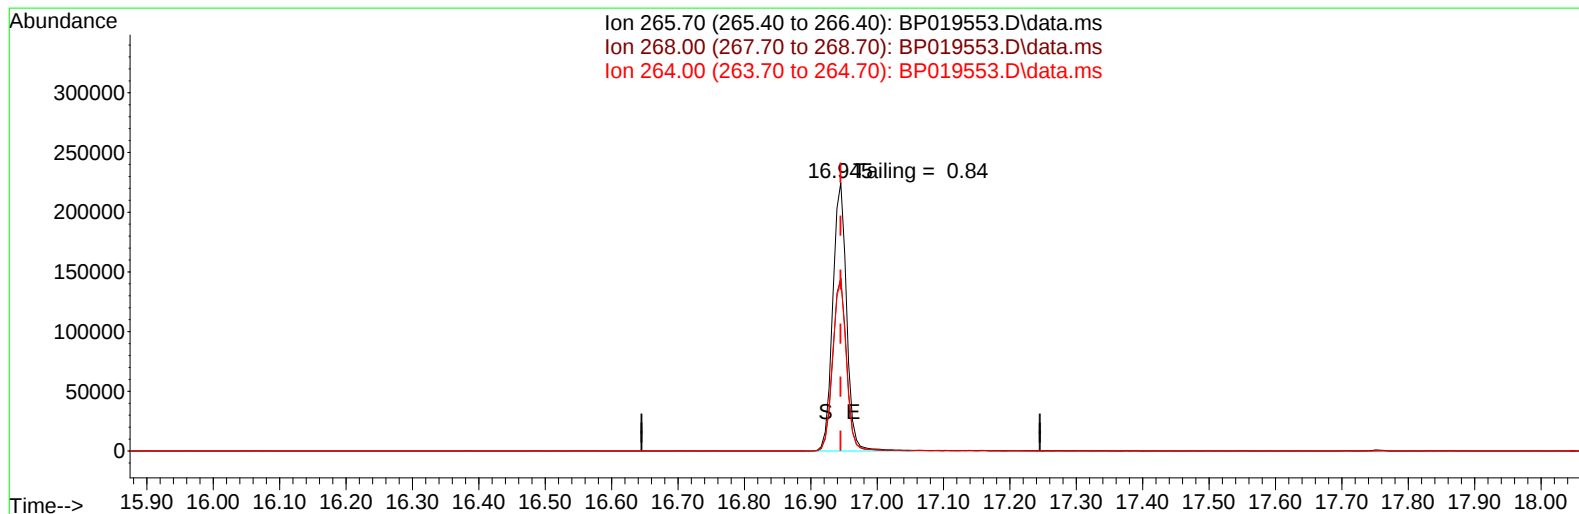

TIC: BP019553.D\data.ms

(70) Pentachlorophenol (C)

16.945min (+ 0.000) 304292.54 ng




response 326433

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	64.27
264.00	62.10	64.44
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020524\
Data File : BP019553.D
Acq On : 05 Feb 2024 09:31
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Feb 06 18:49:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 01 00:51:48 2024
Response via : Initial Calibration

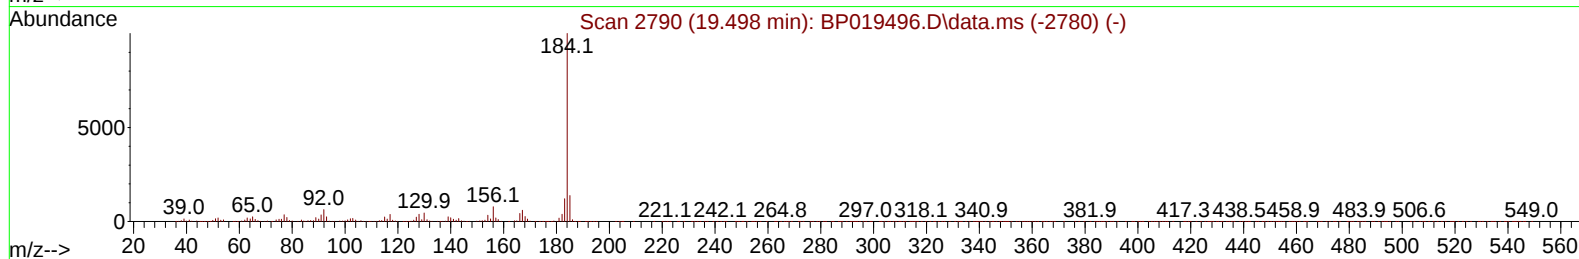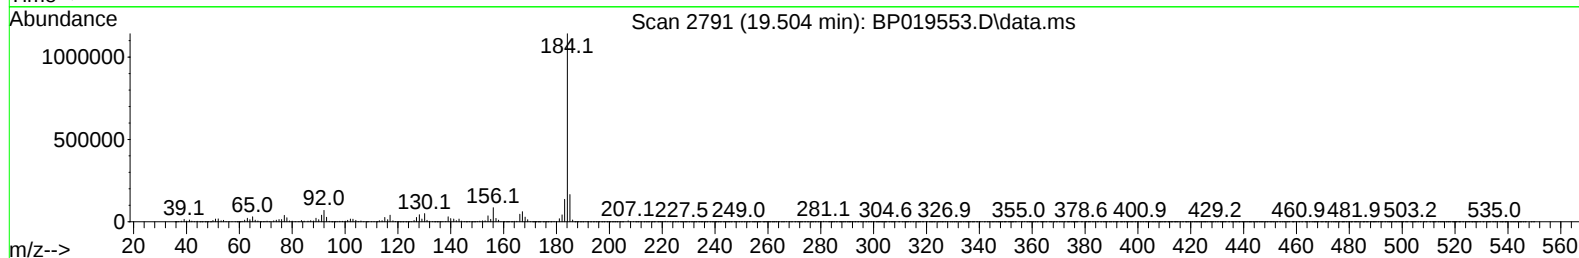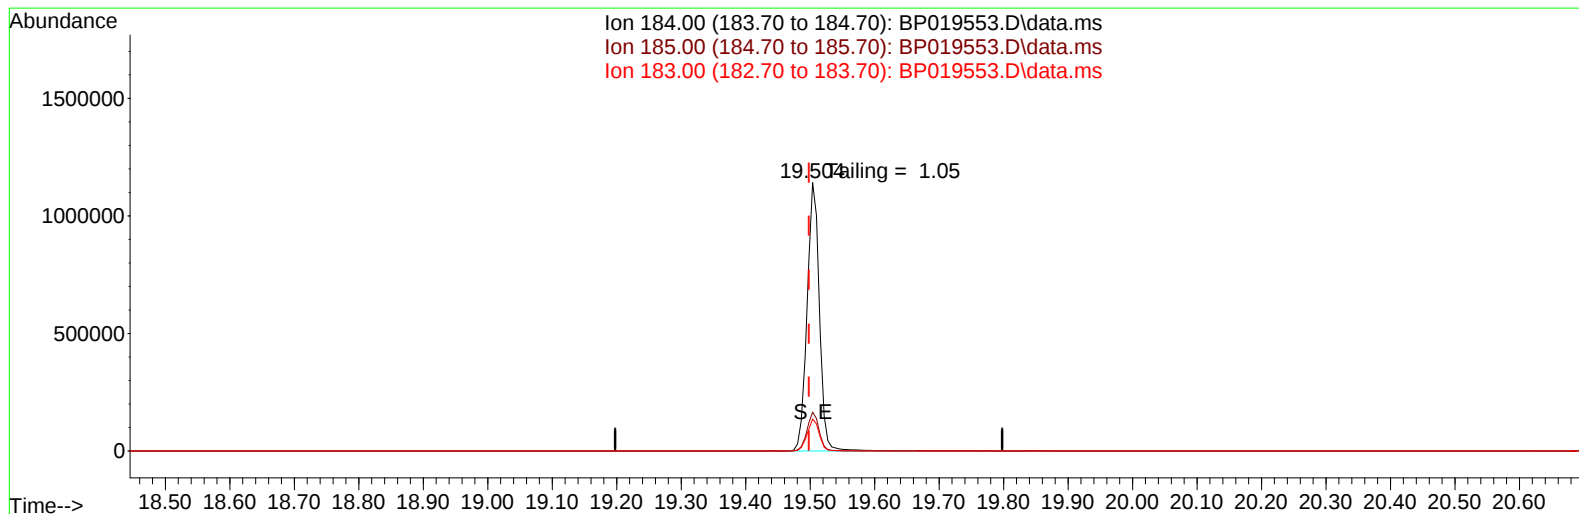

TIC: BP019553.D\data.ms

(77) Benzidine

19.504min (+ 0.006) 2105.64 ng

response 1523333

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.47
183.00	12.10	11.92
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/5/2024	BNA_P	<u>BP019553.D</u>
Compound Name	Response	Retention Time
DDT	961104	20.704
DDD	26802	20.274
DDE	2926	19.78
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
29728	990832	3.00

Instrument :
BNA_P
ClientSampleId :
DFTPP