

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020525\
 Data File : BP023940.D
 Acq On : 05 Feb 2025 17:45
 Operator : RC/JU
 Sample : Q1247-14
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A6341

Quant Time: Feb 06 07:33:35 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Feb 03 11:19:36 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.769	152	411437	20.000	ng/ul	0.00
20) Naphthalene-d8	10.546	136	1777857	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.393	164	1104258	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.186	188	2166397	20.000	ng/ul	0.00
79) Chrysene-d12	21.639	240	2017133	20.000	ng/ul	0.00
88) Perylene-d12	24.992	264	2061460	20.000	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.293	96	43824	4.426	ng/uL	0.00
4) Pyridine-d5	3.711	84	105803	3.703	ng/ul	0.00
7) Phenol-d5	6.952	99	250118	6.869	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.105	67	490160	25.433	ng/ul	0.00
11) 2-Chlorophenol-d4	7.311	132	649010	22.698	ng/ul	0.00
15) 4-Methylphenol-d8	8.469	113	477198	16.044	ng/ul	0.00
21) Nitrobenzene-d5	8.916	128	341055	23.977	ng/ul	0.00
24) 2-Nitrophenol-d4	9.628	143	340857	22.209	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.169	165	682143	24.227	ng/ul	0.00
31) 4-Chloroaniline-d4	10.675	131	259382	6.160	ng/ul	0.00
46) Dimethylphthalate-d6	13.798	166	2220873	26.963	ng/ul	0.00
49) Acenaphthylene-d8	14.081	160	2491697	26.822	ng/ul	0.00
54) 4-Nitrophenol-d4	14.604	143	77213	4.720	ng/ul	0.00
60) Fluorene-d10	15.398	176	1926107	27.769	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.510	200	223512	16.724	ng/ul	0.00
73) Anthracene-d10	17.281	188	2996157	28.167	ng/ul	0.00
81) Pyrene-d10	19.657	212	3566587	32.999	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.757	264	3157501	29.356	ng/ul	-0.02
Target Compounds						
					Qvalue	
8) Phenol	6.981	94	61618	1.648	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020525\
Data File : BP023940.D
Acq On : 05 Feb 2025 17:45
Operator : RC/JU
Sample : Q1247-14
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A6341

Quant Time: Feb 06 07:33:35 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Feb 03 11:19:36 2025
Response via : Initial Calibration

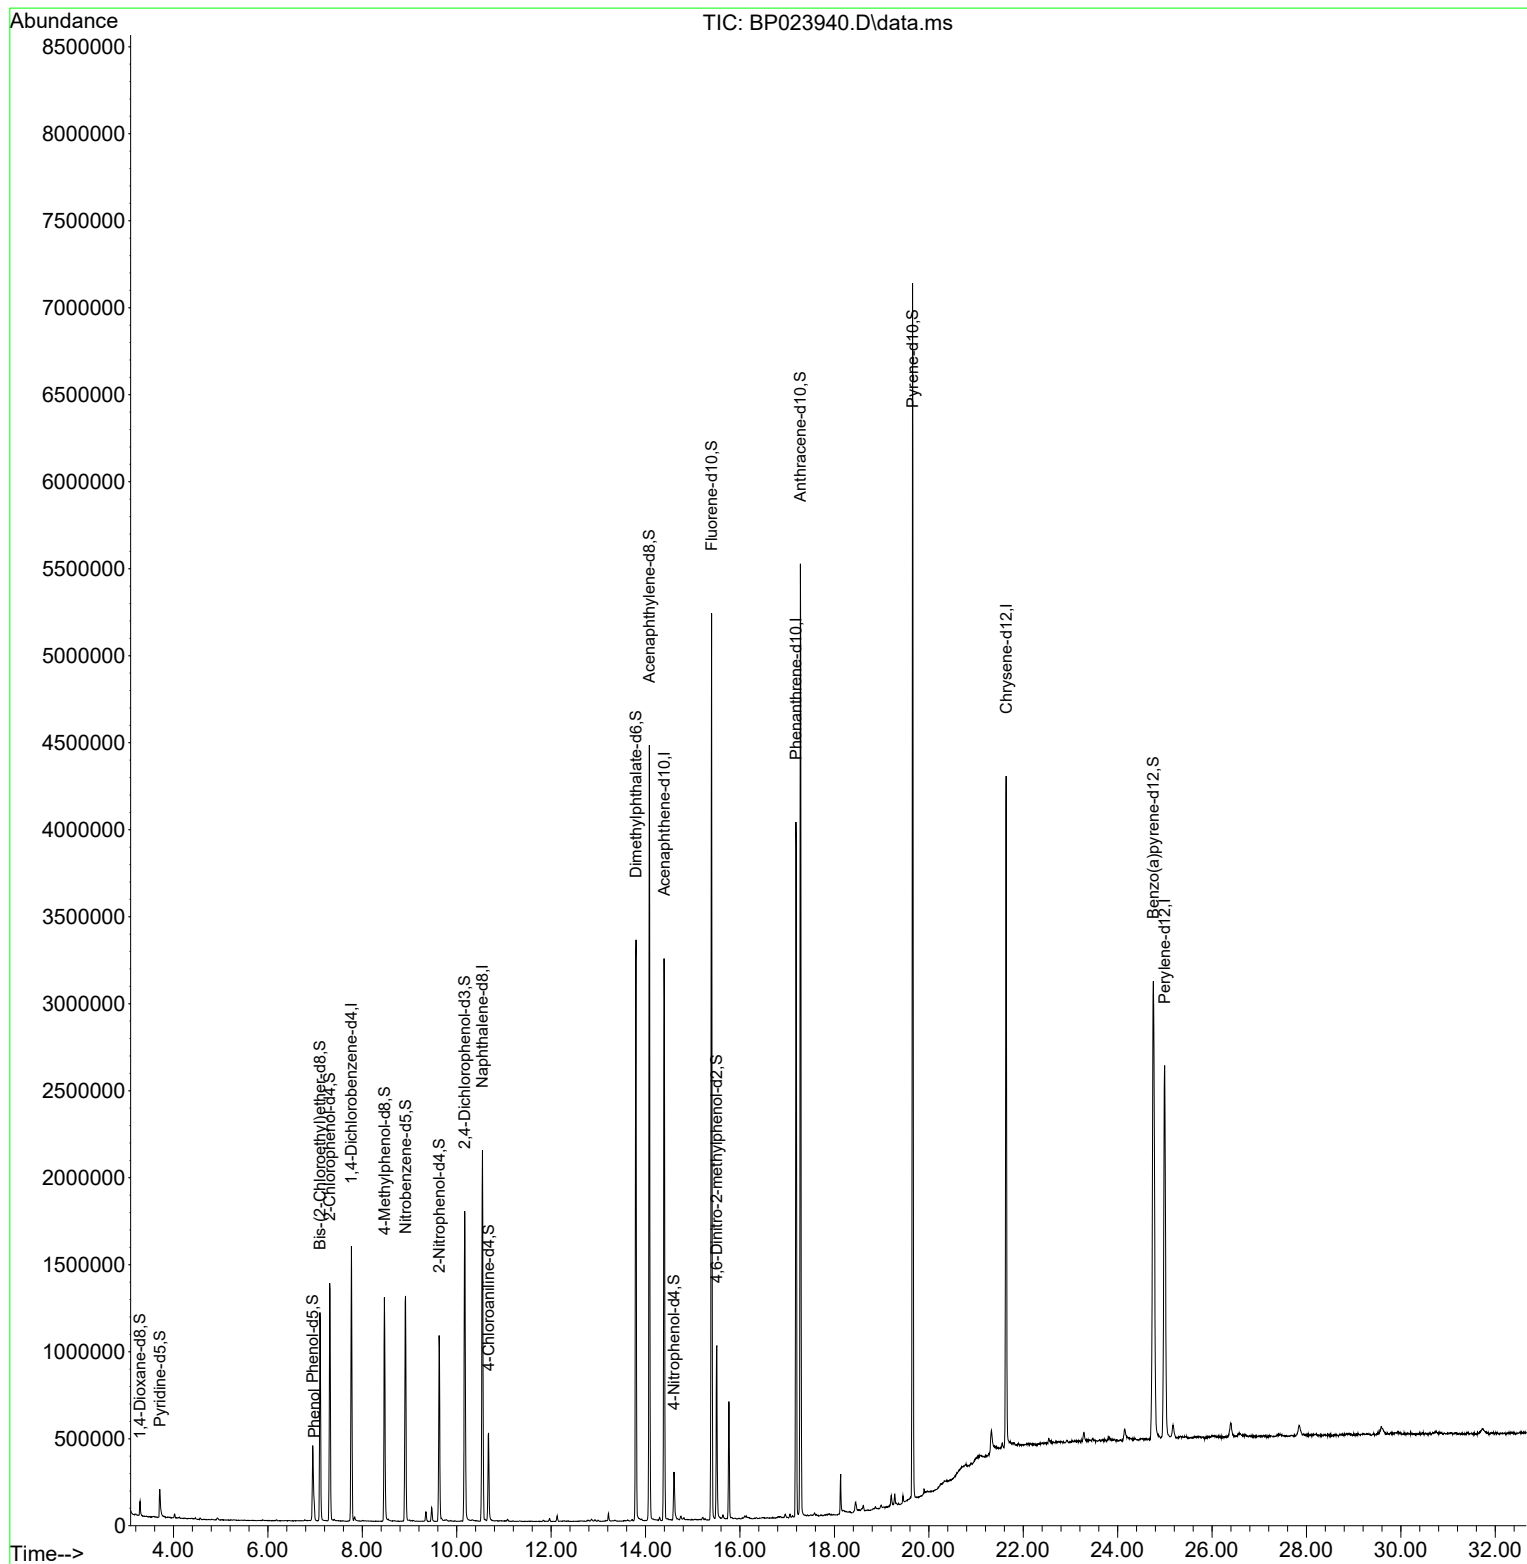

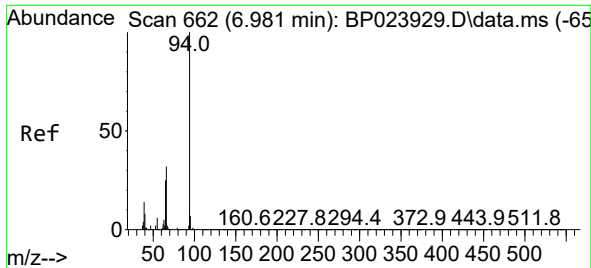

#8
Phenol
Concen: 1.648 ng/ul
RT: 6.981 min Scan# 60
Delta R.T. 0.000 min
Lab File: BP023940.D
Acq: 05 Feb 2025 17:45

Instrument :
BNA_P
ClientSampleId :
A6341

Tgt Ion: 94 Resp: 61618
Ion Ratio Lower Upper
94 100
65 28.2 20.1 30.1
66 32.8 26.0 39.0

