

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020525\
 Data File : BP023942.D
 Acq On : 05 Feb 2025 19:05
 Operator : RC/JU
 Sample : Q1247-11
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A6338

Quant Time: Feb 06 07:34:04 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Feb 03 11:19:36 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.769	152	415473	20.000	ng/ul	0.00
20) Naphthalene-d8	10.546	136	1839623	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.387	164	1143862	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.187	188	2163896	20.000	ng/ul	0.00
79) Chrysene-d12	21.616	240	1963986	20.000	ng/ul	-0.02
88) Perylene-d12	24.969	264	2013369	20.000	ng/ul	-0.04
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.293	96	48781	4.878	ng/uL	0.00
4) Pyridine-d5	3.717	84	34596	1.199	ng/ul	0.01
7) Phenol-d5	6.952	99	308517	8.391	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.105	67	573789	29.483	ng/ul	0.00
11) 2-Chlorophenol-d4	7.317	132	771503	26.720	ng/ul	0.00
15) 4-Methylphenol-d8	8.475	113	548939	18.276	ng/ul	0.00
21) Nitrobenzene-d5	8.916	128	405636	27.560	ng/ul	0.00
24) 2-Nitrophenol-d4	9.628	143	411540	25.914	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.169	165	807830	27.728	ng/ul	0.00
31) 4-Chloroaniline-d4	10.675	131	341631	7.841	ng/ul	0.00
46) Dimethylphthalate-d6	13.793	166	2446445	28.673	ng/ul	0.00
49) Acenaphthylene-d8	14.075	160	2801408	29.112	ng/ul	0.00
54) 4-Nitrophenol-d4	14.604	143	89711	5.294	ng/ul	0.00
60) Fluorene-d10	15.393	176	2176767	30.296	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.510	200	253716	19.006	ng/ul	0.00
73) Anthracene-d10	17.287	188	3090002	29.083	ng/ul	0.00
81) Pyrene-d10	19.663	212	3609318	34.298	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.745	264	3075802	29.280	ng/ul	-0.03
Target Compounds						
					Qvalue	
8) Phenol	6.981	94	69878	1.851	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020525\
Data File : BP023942.D
Acq On : 05 Feb 2025 19:05
Operator : RC/JU
Sample : Q1247-11
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A6338

Quant Time: Feb 06 07:34:04 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Feb 03 11:19:36 2025
Response via : Initial Calibration

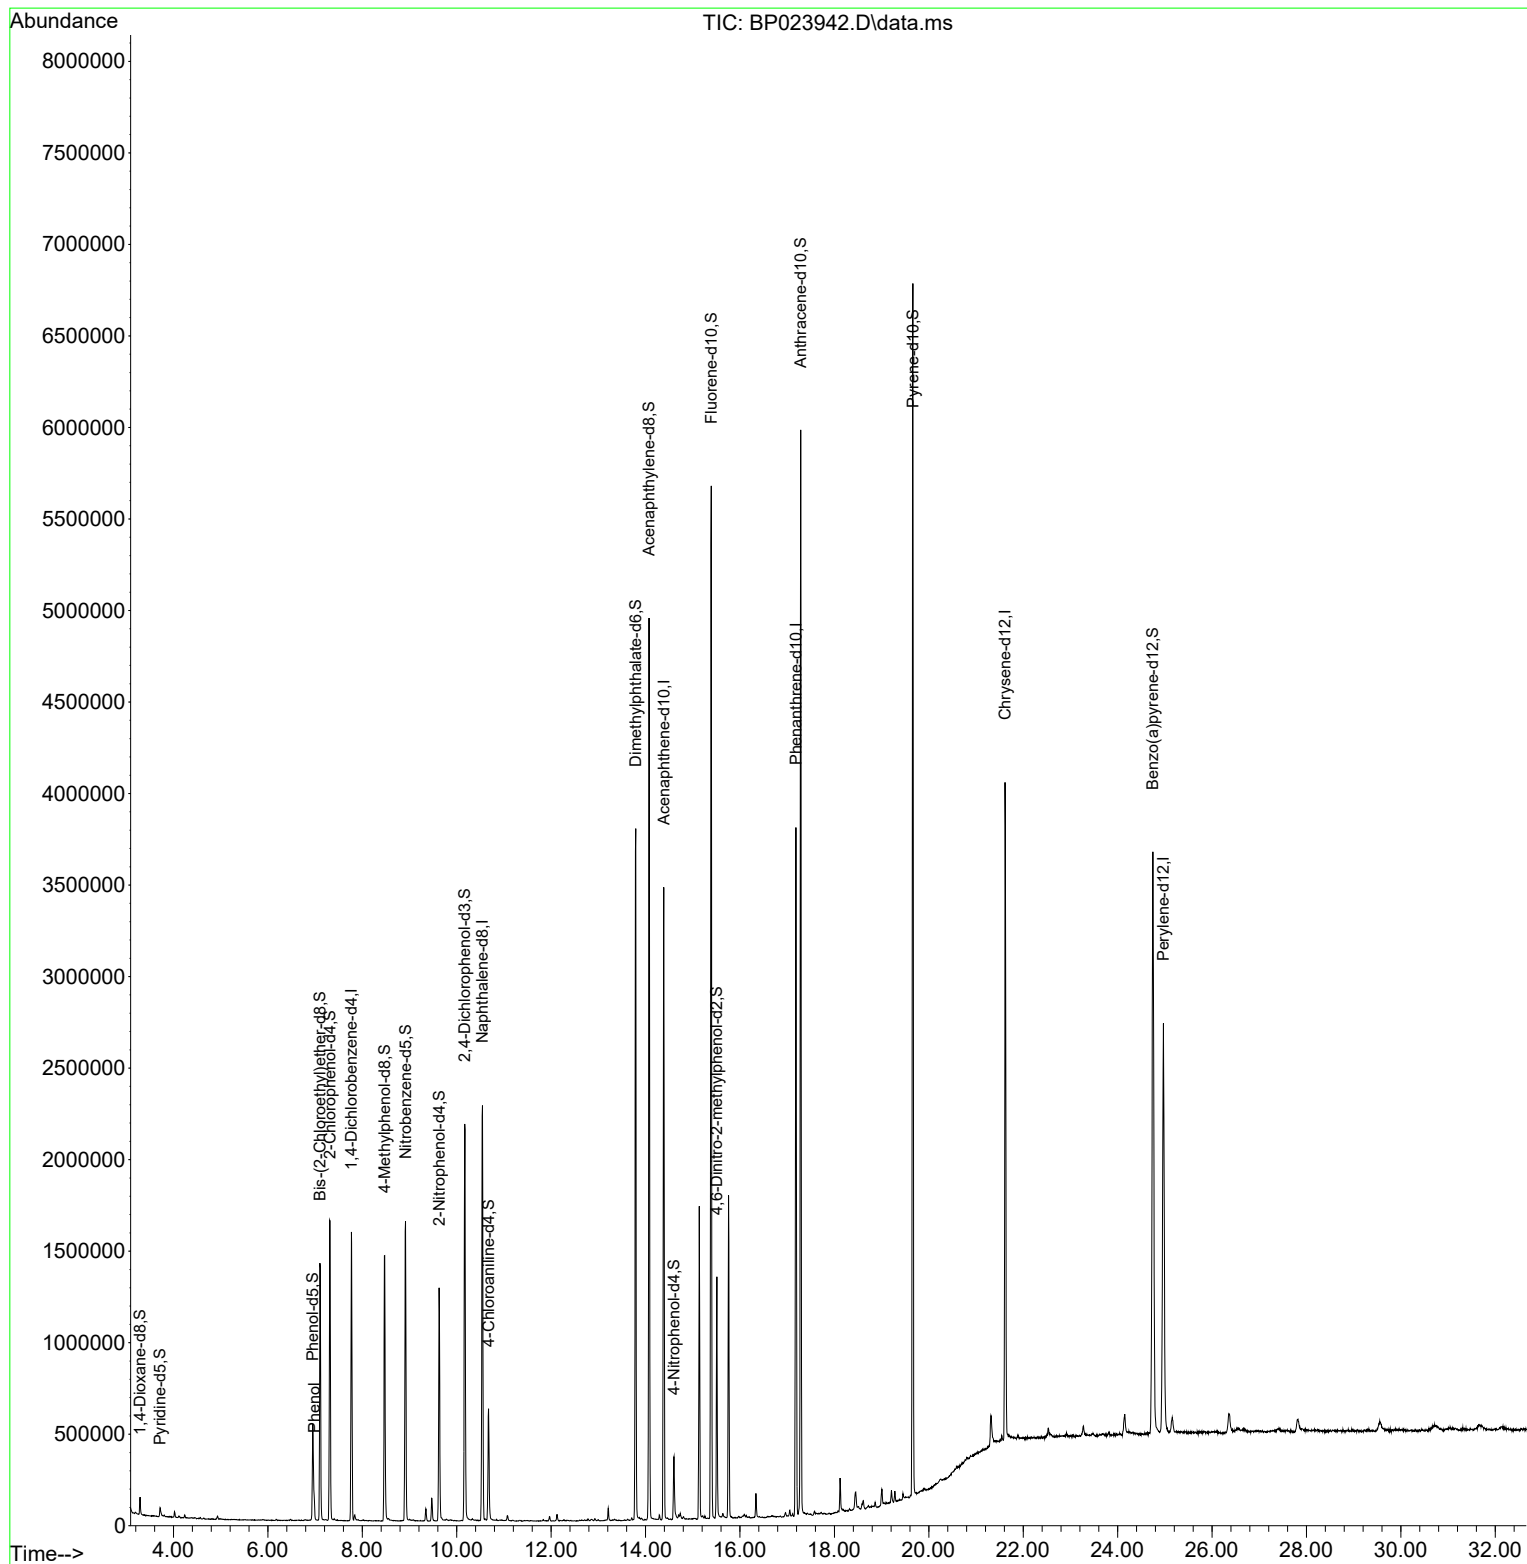

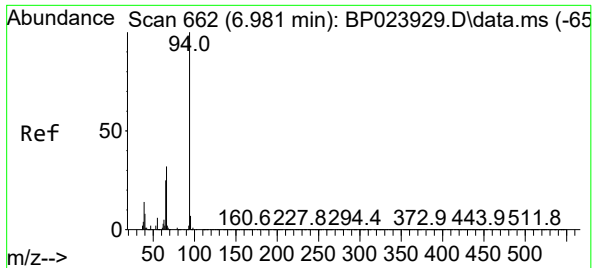

#8
Phenol
Concen: 1.851 ng/ul
RT: 6.981 min Scan# 60
Delta R.T. 0.000 min
Lab File: BP023942.D
Acq: 05 Feb 2025 19:05

Instrument :
BNA_P
ClientSampleId :
A6338

Tgt Ion: 94 Resp: 69878
Ion Ratio Lower Upper
94 100
65 26.3 20.1 30.1
66 34.6 26.0 39.0

