

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020525\
 Data File : BP023943.D
 Acq On : 05 Feb 2025 19:46
 Operator : RC/JU
 Sample : Q1247-12
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A6339

Quant Time: Feb 06 07:34:18 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Feb 03 11:19:36 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.775	152	435024	20.000	ng/ul	0.00
20) Naphthalene-d8	10.546	136	1895804	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.393	164	1211572	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.175	188	2364902	20.000	ng/ul	-0.01
79) Chrysene-d12	21.616	240	2266708	20.000	ng/ul	-0.02
88) Perylene-d12	24.968	264	2334097	20.000	ng/ul	-0.04
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.293	96	43753	4.179	ng/uL	0.00
4) Pyridine-d5	3.711	84	235896	7.808	ng/ul	0.00
7) Phenol-d5	6.952	99	256720	6.668	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.105	67	404849	19.867	ng/ul	0.00
11) 2-Chlorophenol-d4	7.311	132	579557	19.170	ng/ul	0.00
15) 4-Methylphenol-d8	8.469	113	473558	15.058	ng/ul	0.00
21) Nitrobenzene-d5	8.916	128	268713	17.716	ng/ul	0.00
24) 2-Nitrophenol-d4	9.634	143	273457	16.709	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.169	165	568430	18.933	ng/ul	0.00
31) 4-Chloroaniline-d4	10.675	131	906804	20.196	ng/ul	0.00
46) Dimethylphthalate-d6	13.793	166	1736059	19.210	ng/ul	0.00
49) Acenaphthylene-d8	14.081	160	1926855	18.905	ng/ul	0.00
54) 4-Nitrophenol-d4	14.604	143	84905	4.731	ng/ul	0.00
60) Fluorene-d10	15.393	176	1516105	19.922	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.510	200	167268	11.465	ng/ul	0.00
73) Anthracene-d10	17.275	188	2210914	19.040	ng/ul	-0.01
81) Pyrene-d10	19.651	212	2722387	22.415	ng/ul	-0.01
92) Benzo(a)pyrene-d12	24.745	264	2480278	20.366	ng/ul	-0.03
Target Compounds						
					Qvalue	
8) Phenol	6.975	94	70212	1.776	ng/ul	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020525\
Data File : BP023943.D
Acq On : 05 Feb 2025 19:46
Operator : RC/JU
Sample : Q1247-12
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A6339

Quant Time: Feb 06 07:34:18 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Feb 03 11:19:36 2025
Response via : Initial Calibration

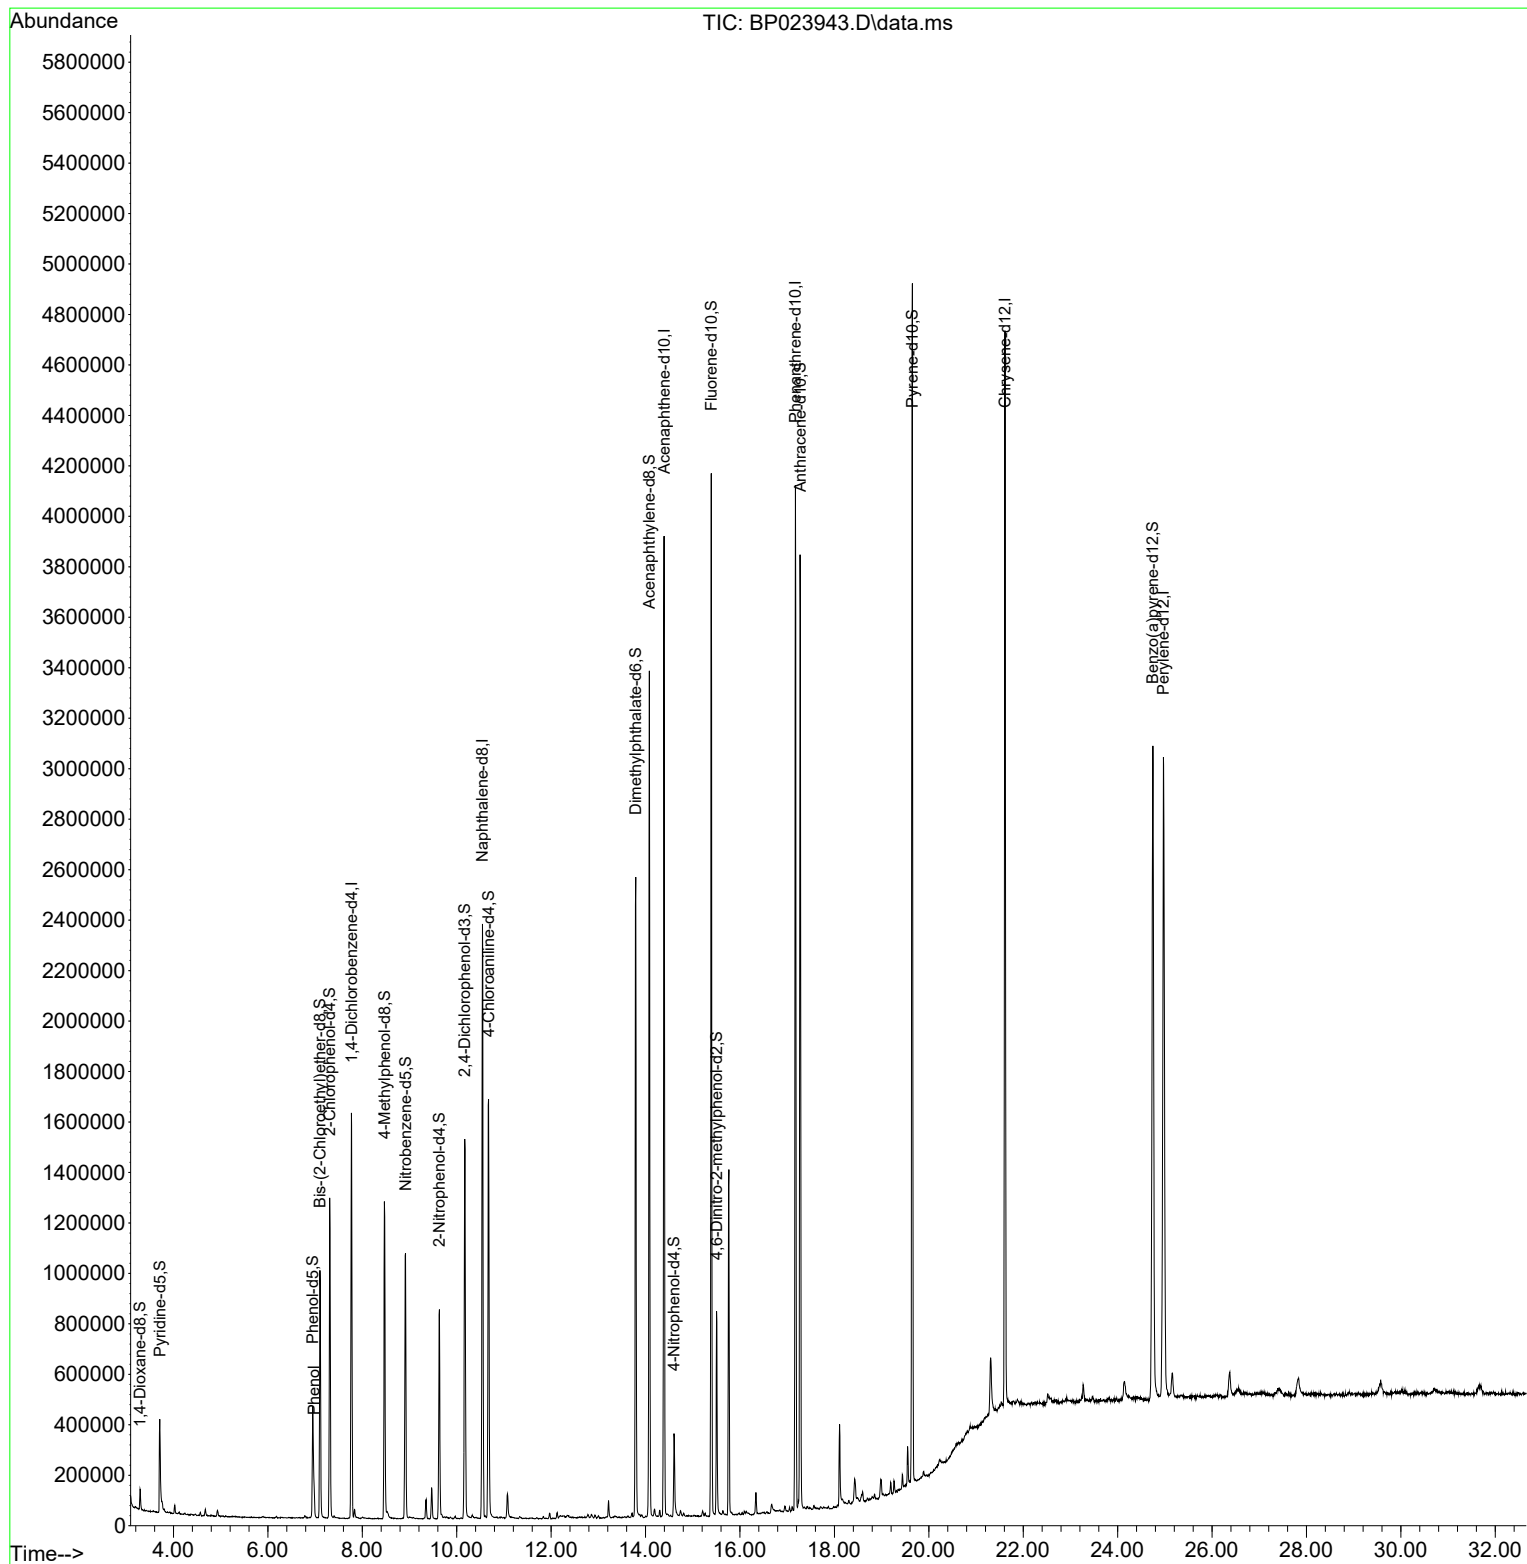

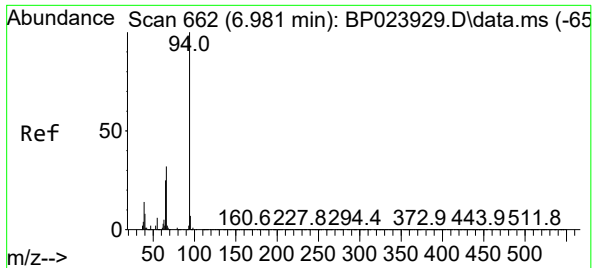

#8
Phenol
Concen: 1.776 ng/ul
RT: 6.975 min Scan# 60
Delta R.T. -0.006 min
Lab File: BP023943.D
Acq: 05 Feb 2025 19:46

Instrument :
BNA_P
ClientSampleId :
A6339

Tgt Ion:	94	Resp:	70212
Ion	Ratio	Lower	Upper
94	100		
65	29.4	20.1	30.1
66	35.3	26.0	39.0

