

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020525\
 Data File : BP023946.D
 Acq On : 05 Feb 2025 21:47
 Operator : RC/JU
 Sample : Q1247-13
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A6340

Quant Time: Feb 06 07:35:00 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Feb 03 11:19:36 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.769	152	433589	20.000	ng/ul	0.00
20) Naphthalene-d8	10.546	136	1896645	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.393	164	1183686	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.181	188	2266049	20.000	ng/ul	0.00
79) Chrysene-d12	21.604	240	2081965	20.000	ng/ul	-0.04
88) Perylene-d12	24.963	264	2110355	20.000	ng/ul	-0.05
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.293	96	53840	5.159	ng/uL	0.00
4) Pyridine-d5	3.705	84	219202	7.279	ng/ul	0.00
7) Phenol-d5	6.952	99	319515	8.327	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.105	67	588720	28.986	ng/ul	0.00
11) 2-Chlorophenol-d4	7.311	132	784673	26.041	ng/ul	0.00
15) 4-Methylphenol-d8	8.475	113	600910	19.171	ng/ul	0.00
21) Nitrobenzene-d5	8.911	128	408229	26.903	ng/ul	0.00
24) 2-Nitrophenol-d4	9.634	143	444408	27.142	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.169	165	843429	28.079	ng/ul	0.00
31) 4-Chloroaniline-d4	10.675	131	663792	14.777	ng/ul	0.00
46) Dimethylphthalate-d6	13.798	166	2615176	29.620	ng/ul	0.00
49) Acenaphthylene-d8	14.081	160	2976758	29.893	ng/ul	0.00
54) 4-Nitrophenol-d4	14.604	143	98899	5.640	ng/ul	0.00
60) Fluorene-d10	15.398	176	2317784	31.173	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.510	200	281444	20.132	ng/ul	0.00
73) Anthracene-d10	17.281	188	3400106	30.559	ng/ul	0.00
81) Pyrene-d10	19.645	212	4080284	36.576	ng/ul	-0.02
92) Benzo(a)pyrene-d12	24.739	264	3493929	31.732	ng/ul	-0.04
Target Compounds						
					Qvalue	
8) Phenol	6.981	94	117782	2.989	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020525\
Data File : BP023946.D
Acq On : 05 Feb 2025 21:47
Operator : RC/JU
Sample : Q1247-13
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A6340

Quant Time: Feb 06 07:35:00 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Feb 03 11:19:36 2025
Response via : Initial Calibration

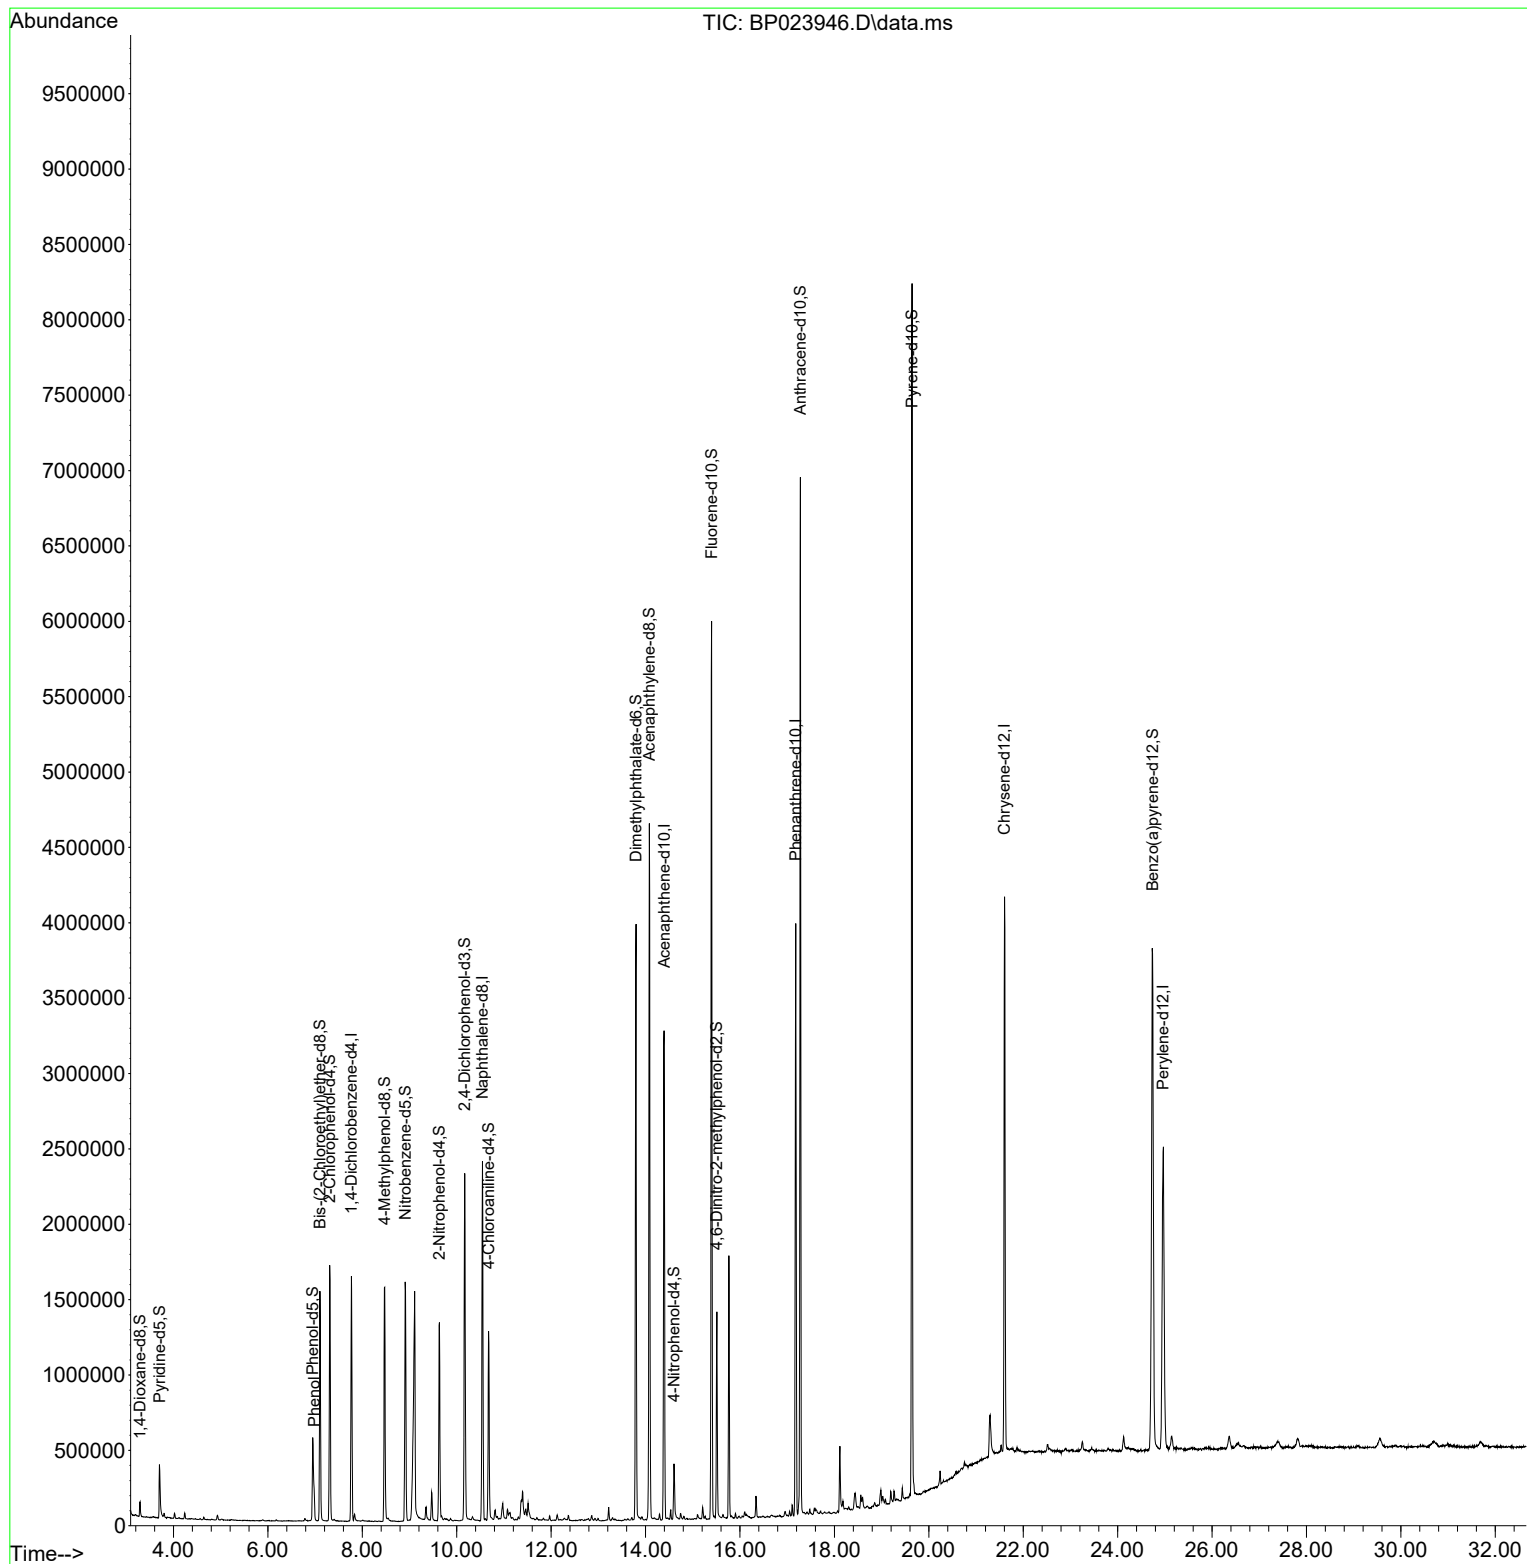

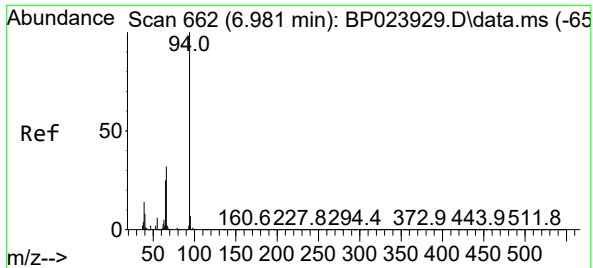

#8
Phenol
Concen: 2.989 ng/ul
RT: 6.981 min Scan# 60
Delta R.T. 0.000 min
Lab File: BP023946.D
Acq: 05 Feb 2025 21:47

Instrument :
BNA_P
ClientSampleId :
A6340

Tgt Ion: 94 Resp: 117782
Ion Ratio Lower Upper
94 100
65 25.9 20.1 30.1
66 32.4 26.0 39.0

