

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020525\
 Data File : BP023992.D
 Acq On : 07 Feb 2025 06:12
 Operator : RC/JU
 Sample : Q1226-25
 Misc :
 ALS Vial : 67 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCZN7

Quant Time: Feb 07 07:36:17 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Feb 03 11:19:36 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.769	152	493807	20.000	ng/ul	0.00
20) Naphthalene-d8	10.540	136	2135541	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.387	164	1324621	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.181	188	2600029	20.000	ng/ul	0.00
79) Chrysene-d12	21.616	240	2483884	20.000	ng/ul	-0.02
88) Perylene-d12	24.986	264	2613788	20.000	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.293	96	65198	5.486	ng/uL	0.00
4) Pyridine-d5	3.705	84	235883	6.878	ng/ul	0.00
7) Phenol-d5	6.952	99	410650	9.397	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.105	67	854228	36.930	ng/ul	0.00
11) 2-Chlorophenol-d4	7.311	132	1134999	33.074	ng/ul	0.00
15) 4-Methylphenol-d8	8.469	113	799397	22.393	ng/ul	0.00
21) Nitrobenzene-d5	8.910	128	626701	36.680	ng/ul	0.00
24) 2-Nitrophenol-d4	9.622	143	669304	36.304	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.169	165	1246256	36.849	ng/ul	0.00
31) 4-Chloroaniline-d4	10.675	131	1143796	22.614	ng/ul	0.00
46) Dimethylphthalate-d6	13.793	166	3876447	39.234	ng/ul	0.00
49) Acenaphthylene-d8	14.081	160	4403363	39.515	ng/ul	0.00
54) 4-Nitrophenol-d4	14.616	143	160781	8.194	ng/ul	0.00
60) Fluorene-d10	15.392	176	3383704	40.667	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.510	200	514098	32.051	ng/ul	0.00
73) Anthracene-d10	17.286	188	5384327	42.177	ng/ul	0.00
81) Pyrene-d10	19.651	212	6113805	45.937	ng/ul	-0.01
92) Benzo(a)pyrene-d12	24.757	264	6064005	44.466	ng/ul	-0.02
Target Compounds						Qvalue
58) 2,3,4,6-Tetrachlorophenol	15.022	232	49758	2.074	ng/ul#	91
71) Pentachlorophenol	16.828	266	509441	23.303	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020525\
Data File : BP023992.D
Acq On : 07 Feb 2025 06:12
Operator : RC/JU
Sample : Q1226-25
Misc :
ALS Vial : 67 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCZN7

Quant Time: Feb 07 07:36:17 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Feb 03 11:19:36 2025
Response via : Initial Calibration




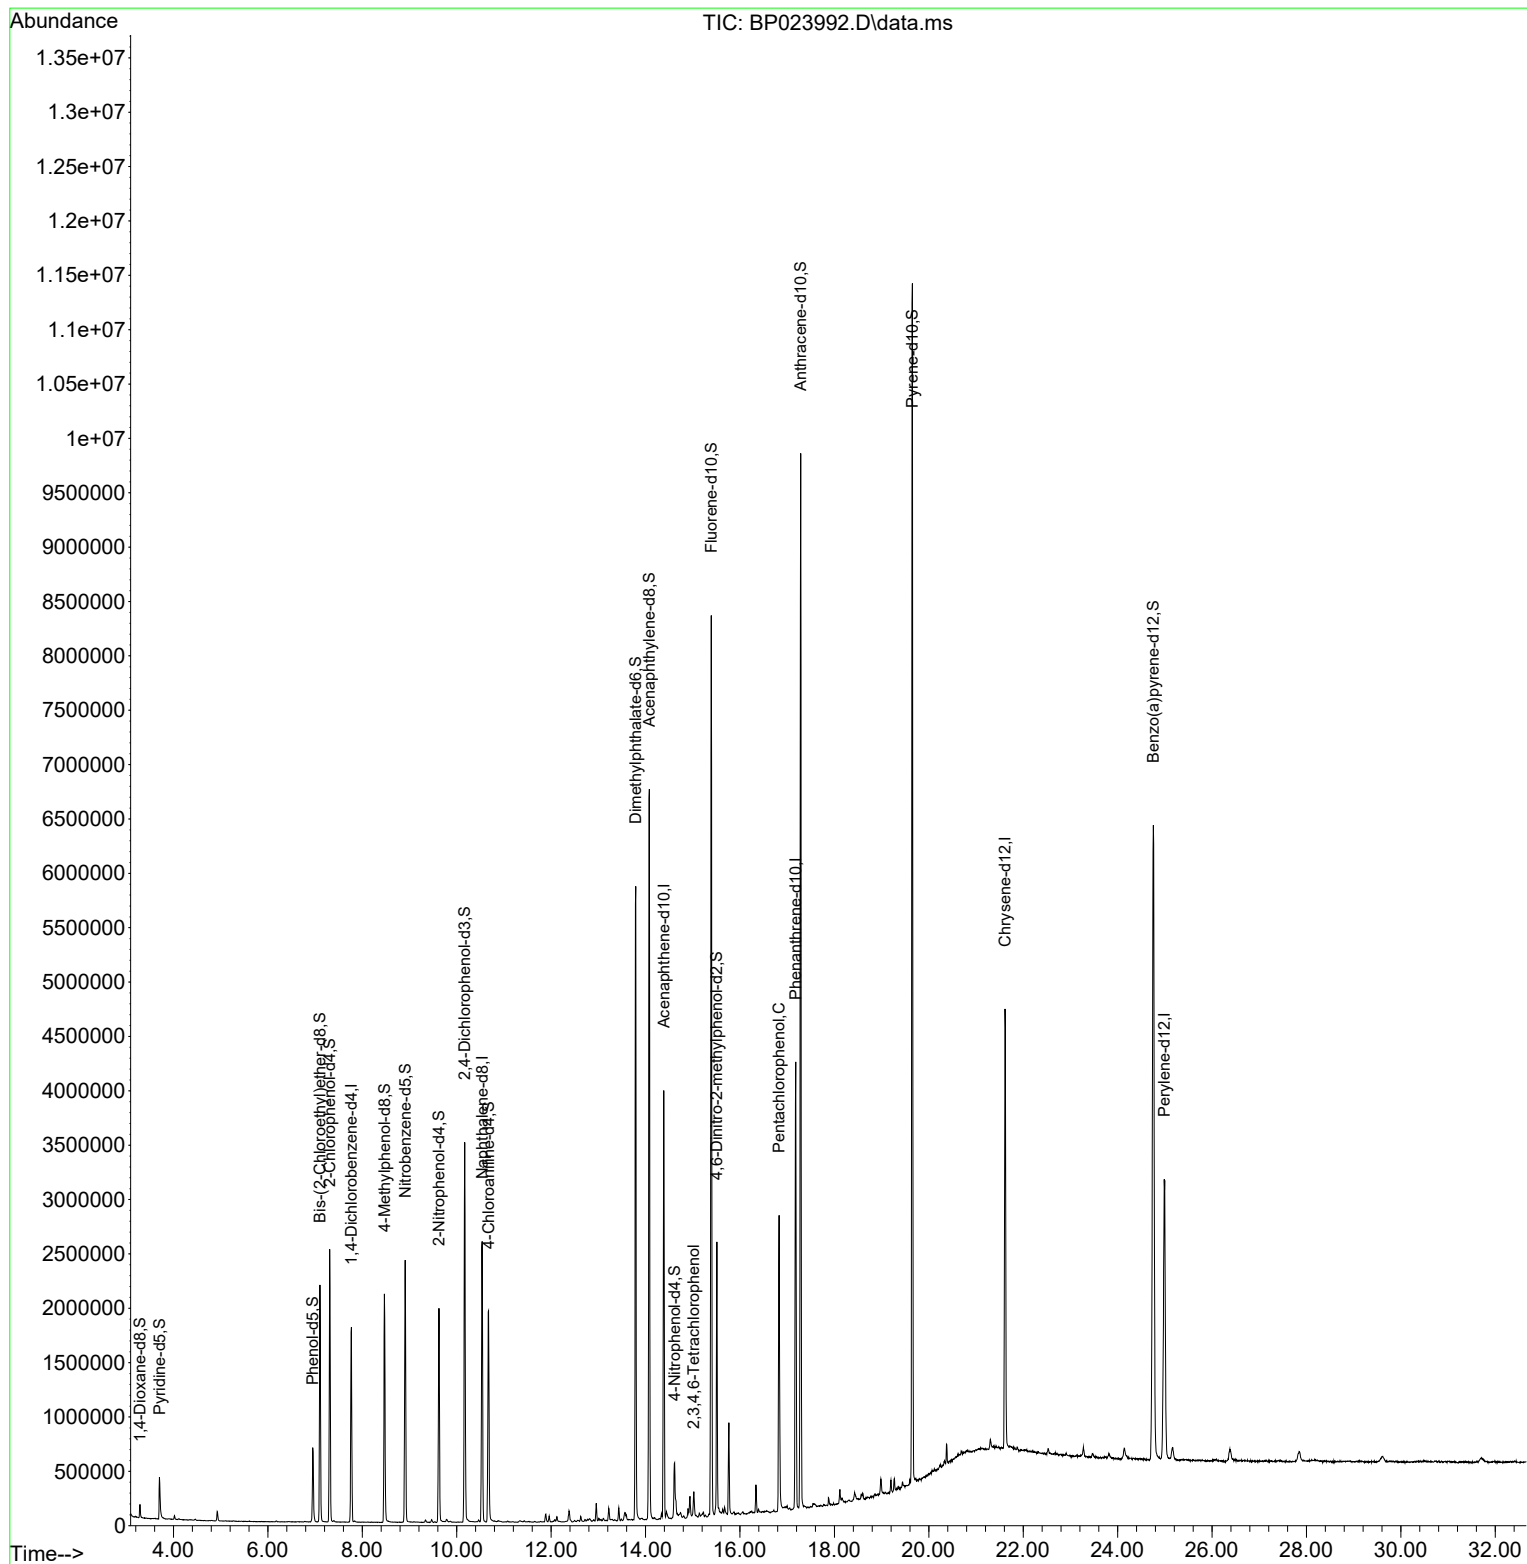


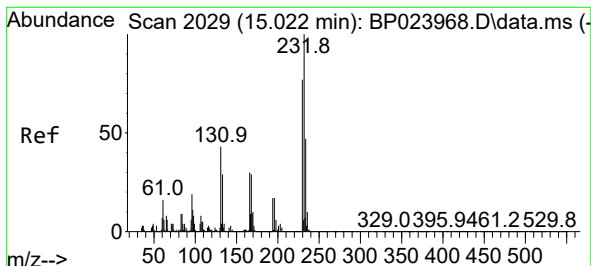

#58
2,3,4,6-Tetrachlorophenol
Concen: 2.074 ng/ul
RT: 15.022 min Scan# 2029
Delta R.T. 0.000 min
Lab File: BP023992.D
Acq: 07 Feb 2025 06:12

Instrument :
BNA_P
ClientSampleId :
DCZN7

Tgt Ion:232	Resp:	49758
Ion Ratio	Lower	Upper
232	100	
131	47.4	32.4 48.6
130	3.6	1.7 2.5#
166	31.6	23.0 34.4

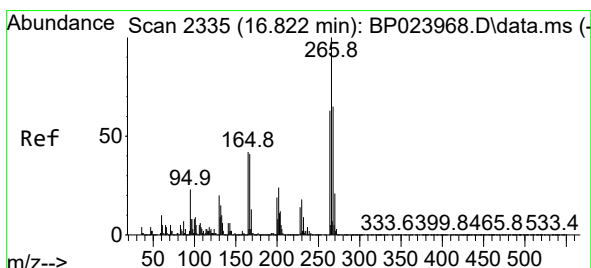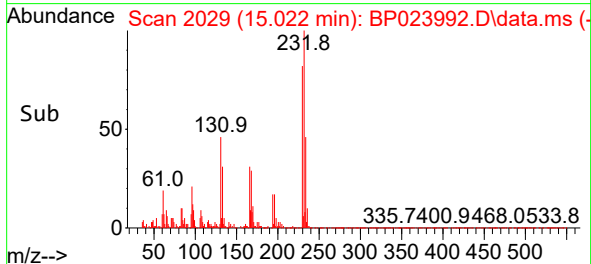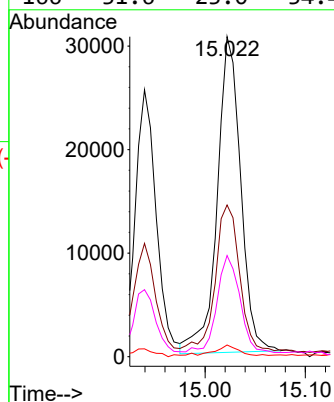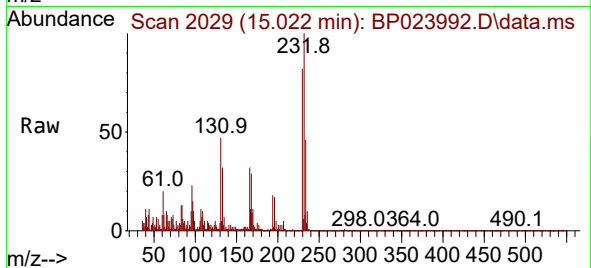

#71
Pentachlorophenol
Concen: 23.303 ng/ul
RT: 16.828 min Scan# 2336
Delta R.T. 0.000 min
Lab File: BP023992.D
Acq: 07 Feb 2025 06:12

Tgt Ion:266	Resp:	509441
Ion Ratio	Lower	Upper
266	100	
264	63.0	50.8 76.2
268	63.4	51.1 76.7

