




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020525\
Data File : BP023987.D
Acq On : 07 Feb 2025 02:49
Operator : RC/JU
Sample : Q1229-11
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E29B5

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 02/07/2025
Supervised By :Sohil Jodhani 02/10/2025

Quant Time: Feb 07 07:35:02 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Feb 03 11:19:36 2025
Response via : Initial Calibration

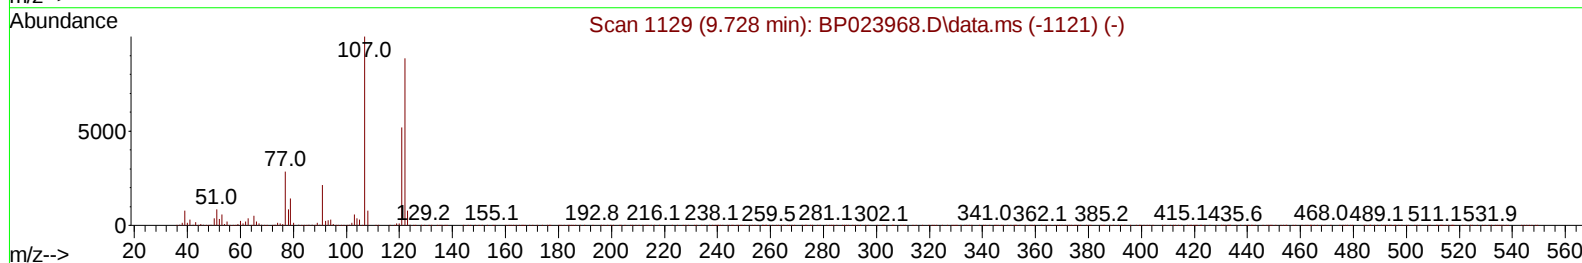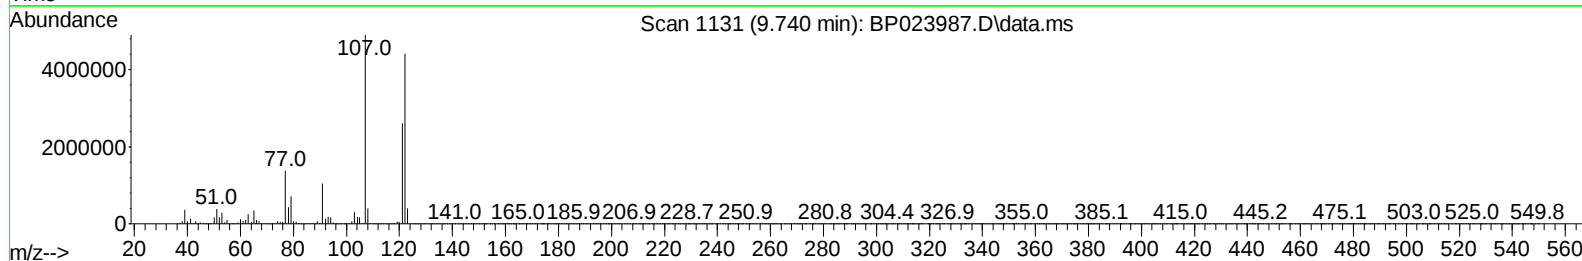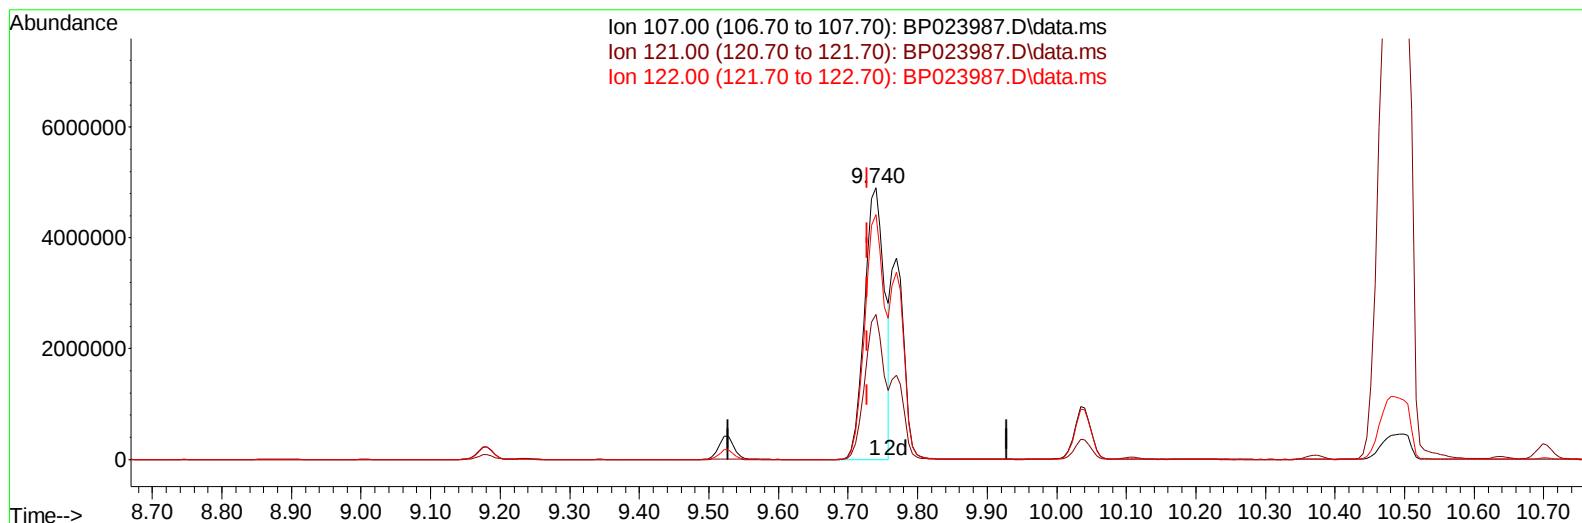

TIC: BP023987.D\data.ms

(26) 2,4-Dimethylphenol

9.740min (+ 0.012) 272.99 ng/u1

response 9850979

Ion	Exp%	Act%
107.00	100.00	100.00
121.00	51.80	53.38
122.00	89.40	90.24
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020525\
Data File : BP023987.D
Acq On : 07 Feb 2025 02:49
Operator : RC/JU
Sample : Q1229-11
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E29B5

Manual IntegrationsAPPROVED

Quant Time: Feb 07 07:35:02 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Feb 03 11:19:36 2025
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/07/2025
Supervised By :Sohil Jodhani 02/10/2025

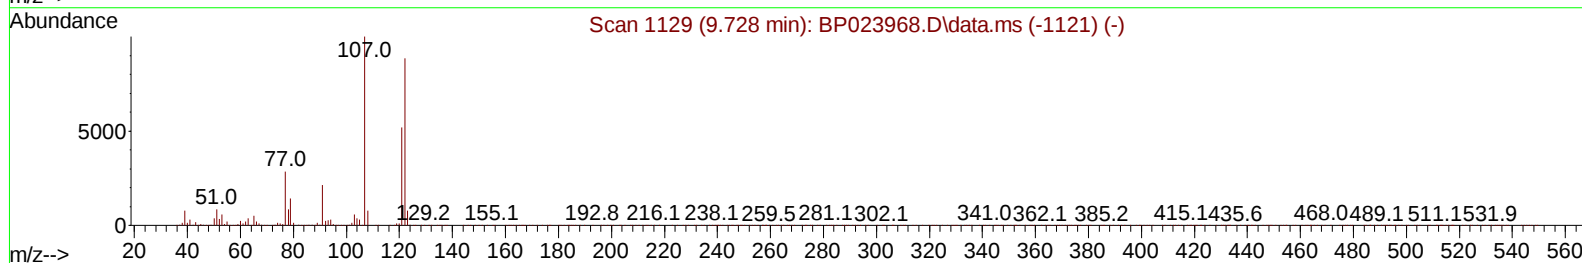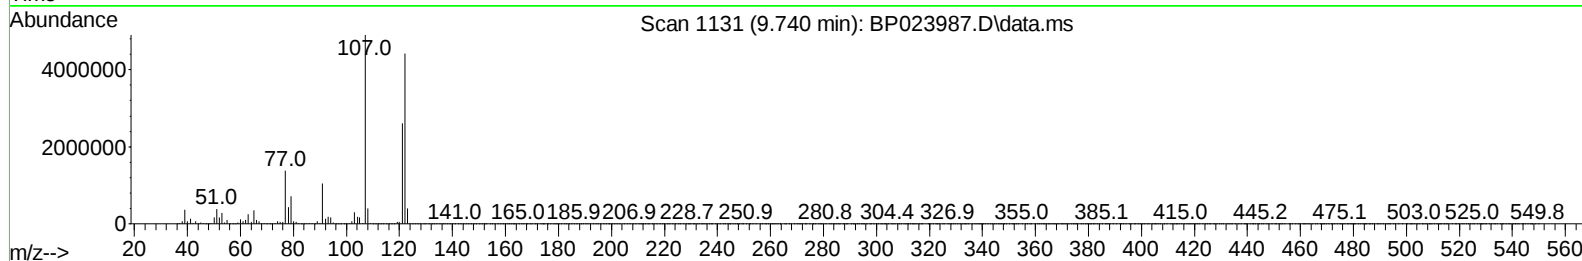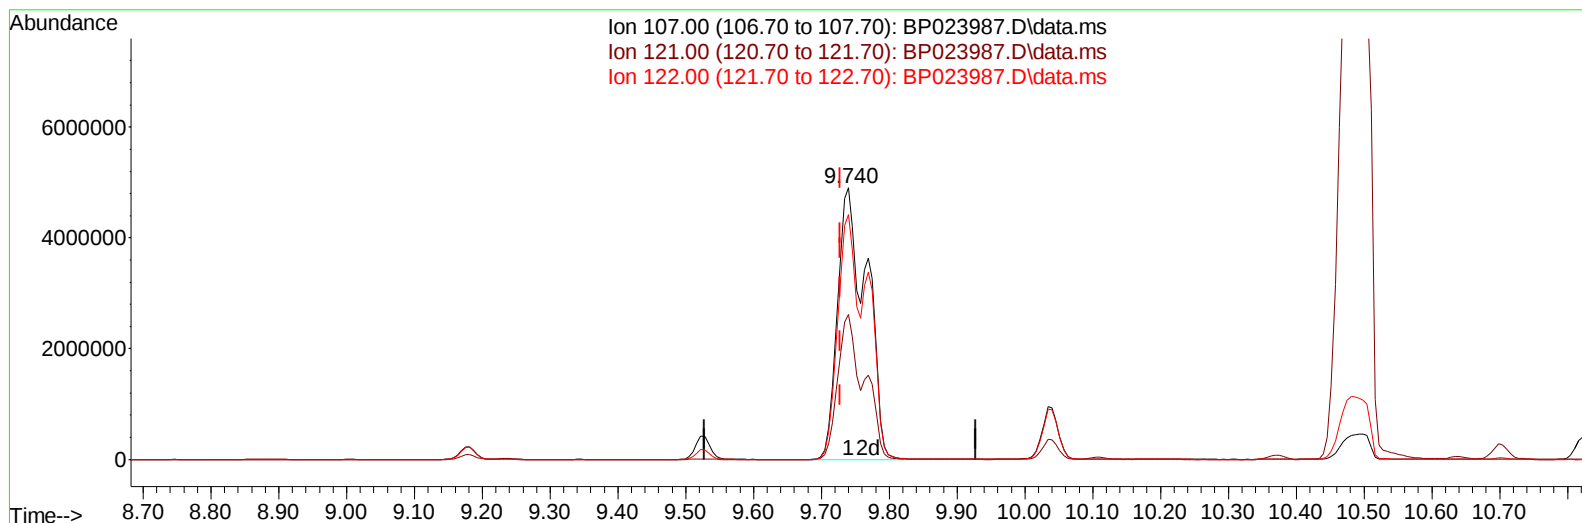

TIC: BP023987.D\data.ms

(26) 2,4-Dimethylphenol

9.740min (+ 0.012) 404.25 ng/ul m

response 14587343

Ion	Exp%	Act%
107.00	100.00	100.00
121.00	51.80	53.38
122.00	89.40	90.24
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020525\
 Data File : BP023987.D
 Acq On : 07 Feb 2025 02:49
 Operator : RC/JU
 Sample : Q1229-11
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E29B5

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 02/07/2025
 Supervised By :Sohil Jodhani 02/10/2025

Quant Time: Feb 07 08:03:00 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Feb 03 11:19:36 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.764	152	516056	20.000	ng/ul	-0.01
20) Naphthalene-d8	10.546	136	2070497	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.398	164	1361788	20.000	ng/ul	0.01
64) Phenanthrene-d10	17.192	188	2640012	20.000	ng/ul	0.00
79) Chrysene-d12	21.639	240	2636106	20.000	ng/ul	0.00
88) Perylene-d12	25.010	264	2857106	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.293	96	58061	4.675	ng/uL	0.00
4) Pyridine-d5	3.717	84	582920	16.265	ng/ul	0.01
7) Phenol-d5	6.952	99	280202	6.135	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.105	67	538252	22.266	ng/ul	0.00
11) 2-Chlorophenol-d4	7.311	132	692192	19.301	ng/ul	0.00
15) 4-Methylphenol-d8	8.469	113	509102	13.646	ng/ul	0.00
21) Nitrobenzene-d5	8.916	128	384858	23.233	ng/ul	0.00
24) 2-Nitrophenol-d4	9.628	143	410275	22.953	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.175	165	732612	22.342	ng/ul	0.00
31) 4-Chloroaniline-d4	10.699	131	951538	19.404	ng/ul	0.02
46) Dimethylphthalate-d6	13.804	166	2502352	24.635	ng/ul	0.01
49) Acenaphthylene-d8	14.087	160	2740927	23.925	ng/ul	0.00
54) 4-Nitrophenol-d4	14.616	143	140311	6.956	ng/ul	0.00
60) Fluorene-d10	15.404	176	2168694	25.353	ng/ul	0.01
65) 4,6-Dinitro-2-methylph...	15.516	200	364575	22.385	ng/ul	0.00
73) Anthracene-d10	17.292	188	3485002	26.885	ng/ul	0.00
81) Pyrene-d10	19.669	212	4031694	28.544	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.774	264	4103323	27.526	ng/ul	0.00
Target Compounds						
						Qvalue
8) Phenol	6.981	94	150328	3.206	ng/ul	99
26) 2,4-Dimethylphenol	9.740	107	14587343m	404.249	ng/ul	
42) 2,4,5-Trichlorophenol	12.887	196	44675	1.541	ng/ul	98
71) Pentachlorophenol	16.834	266	25189	1.135	ng/ul	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020525\
Data File : BP023987.D
Acq On : 07 Feb 2025 02:49
Operator : RC/JU
Sample : Q1229-11
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E29B5

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 02/07/2025
Supervised By :Sohil Jodhani 02/10/2025

Quant Time: Feb 07 08:03:00 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Feb 03 11:19:36 2025
Response via : Initial Calibration

