

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020525\
 Data File : BP023955.D
 Acq On : 06 Feb 2025 04:32
 Operator : RC/JU
 Sample : Q1202-18
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E29B1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 02/07/2025
 Supervised By :mohammad ahmed 02/07/2025

Quant Time: Feb 06 08:01:24 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Feb 03 11:19:36 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.769	152	454789	20.000	ng/u1	0.00
20) Naphthalene-d8	10.546	136	1946312	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.387	164	1253027	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.175	188	2439792	20.000	ng/u1	-0.01
79) Chrysene-d12	21.616	240	2517879	20.000	ng/u1	-0.02
88) Perylene-d12	24.986	264	2665407	20.000	ng/u1	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.293	96	59150	5.404	ng/uL	0.00
4) Pyridine-d5	3.711	84	349915	11.079	ng/u1	0.00
7) Phenol-d5	6.952	99	358103	8.898	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.111	67	720788	33.834	ng/u1	0.00
11) 2-Chlorophenol-d4	7.311	132	989024	31.293	ng/u1	0.00
15) 4-Methylphenol-d8	8.475	113	693224	21.085	ng/u1	0.00
21) Nitrobenzene-d5	8.910	128	521432	33.486	ng/u1	0.00
24) 2-Nitrophenol-d4	9.634	143	568008	33.805	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.169	165	1049033	34.033	ng/u1	0.00
31) 4-Chloroaniline-d4	10.681	131	557183	12.087	ng/u1	0.00
46) Dimethylphthalate-d6	13.793	166	3022294	32.337	ng/u1	0.00
49) Acenaphthylene-d8	14.075	160	3539611	33.578	ng/u1	0.00
54) 4-Nitrophenol-d4	14.604	143	166055	8.946	ng/u1	0.00
60) Fluorene-d10	15.387	176	2678997	34.037	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.504	200	435231	28.916	ng/u1	0.00
73) Anthracene-d10	17.275	188	4324807	36.102	ng/u1	-0.01
81) Pyrene-d10	19.639	212	4878768	36.163	ng/u1	-0.02
92) Benzo(a)pyrene-d12	24.757	264	5031343	36.179	ng/u1	-0.02
Target Compounds					Qvalue	
13) 2-Methylphenol	8.210	108	45481	1.463	ng/u1	97
18) 4-Methylphenol	8.540	108	427691	12.397	ng/u1	92
26) 2,4-Dimethylphenol	9.757	107	2658802m	78.383	ng/u1	
30) Naphthalene	10.593	128	453653	4.354	ng/u1	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020525\
Data File : BP023955.D
Acq On : 06 Feb 2025 04:32
Operator : RC/JU
Sample : Q1202-18
Misc :
ALS Vial : 28 Sample Multiplier: 1


Instrument :
BNA_P
ClientSampleId :
E29B1

Quant Time: Feb 06 08:01:24 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Feb 03 11:19:36 2025
Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/07/2025
Supervised By :mohammad ahmed 02/07/2025

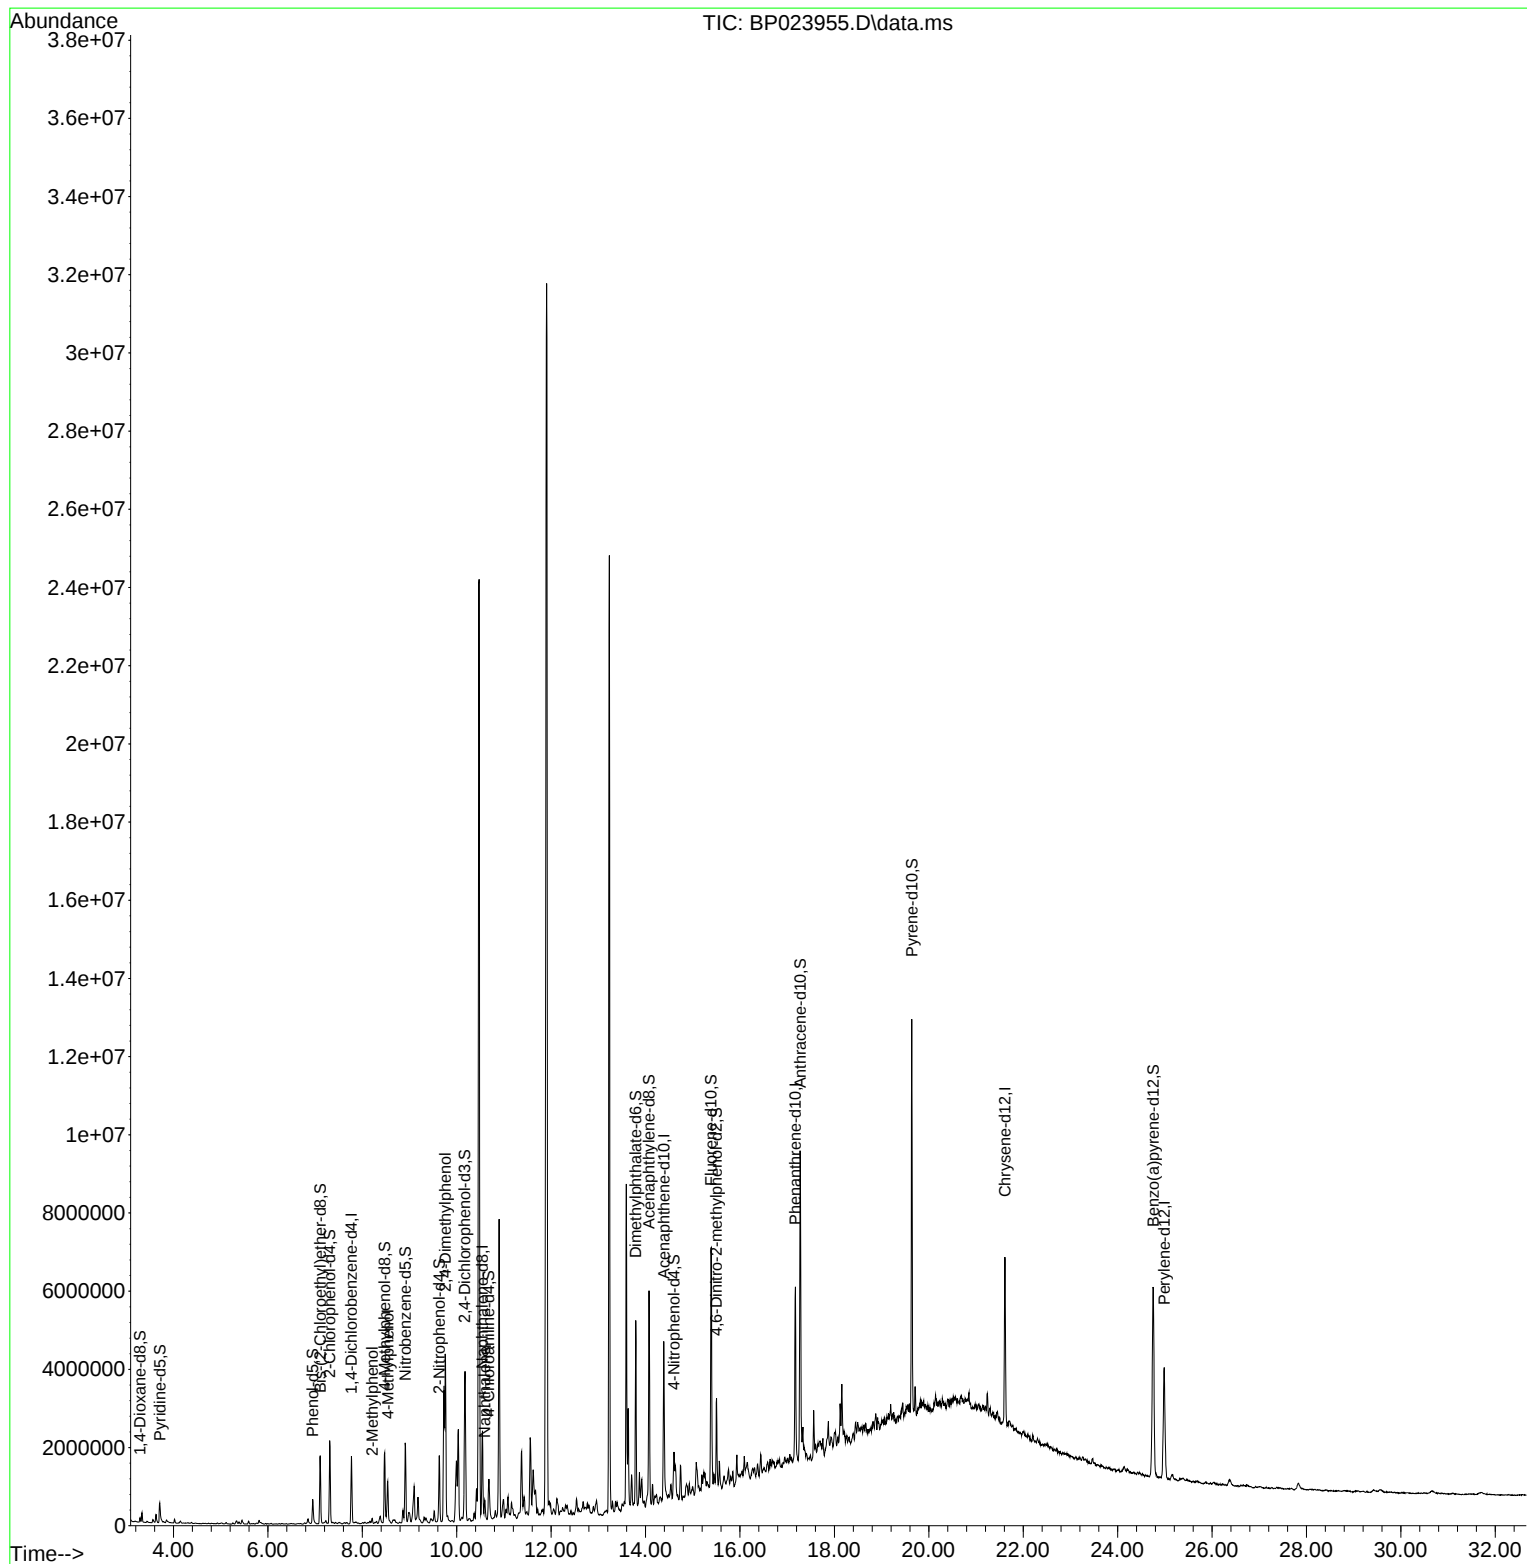

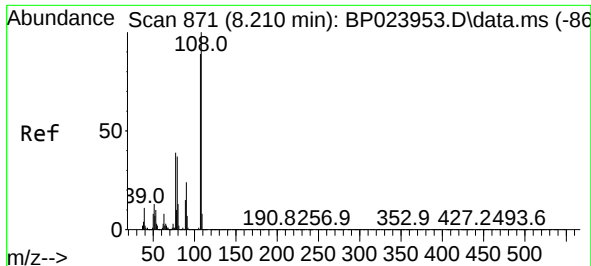





#13
2-Methylphenol
Concen: 1.463 ng/ul
RT: 8.210 min Scan# 81
Delta R.T. -0.006 min
Lab File: BP023955.D
Acq: 06 Feb 2025 04:32

Instrument :
BNA_P
ClientSampleId :
E29B1

Tgt Ion:108 Resp: 4548
Ion Ratio Lower Upper
108 100
107 91.7 71.0 106.6




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 02/07/2025
Supervised By :mohammad ahmed 02/07/2025

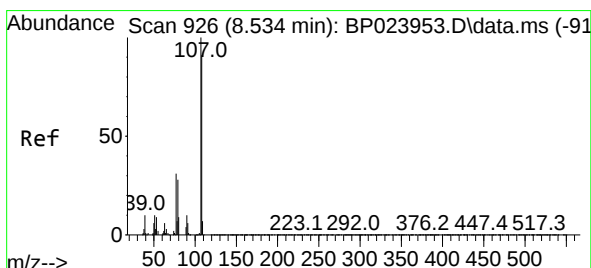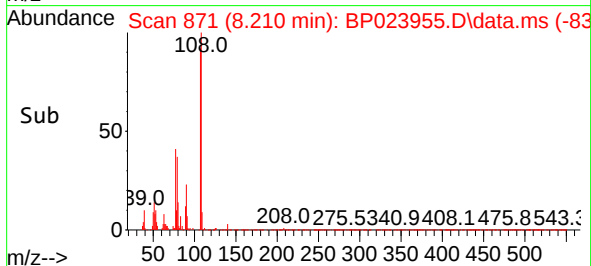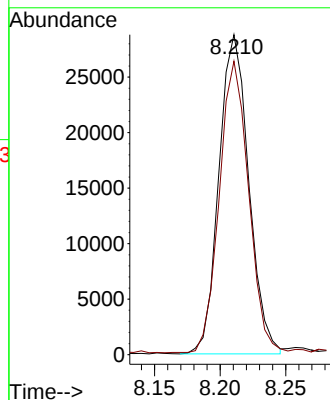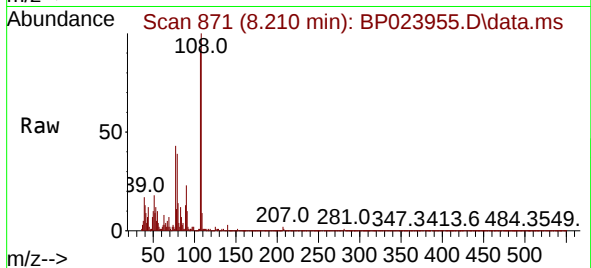

#18
4-Methylphenol
Concen: 12.397 ng/ul
RT: 8.540 min Scan# 927
Delta R.T. 0.006 min
Lab File: BP023955.D
Acq: 06 Feb 2025 04:32


Tgt Ion:108 Resp: 427691
Ion Ratio Lower Upper
108 100
107 101.4 87.8 131.6

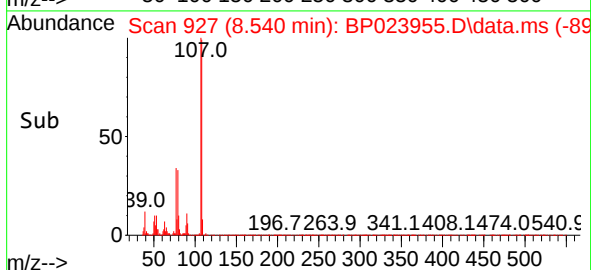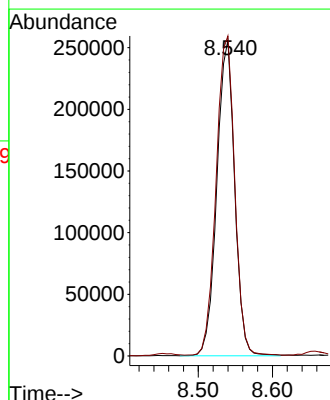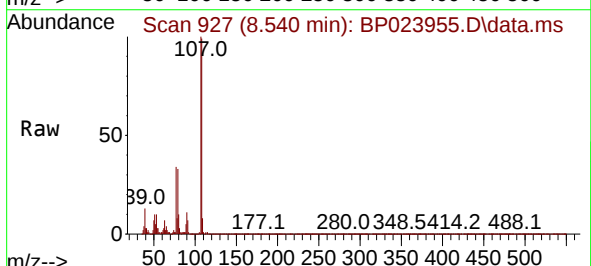

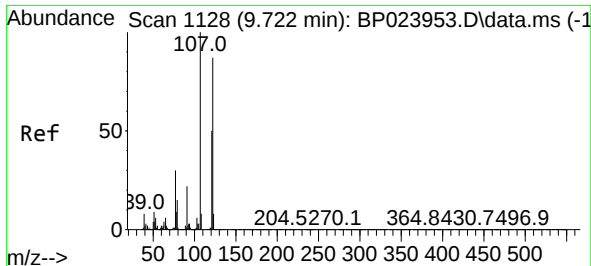

#26
2,4-Dimethylphenol
Concen: 78.383 ng/ul m
RT: 9.757 min Scan# 1128
Delta R.T. 0.029 min
Lab File: BP023955.D
Acq: 06 Feb 2025 04:32




Instrument :
BNA_P
ClientSampleId :
E29B1

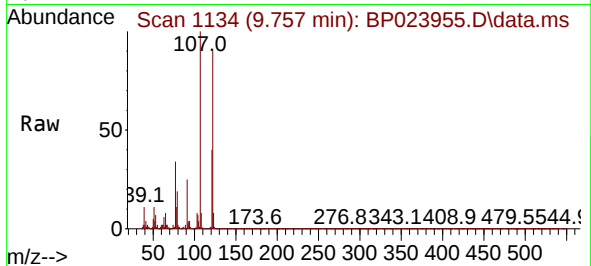

Tgt Ion:107 Resp: 265880
Ion Ratio Lower Upper
107 100
121 39.8 41.4 62.2
122 90.4 71.5 107.3

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/07/2025
Supervised By :mohammad ahmed 02/07/2025

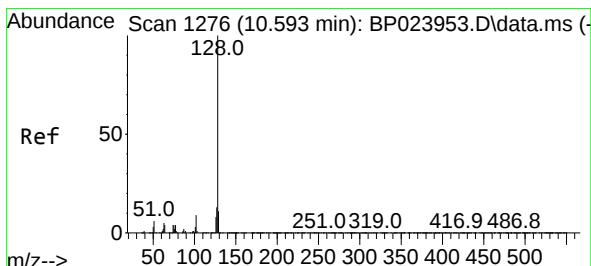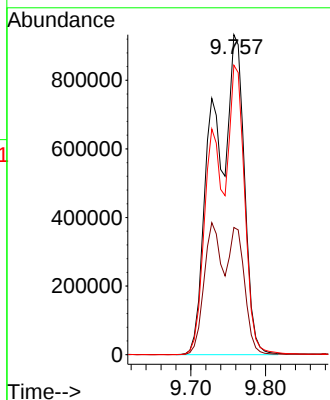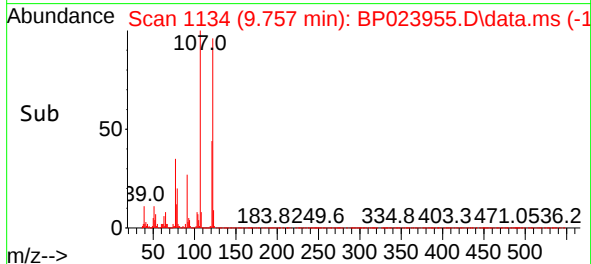

#30
Naphthalene
Concen: 4.354 ng/ul
RT: 10.593 min Scan# 1276
Delta R.T. -0.000 min
Lab File: BP023955.D
Acq: 06 Feb 2025 04:32

Tgt Ion:128 Resp: 453653
Ion Ratio Lower Upper
128 100
129 10.8 8.7 13.1
127 13.2 10.5 15.7

