

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020525\
 Data File : BP023961.D
 Acq On : 06 Feb 2025 08:34
 Operator : RC/JU
 Sample : Q1226-22
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCZL9

Quant Time: Feb 06 09:10:35 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Feb 03 11:19:36 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.769	152	500067	20.000	ng/u1	0.00
20) Naphthalene-d8	10.546	136	2160276	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.387	164	1360410	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.181	188	2684903	20.000	ng/u1	0.00
79) Chrysene-d12	21.622	240	2673099	20.000	ng/u1	-0.02
88) Perylene-d12	24.986	264	2908081	20.000	ng/u1	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.293	96	57405	4.770	ng/uL	0.00
4) Pyridine-d5	3.705	84	291690	8.399	ng/u1	0.00
7) Phenol-d5	6.958	99	325527	7.356	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.105	67	693357	29.600	ng/u1	0.00
11) 2-Chlorophenol-d4	7.316	132	971373	27.952	ng/u1	0.00
15) 4-Methylphenol-d8	8.481	113	644918	17.840	ng/u1	0.00
21) Nitrobenzene-d5	8.916	128	539979	31.242	ng/u1	0.00
24) 2-Nitrophenol-d4	9.634	143	590321	31.654	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.181	165	1054901	30.834	ng/u1	0.01
31) 4-Chloroaniline-d4	10.681	131	1204196	23.536	ng/u1	0.00
46) Dimethylphthalate-d6	13.793	166	3334103	32.857	ng/u1	0.00
49) Acenaphthylene-d8	14.075	160	3677283	32.131	ng/u1	0.00
54) 4-Nitrophenol-d4	14.622	143	150549	7.471	ng/u1	0.01
60) Fluorene-d10	15.392	176	2840722	33.243	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.516	200	497708	30.048	ng/u1	0.00
73) Anthracene-d10	17.281	188	4707408	35.709	ng/u1	0.00
81) Pyrene-d10	19.651	212	5441712	37.993	ng/u1	-0.01
92) Benzo(a)pyrene-d12	24.763	264	5557743	36.629	ng/u1	-0.01
Target Compounds						
					Qvalue	
71) Pentachlorophenol	16.828	266	223012	9.878	ng/u1	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020525\
Data File : BP023961.D
Acq On : 06 Feb 2025 08:34
Operator : RC/JU
Sample : Q1226-22
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCZL9


Quant Time: Feb 06 09:10:35 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Feb 03 11:19:36 2025
Response via : Initial Calibration

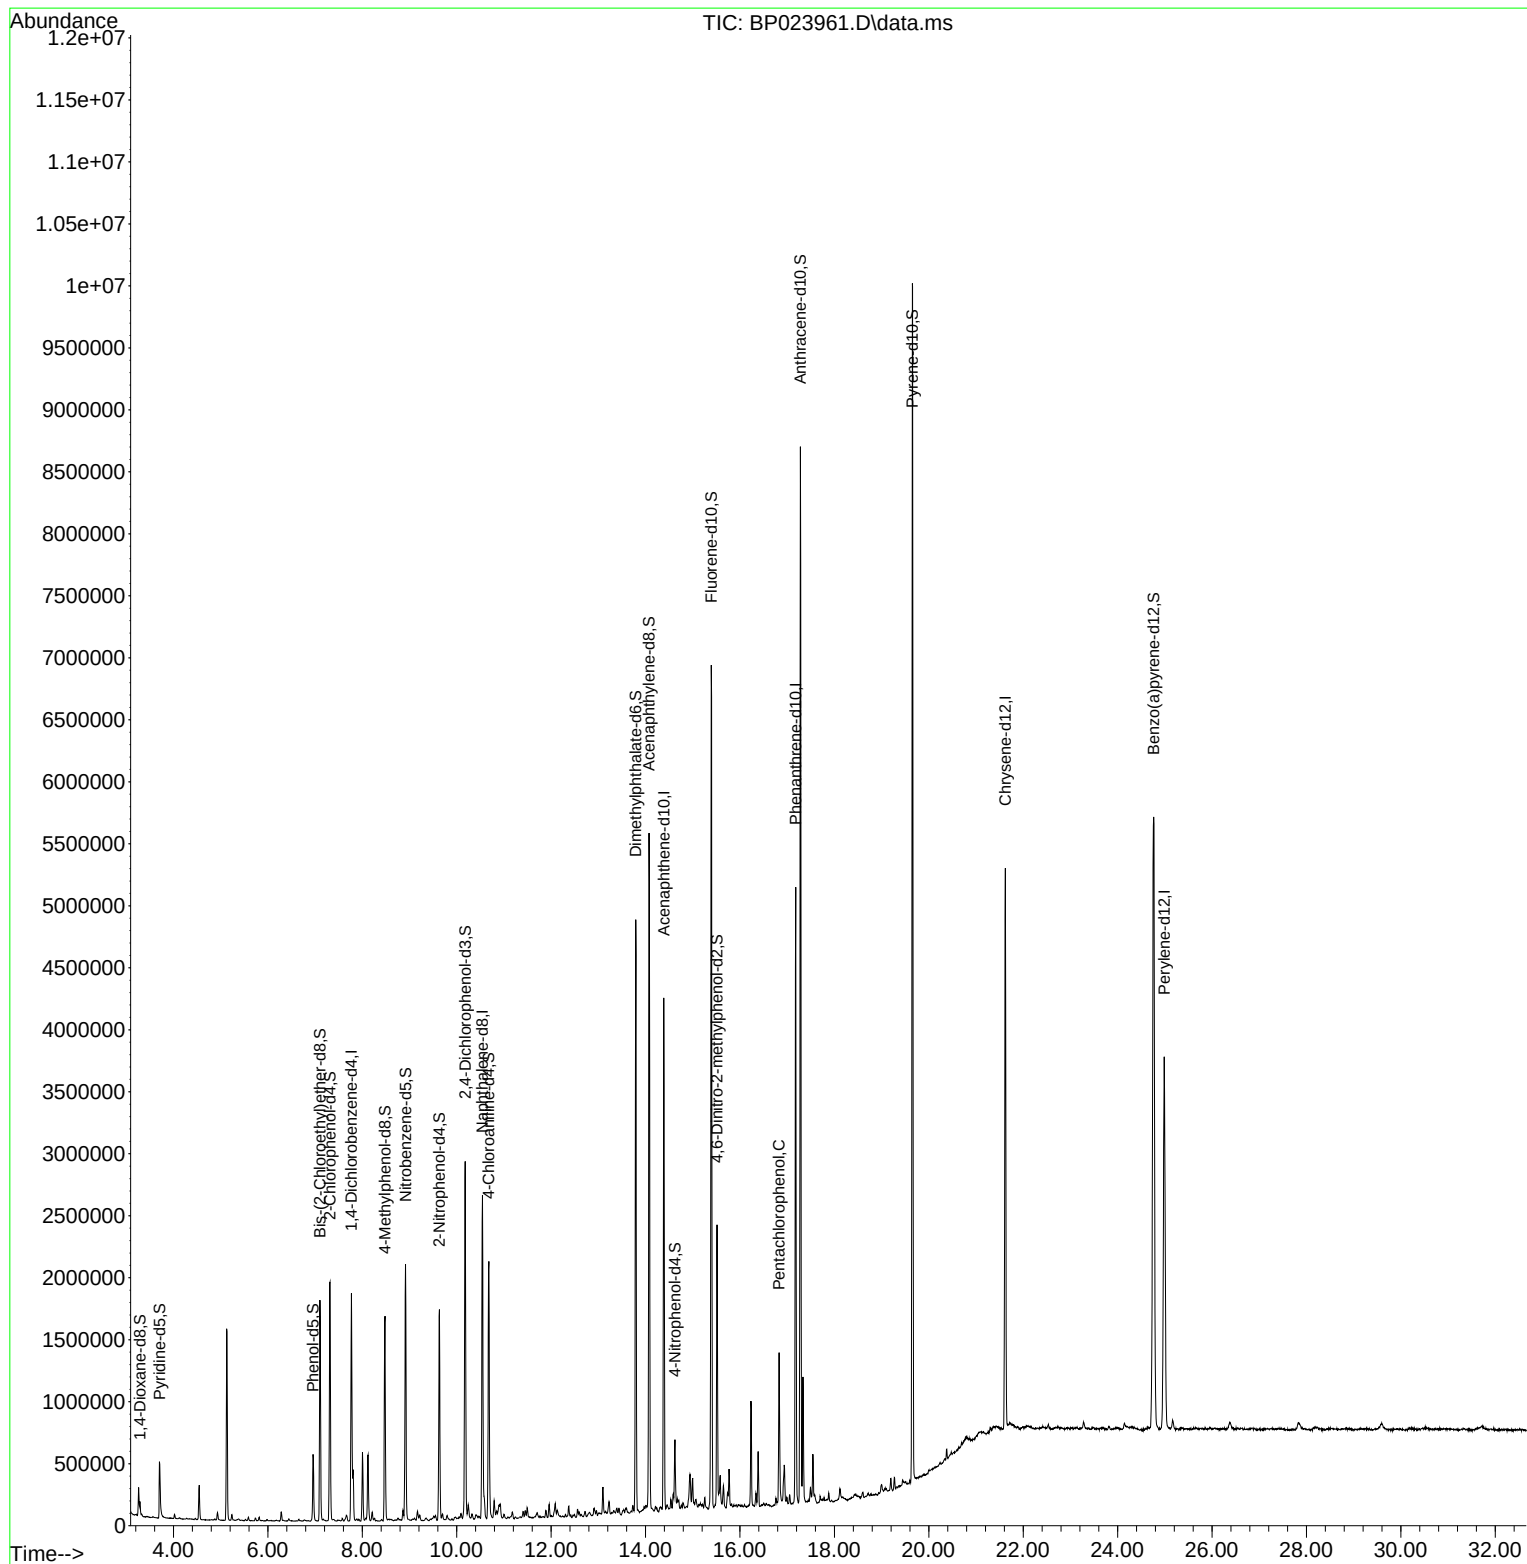

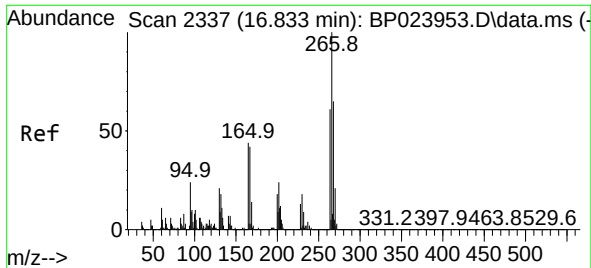

#71
 Pentachlorophenol
 Concen: 9.878 ng/ul
 RT: 16.828 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: BP023961.D
 Acq: 06 Feb 2025 08:34

Instrument :
 BNA_P
 ClientSampleId :
 DCZL9

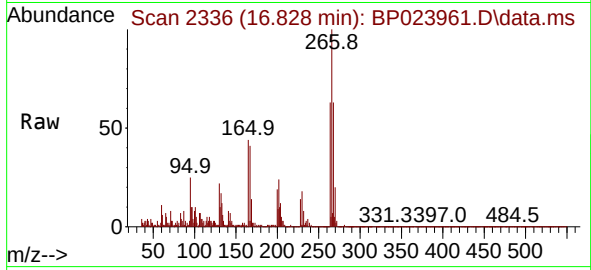

Tgt Ion:266 Resp: 223012
 Ion Ratio Lower Upper
 266 100
 264 62.5 50.8 76.2
 268 62.6 51.1 76.7

