

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020525\
 Data File : BP023971.D
 Acq On : 06 Feb 2025 15:19
 Operator : RC/JU
 Sample : Q1226-23
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCZN9

Quant Time: Feb 06 15:42:56 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Feb 03 11:19:36 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.769	152	455882	20.000	ng/ul	0.00
20) Naphthalene-d8	10.540	136	1983651	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.392	164	1286517	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.186	188	2587081	20.000	ng/ul	0.00
79) Chrysene-d12	21.627	240	2517167	20.000	ng/ul	-0.01
88) Perylene-d12	24.998	264	2634695	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.287	96	57728	5.261	ng/uL	0.00
4) Pyridine-d5	3.705	84	313692	9.908	ng/ul	0.00
7) Phenol-d5	6.957	99	282641	7.006	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.105	67	619757	29.022	ng/ul	0.00
11) 2-Chlorophenol-d4	7.310	132	831560	26.248	ng/ul	0.00
15) 4-Methylphenol-d8	8.475	113	562521	17.068	ng/ul	0.00
21) Nitrobenzene-d5	8.910	128	459942	28.981	ng/ul	0.00
24) 2-Nitrophenol-d4	9.628	143	494919	28.901	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.175	165	871654	27.746	ng/ul	0.00
31) 4-Chloroaniline-d4	10.675	131	1322281	28.145	ng/ul	0.00
46) Dimethylphthalate-d6	13.792	166	3023821	31.511	ng/ul	0.00
49) Acenaphthylene-d8	14.081	160	3315983	30.638	ng/ul	0.00
54) 4-Nitrophenol-d4	14.616	143	116951	6.137	ng/ul	0.00
60) Fluorene-d10	15.398	176	2635840	32.617	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.510	200	381445	23.900	ng/ul	0.00
73) Anthracene-d10	17.292	188	4291176	33.782	ng/ul	0.00
81) Pyrene-d10	19.657	212	4923379	36.504	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.774	264	4848967	35.274	ng/ul	0.00
Target Compounds						
					Qvalue	
58) 2,3,4,6-Tetrachlorophenol	15.034	232	72355	3.105	ng/ul	93
71) Pentachlorophenol	16.833	266	313353	14.405	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020525\
Data File : BP023971.D
Acq On : 06 Feb 2025 15:19
Operator : RC/JU
Sample : Q1226-23
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCZN9

Quant Time: Feb 06 15:42:56 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Feb 03 11:19:36 2025
Response via : Initial Calibration




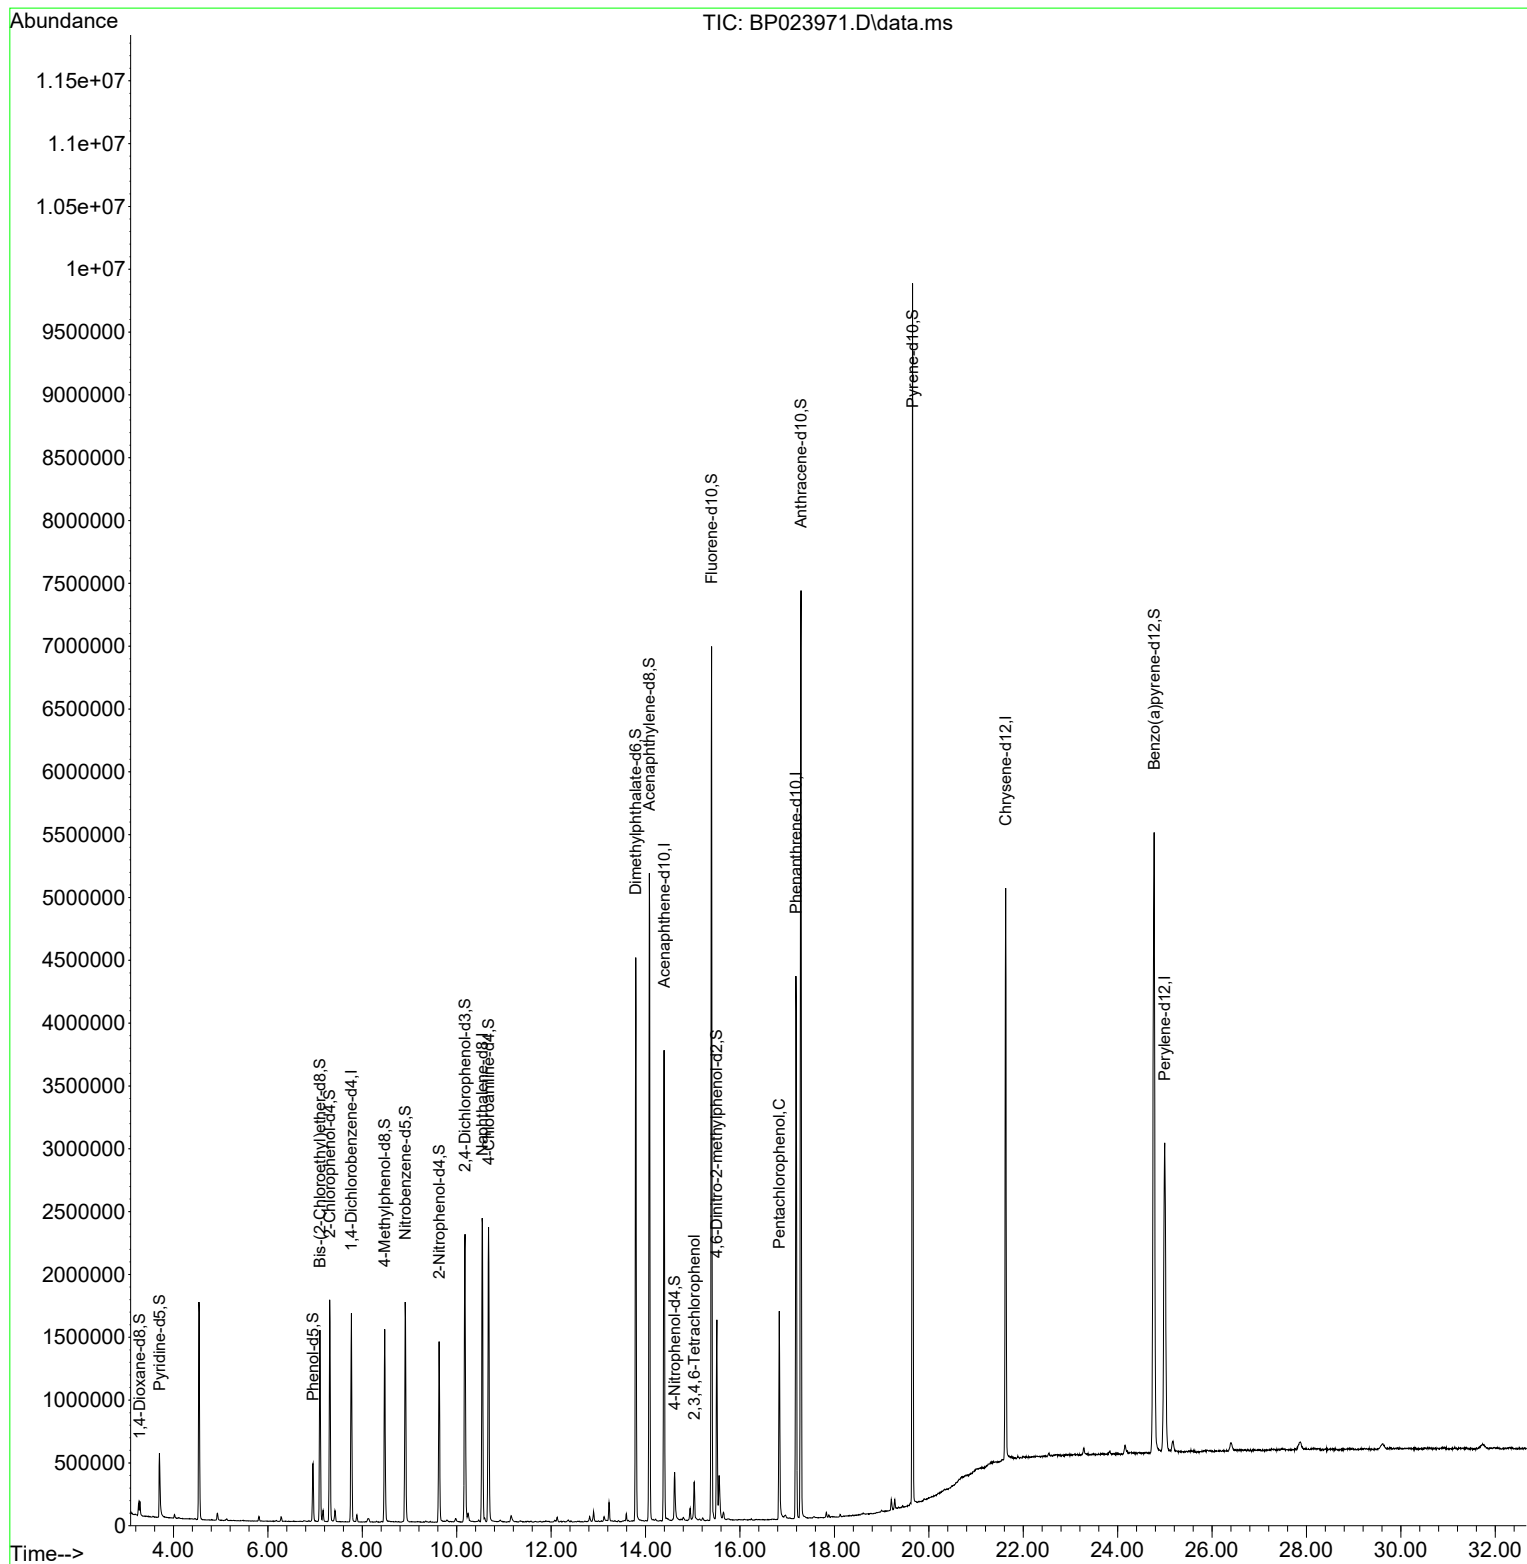


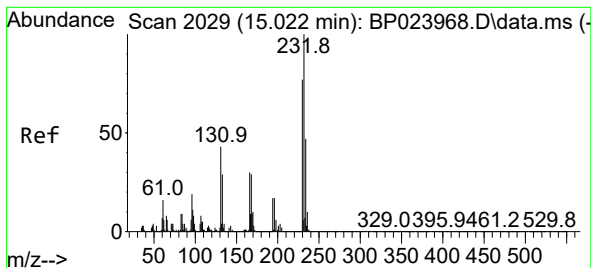

#58
2,3,4,6-Tetrachlorophenol
Concen: 3.105 ng/ul
RT: 15.034 min Scan# 2029
Delta R.T. 0.012 min
Lab File: BP023971.D
Acq: 06 Feb 2025 15:19

Instrument :
BNA_P
ClientSampleId :
DCZN9

Tgt Ion:232	Resp:	72355
Ion Ratio	Lower	Upper
232	100	
131	46.5	32.4 48.6
130	2.4	1.7 2.5
166	30.9	23.0 34.4

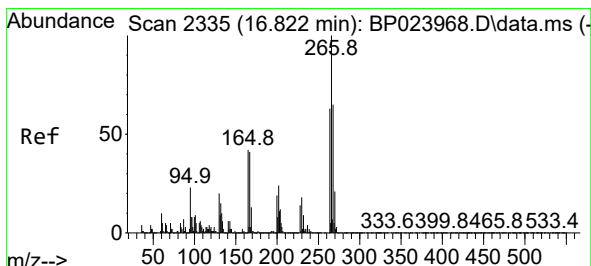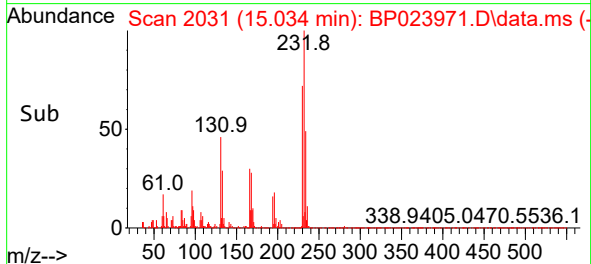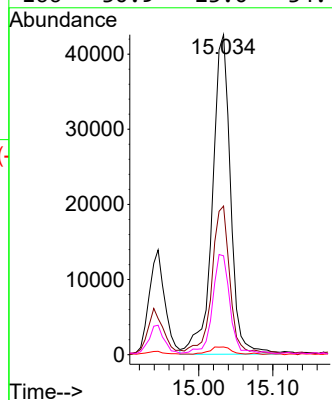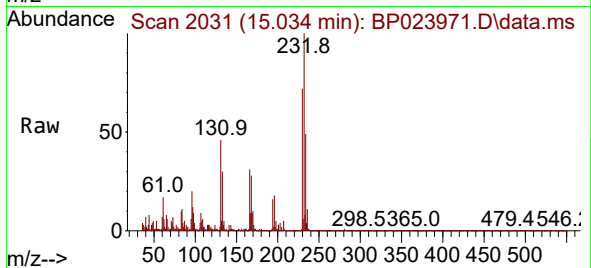

#71
Pentachlorophenol
Concen: 14.405 ng/ul
RT: 16.833 min Scan# 2337
Delta R.T. 0.006 min
Lab File: BP023971.D
Acq: 06 Feb 2025 15:19

Tgt Ion:266	Resp:	313353
Ion Ratio	Lower	Upper
266	100	
264	61.5	50.8 76.2
268	63.5	51.1 76.7

