

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020525\
 Data File : BP023930.D
 Acq On : 05 Feb 2025 10:10
 Operator : RC/JU
 Sample : PB166495BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK495

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP023930.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.293	31	35	43	rVB	100680	136155	1.44%	0.140%
2	3.699	100	104	126	rBV	1337253	2066050	21.81%	2.126%
3	4.022	155	159	166	rVB	26337	38366	0.40%	0.039%
4	6.952	650	657	671	rBV	1615835	2653684	28.01%	2.731%
5	7.105	677	683	694	rVB	1356116	1973314	20.83%	2.031%
6	7.316	709	719	730	rBV	1676905	2655079	28.02%	2.732%
7	7.769	789	796	806	rVB	1336383	2043975	21.57%	2.103%
8	8.475	908	916	931	rBV	2149468	3335644	35.21%	3.432%
9	8.916	982	991	1003	rBV	1434500	2358492	24.89%	2.427%
10	9.040	1008	1012	1017	rBV4	12933	20171	0.21%	0.021%
11	9.628	1104	1112	1126	rBV	1092903	1870211	19.74%	1.924%
12	10.175	1197	1205	1223	rBV	2140090	3314761	34.99%	3.411%
13	10.546	1259	1268	1276	rBV	1991612	3039751	32.08%	3.128%
14	10.681	1282	1291	1305	rBV	1864885	3316699	35.01%	3.413%
15	12.134	1532	1538	1545	rBV2	30773	55052	0.58%	0.057%
16	13.363	1742	1747	1753	rVB7	6700	13499	0.14%	0.014%
17	13.793	1814	1820	1831	rBV	3413523	4620297	48.76%	4.754%
18	14.081	1862	1869	1887	rBV	4112953	5955659	62.86%	6.129%
19	14.392	1913	1922	1930	rBV	2852129	4175539	44.07%	4.297%
20	14.610	1952	1959	1982	rBV	1288257	2184437	23.06%	2.248%
21	14.810	1991	1993	2000	rVB6	8572	12621	0.13%	0.013%
22	15.063	2030	2036	2042	rVB9	8745	16857	0.18%	0.017%
23	15.398	2087	2093	2108	rBV	5709439	7434215	78.46%	7.650%
24	15.528	2108	2115	2127	rVV	1008029	1389661	14.67%	1.430%
25	15.651	2130	2136	2146	rVB2	28807	55349	0.58%	0.057%
26	16.981	2356	2362	2367	rBV	13641	25250	0.27%	0.026%
27	17.192	2392	2398	2408	rBV2	3647990	4997701	52.75%	5.143%
28	17.298	2408	2416	2426	rBV	6083190	8186560	86.40%	8.424%
29	17.892	2514	2517	2522	rBV6	10460	15060	0.16%	0.015%
30	18.128	2554	2557	2561	rBV6	7524	11595	0.12%	0.012%
31	19.204	2736	2740	2746	rVB2	53698	80150	0.85%	0.082%
32	19.280	2749	2753	2760	rVV	52083	74665	0.79%	0.077%
33	19.657	2811	2817	2827	rBV	7848966	9474690	100.00%	9.750%
34	21.616	3144	3150	3165	rBV	3740083	5387868	56.87%	5.544%
35	24.739	3674	3681	3700	rVB	3228585	8943652	94.40%	9.203%
36	24.980	3714	3722	3733	rVB	2086473	5246604	55.37%	5.399%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020525\
Data File : BP023930.D
Acq On : 05 Feb 2025 10:10
Operator : RC/JU
Sample : PB166495BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK495

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 97179333

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020525\
Data File : BP023930.D
Acq On : 05 Feb 2025 10:10
Operator : RC/JU
Sample : PB166495BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK495

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

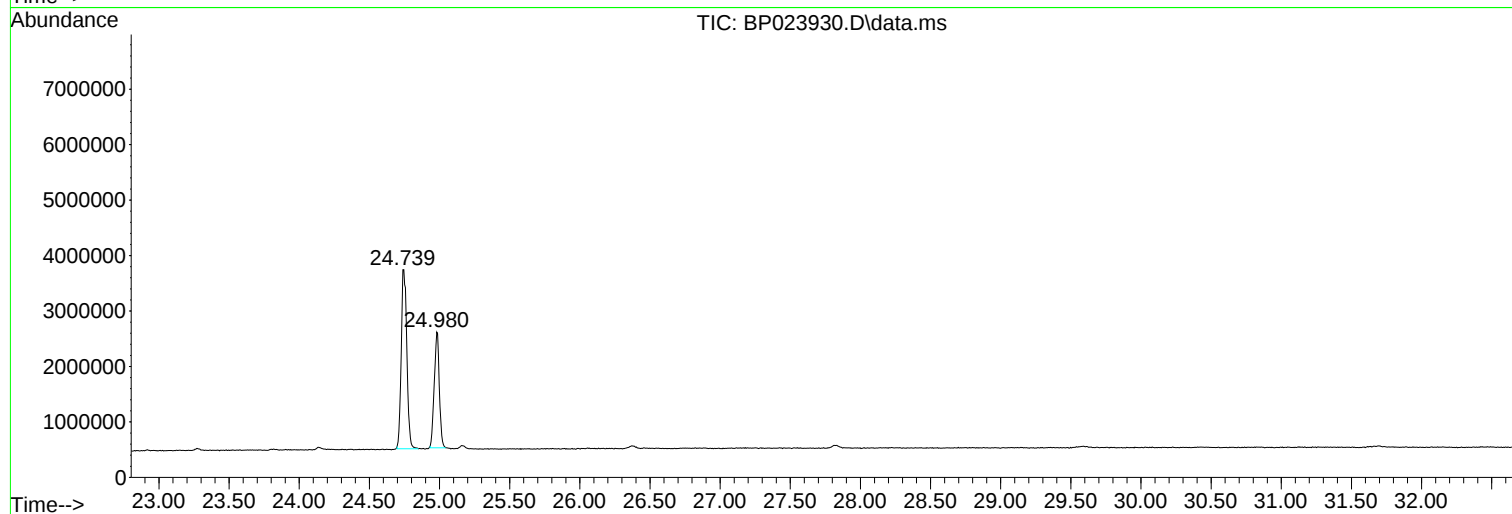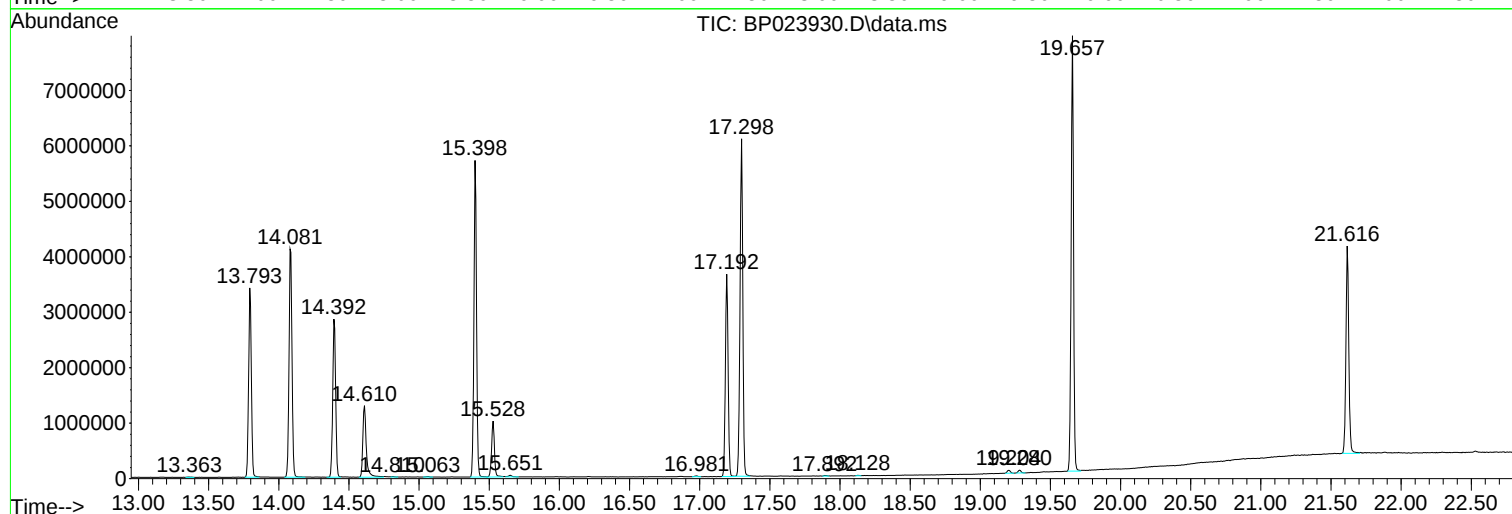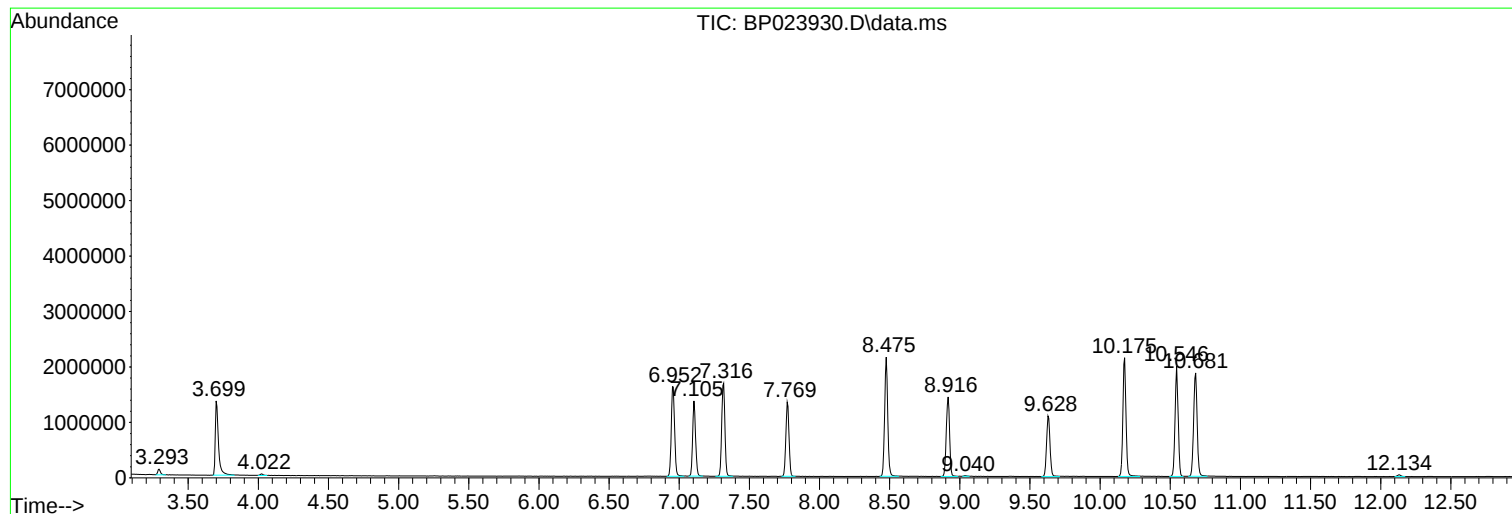

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020525\
Data File : BP023930.D
Acq On : 05 Feb 2025 10:10
Operator : RC/JU
Sample : PB166495BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK495

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020525\
Data File : BP023930.D
Acq On : 05 Feb 2025 10:10
Operator : RC/JU
Sample : PB166495BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK495

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc