

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020525\
 Data File : BP023934.D
 Acq On : 05 Feb 2025 13:42
 Operator : RC/JU
 Sample : Q1226-08
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCZP0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP023934.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.293	32	35	46	rVB	121056	151735	1.23%	0.136%
2	3.711	102	106	126	rBV	338114	593791	4.83%	0.534%
3	4.028	155	160	166	rVB	67809	95557	0.78%	0.086%
4	4.117	172	175	183	rVB8	8563	13593	0.11%	0.012%
5	4.464	231	234	238	rVB2	10755	14475	0.12%	0.013%
6	4.546	244	248	256	rVB2	23801	39629	0.32%	0.036%
7	4.934	309	314	322	rVB2	45638	71017	0.58%	0.064%
8	5.134	342	348	354	rVB	104885	151397	1.23%	0.136%
9	6.181	520	526	531	rBV4	7798	13574	0.11%	0.012%
10	6.781	622	628	631	rBV6	7100	15894	0.13%	0.014%
11	6.952	648	657	668	rBV	713590	1093247	8.89%	0.983%
12	7.105	676	683	694	rBV	1615542	2557534	20.80%	2.301%
13	7.211	698	701	707	rVV6	9123	14265	0.12%	0.013%
14	7.311	711	718	730	rVV	1992740	2980443	24.24%	2.681%
15	7.405	730	734	744	rVB10	10922	22683	0.18%	0.020%
16	7.775	789	797	811	rBV	1519090	2464135	20.04%	2.217%
17	8.005	831	836	843	rVB	31973	48712	0.40%	0.044%
18	8.146	851	860	865	rBV	61294	102759	0.84%	0.092%
19	8.199	865	869	876	rVB	12836	19416	0.16%	0.017%
20	8.475	909	916	928	rBV	1890883	2982436	24.25%	2.683%
21	8.575	930	933	938	rVB6	10306	15513	0.13%	0.014%
22	8.916	978	991	1002	rBV	1890493	3115538	25.33%	2.803%
23	9.346	1060	1064	1073	rVB5	7439	15521	0.13%	0.014%
24	9.634	1105	1113	1129	rBV	1502408	2480767	20.17%	2.232%
25	9.799	1134	1141	1150	rVV2	25627	56485	0.46%	0.051%
26	10.169	1194	1204	1216	rBV	2613444	4179383	33.99%	3.759%
27	10.546	1260	1268	1282	rBV	2243769	3671344	29.85%	3.302%
28	10.681	1283	1291	1303	rBV	372280	650695	5.29%	0.585%
29	11.340	1398	1403	1409	rBV9	9324	19103	0.16%	0.017%
30	11.469	1417	1425	1436	rBV	72542	187075	1.52%	0.168%
31	12.128	1532	1537	1543	rVB	35693	59756	0.49%	0.054%
32	13.104	1696	1703	1707	rBV9	7007	14474	0.12%	0.013%
33	13.346	1737	1744	1752	rVB8	6546	13965	0.11%	0.013%
34	13.793	1813	1820	1830	rBV	4501472	6250789	50.83%	5.623%
35	14.081	1861	1869	1886	rBV	5046896	7368076	59.91%	6.628%
36	14.387	1912	1921	1928	rBV	3282621	4822582	39.22%	4.338%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020525\
 Data File : BP023934.D
 Acq On : 05 Feb 2025 13:42
 Operator : RC/JU
 Sample : Q1226-08
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCZP0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
 Title : SVOA CALIBRATION

37	14.446	1928	1931	1934	rVB4	11233	16188	0.13%	0.015%
38	14.610	1950	1959	1973	rBV	542972	928785	7.55%	0.835%
39	14.816	1991	1994	1999	rVB7	9073	14944	0.12%	0.013%
40	14.993	2019	2024	2028	rBV2	21160	30706	0.25%	0.028%
41	15.222	2058	2063	2068	rBV3	19944	32927	0.27%	0.030%
42	15.393	2084	2092	2106	rBV	7310495	9808476	79.76%	8.823%
43	15.516	2107	2113	2119	rBV	1518567	2302093	18.72%	2.071%
44	15.645	2130	2135	2142	rVB	34578	56303	0.46%	0.051%
45	15.769	2154	2156	2163	rVB8	9184	14719	0.12%	0.013%
46	16.245	2233	2237	2242	rBV6	9832	13307	0.11%	0.012%
47	16.834	2333	2337	2349	rBV3	45611	89458	0.73%	0.080%
48	16.951	2352	2357	2366	rBV2	169242	245623	2.00%	0.221%
49	17.057	2371	2375	2382	rVB2	55183	72380	0.59%	0.065%
50	17.192	2389	2398	2408	rBV	3804395	5368767	43.66%	4.829%
51	17.292	2409	2415	2421	rVV	8442969	11207290	91.13%	10.081%
52	17.339	2421	2423	2437	rVB2	106657	163101	1.33%	0.147%
53	17.504	2447	2451	2457	rBV5	16756	25446	0.21%	0.023%
54	17.892	2513	2517	2523	rBV4	34528	46775	0.38%	0.042%
55	18.610	2636	2639	2642	rBV4	9780	13350	0.11%	0.012%
56	19.210	2736	2741	2746	rBV3	71716	114651	0.93%	0.103%
57	19.281	2748	2753	2757	rBV	69197	103207	0.84%	0.093%
58	19.657	2811	2817	2829	rBV	9867215	12297588	100.00%	11.062%
59	21.616	3144	3150	3161	rBV	3132750	5242915	42.63%	4.716%
60	24.745	3673	3682	3702	rVB	4836530	11288007	91.79%	10.154%
61	24.974	3712	3721	3738	rVB	1838223	5304456	43.13%	4.772%




Sum of corrected areas: 111168820

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020525\
Data File : BP023934.D
Acq On : 05 Feb 2025 13:42
Operator : RC/JU
Sample : Q1226-08
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCZP0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

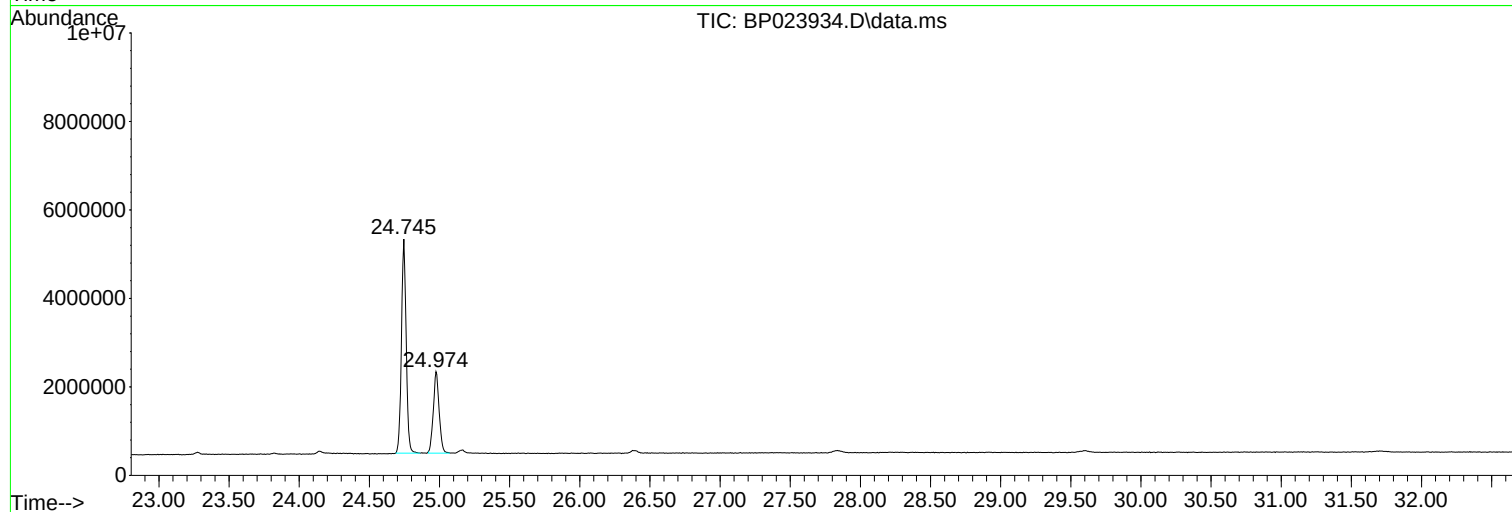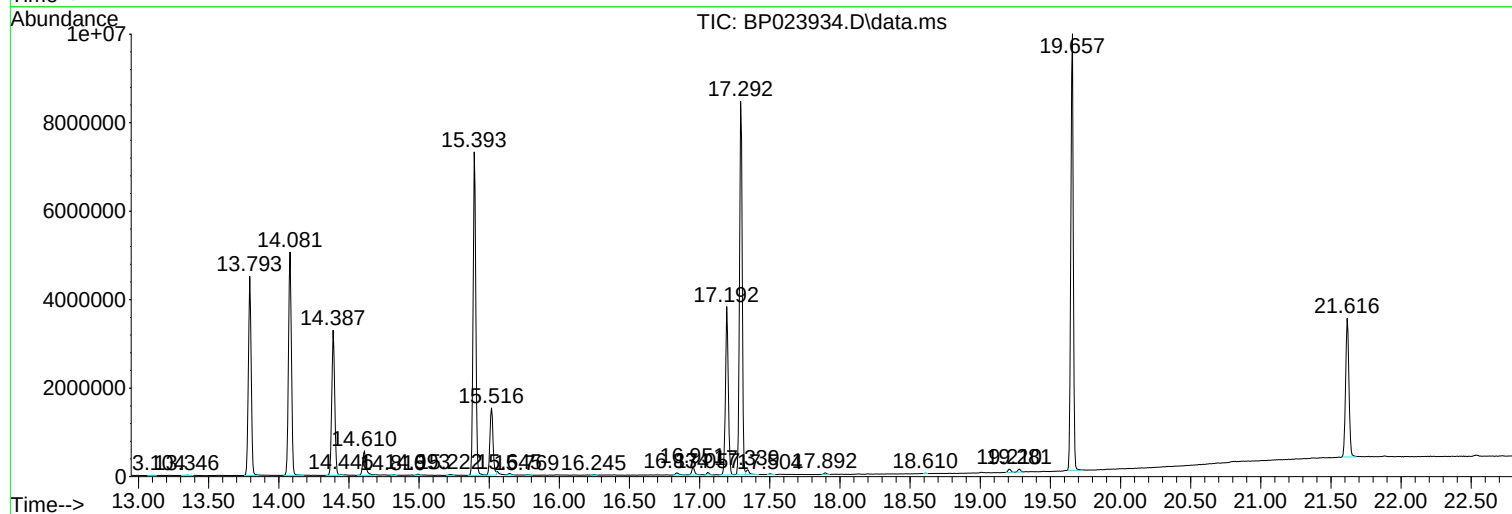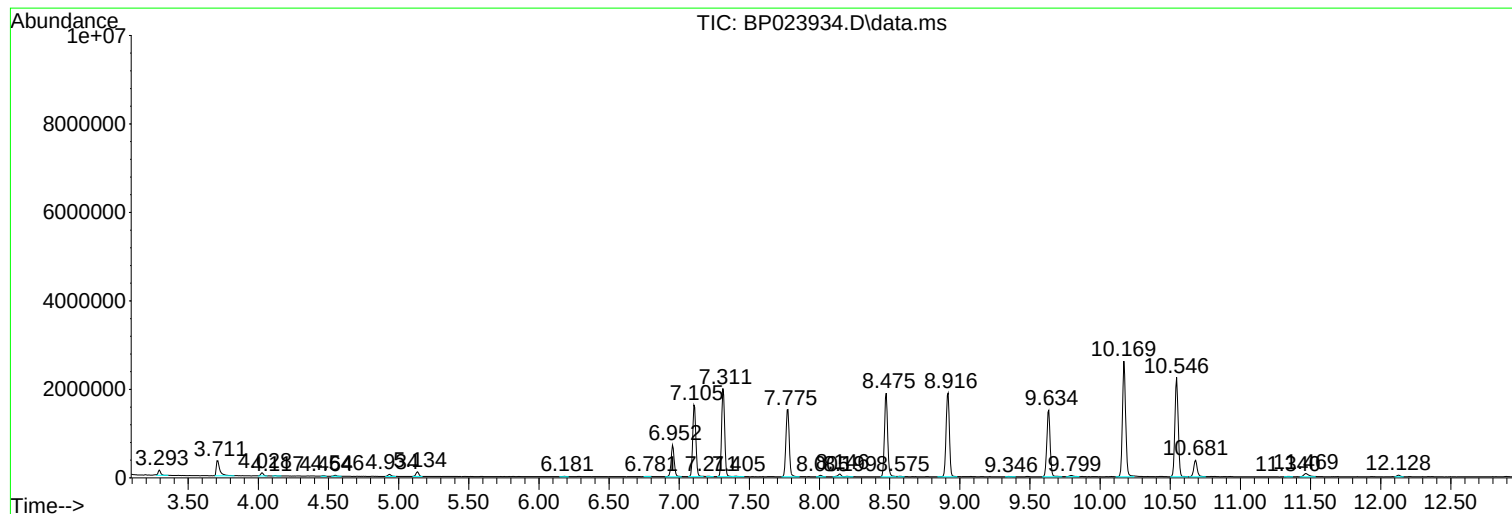

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020525\
Data File : BP023934.D
Acq On : 05 Feb 2025 13:42
Operator : RC/JU
Sample : Q1226-08
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCZP0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020525\
Data File : BP023934.D
Acq On : 05 Feb 2025 13:42
Operator : RC/JU
Sample : Q1226-08
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCZP0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc