

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020525\
 Data File : BP023936.D
 Acq On : 05 Feb 2025 15:03
 Operator : RC/JU
 Sample : Q1226-10
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCZP5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP023936.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.299	32	36	46	rVB	103461	160864	1.25%	0.143%
2	3.711	102	106	120	rBV	569807	938878	7.29%	0.837%
3	4.028	156	160	168	rVB	24936	38133	0.30%	0.034%
4	4.546	245	248	256	rVB3	17474	28117	0.22%	0.025%
5	4.928	309	313	319	rVB3	12558	24344	0.19%	0.022%
6	5.240	362	366	370	rBV3	12336	15606	0.12%	0.014%
7	6.181	519	526	530	rVB6	7410	13534	0.11%	0.012%
8	6.781	623	628	634	rBV9	7952	16003	0.12%	0.014%
9	6.952	649	657	667	rBV	665924	1067534	8.28%	0.952%
10	7.110	677	684	693	rBV	1573658	2390529	18.55%	2.131%
11	7.316	711	719	731	rBV	1827016	2894402	22.46%	2.581%
12	7.769	789	796	805	rBV	1615238	2454397	19.05%	2.188%
13	8.010	830	837	841	rBV	31896	54364	0.42%	0.048%
14	8.475	908	916	926	rBV	1852027	2868812	22.26%	2.558%
15	8.916	983	991	999	rBV	1773916	2792452	21.67%	2.490%
16	9.169	1027	1034	1041	rVB7	9685	21185	0.16%	0.019%
17	9.346	1060	1064	1071	rVB2	15072	23843	0.19%	0.021%
18	9.481	1081	1087	1094	rVB7	10916	21362	0.17%	0.019%
19	9.552	1094	1099	1105	rBV	35093	55478	0.43%	0.049%
20	9.628	1105	1112	1119	rBV	1431310	2259200	17.53%	2.014%
21	9.693	1119	1123	1128	rVB2	38472	65907	0.51%	0.059%
22	10.175	1197	1205	1215	rBV	2547948	4013690	31.15%	3.579%
23	10.546	1260	1268	1277	rBV	2213853	3492054	27.10%	3.114%
24	10.675	1282	1290	1306	rBV	1904955	3304854	25.65%	2.947%
25	10.922	1325	1332	1340	rVB	70934	113856	0.88%	0.102%
26	11.340	1394	1403	1409	rBV	7128	17416	0.14%	0.016%
27	11.957	1502	1508	1512	rBV3	15493	30590	0.24%	0.027%
28	12.122	1529	1536	1545	rVB2	38646	73542	0.57%	0.066%
29	12.363	1571	1577	1584	rVB2	11329	20795	0.16%	0.019%
30	13.210	1717	1721	1730	rVB7	12766	26207	0.20%	0.023%
31	13.716	1801	1807	1811	rVB9	6754	14403	0.11%	0.013%
32	13.792	1813	1820	1834	rBV	4258017	5898950	45.78%	5.259%
33	14.081	1860	1869	1880	rBV	4802593	6867083	53.29%	6.123%
34	14.387	1914	1921	1927	rBV	3225699	4441890	34.47%	3.960%
35	14.434	1927	1929	1933	rVB5	10678	14016	0.11%	0.012%
36	14.528	1942	1945	1949	rVB3	16232	21272	0.17%	0.019%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020525\
 Data File : BP023936.D
 Acq On : 05 Feb 2025 15:03
 Operator : RC/JU
 Sample : Q1226-10
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCZP5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
 Title : SVOA CALIBRATION

37	14.598	1951	1957	1972	rVV	554106	899521	6.98%	0.802%
38	14.734	1977	1980	1986	rVB5	16550	30721	0.24%	0.027%
39	15.204	2056	2060	2066	rVB2	32184	56595	0.44%	0.050%
40	15.392	2085	2092	2101	rBV	6647216	9031409	70.09%	8.052%
41	15.516	2106	2113	2121	rBV	1778009	2342839	18.18%	2.089%
42	15.639	2130	2134	2138	rVB2	26510	37009	0.29%	0.033%
43	15.769	2151	2156	2162	rVB	76758	111877	0.87%	0.100%
44	16.228	2231	2234	2239	rVB5	11395	17286	0.13%	0.015%
45	16.686	2309	2312	2316	rVB5	14136	20228	0.16%	0.018%
46	17.116	2382	2385	2388	rVB4	19151	20643	0.16%	0.018%
47	17.175	2389	2395	2405	rVV2	3708613	5263462	40.85%	4.693%
48	17.281	2406	2413	2425	rBV	7166424	10251250	79.56%	9.140%
49	18.104	2550	2553	2558	rBV2	44087	62824	0.49%	0.056%
50	19.192	2734	2738	2743	rBV	88324	124166	0.96%	0.111%
51	19.269	2747	2751	2755	rBV	86256	118060	0.92%	0.105%
52	19.645	2809	2815	2826	rBV	9914467	12885719	100.00%	11.489%
53	21.604	3143	3148	3161	rBV	3812726	5961164	46.26%	5.315%
54	24.745	3672	3682	3698	rVB	5081089	12279025	95.29%	10.948%
55	24.974	3711	3721	3737	rVB	2247170	6089022	47.25%	5.429%




Sum of corrected areas: 112158382

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020525\
Data File : BP023936.D
Acq On : 05 Feb 2025 15:03
Operator : RC/JU
Sample : Q1226-10
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCZP5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

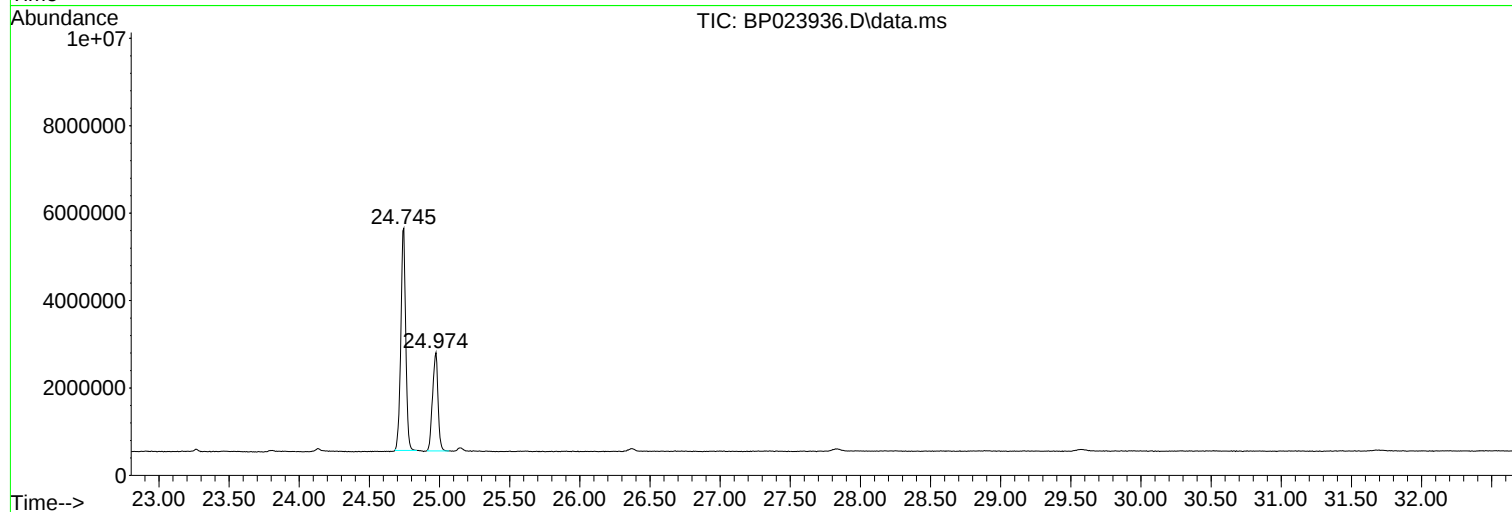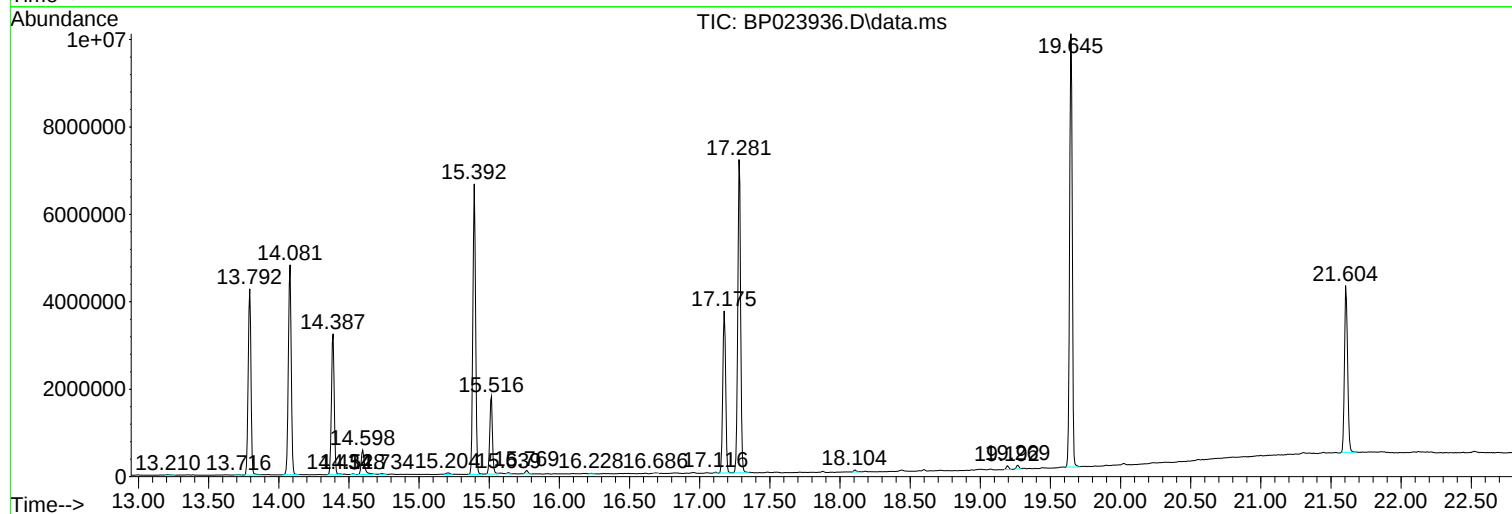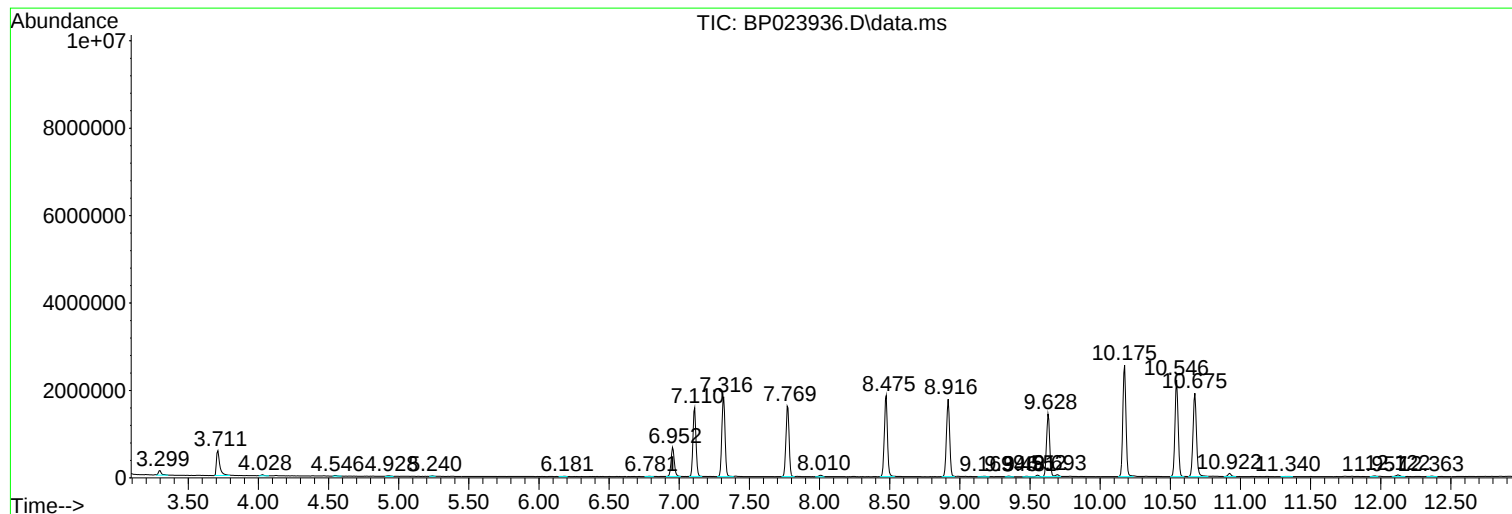

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020525\
Data File : BP023936.D
Acq On : 05 Feb 2025 15:03
Operator : RC/JU
Sample : Q1226-10
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCZP5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020525\
Data File : BP023936.D
Acq On : 05 Feb 2025 15:03
Operator : RC/JU
Sample : Q1226-10
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCZP5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc