

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020525\
 Data File : BP023945.D
 Acq On : 05 Feb 2025 21:07
 Operator : RC/JU
 Sample : Q1226-13
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCZN3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP023945.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.263	26	30	32	rBV	63132	76687	0.61%	0.060%
2	3.293	32	35	42	rVB	94073	121882	0.96%	0.095%
3	3.705	101	105	119	rBV	355994	622078	4.92%	0.486%
4	4.022	155	159	165	rVB	20904	32374	0.26%	0.025%
5	4.546	242	248	260	rVB	1096108	1541030	12.18%	1.203%
6	4.928	308	313	318	rBV3	16987	30291	0.24%	0.024%
7	5.128	339	347	355	rVB	93385	148058	1.17%	0.116%
8	6.287	539	544	549	rVB2	9141	12876	0.10%	0.010%
9	6.787	624	629	635	rVB8	6121	13141	0.10%	0.010%
10	6.951	648	657	670	rBV	587232	901328	7.13%	0.704%
11	7.104	676	683	694	rBV	1609663	2409780	19.05%	1.882%
12	7.310	711	718	729	rBV	1795741	2765243	21.86%	2.159%
13	7.769	789	796	810	rVB	1539238	2506250	19.81%	1.957%
14	8.122	850	856	864	rVB	129178	208685	1.65%	0.163%
15	8.198	864	869	875	rVB8	8902	15972	0.13%	0.012%
16	8.475	908	916	930	rBV	1692820	2610160	20.63%	2.038%
17	8.916	984	991	1004	rVB	1722699	2906652	22.98%	2.270%
18	9.169	1027	1034	1039	rBV3	6660	12940	0.10%	0.010%
19	9.345	1060	1064	1071	rVB6	9738	17687	0.14%	0.014%
20	9.628	1103	1112	1129	rBV	1382839	2345872	18.55%	1.832%
21	9.787	1133	1139	1148	rBV	25018	54503	0.43%	0.043%
22	10.169	1195	1204	1222	rBV	2417293	3984519	31.50%	3.111%
23	10.539	1257	1267	1282	rBV	2185359	3714012	29.36%	2.900%
24	10.675	1282	1290	1304	rBV	1942398	3142029	24.84%	2.454%
25	11.175	1367	1375	1383	rBV	10657	22065	0.17%	0.017%
26	11.334	1395	1402	1409	rBV	8962	24252	0.19%	0.019%
27	11.951	1499	1507	1513	rVB	5657	16890	0.13%	0.013%
28	12.086	1522	1530	1531	rBV7	6964	13643	0.11%	0.011%
29	12.122	1531	1536	1542	rVB	31459	53513	0.42%	0.042%
30	13.169	1707	1714	1716	rBV7	7254	13278	0.10%	0.010%
31	13.786	1812	1819	1833	rBV	4476614	6086386	48.12%	4.753%
32	14.075	1859	1868	1885	rBV	5464824	7304816	57.75%	5.704%
33	14.380	1914	1920	1926	rBV	3812208	4998807	39.52%	3.903%
34	14.427	1926	1928	1939	rVB	69096	119145	0.94%	0.093%
35	14.598	1950	1957	1974	rBV	480758	820088	6.48%	0.640%
36	14.739	1978	1981	1986	rVV7	13674	24440	0.19%	0.019%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020525\
Data File : BP023945.D
Acq On : 05 Feb 2025 21:07
Operator : RC/JU
Sample : Q1226-13
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCZN3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Title : SVOA CALIBRATION

37	14.798	1986	1991	1998	rVB6	13208	28529	0.23%	0.022%
38	14.933	2007	2014	2019	rBV	106569	151888	1.20%	0.119%
39	14.986	2019	2023	2025	rVV5	15742	22973	0.18%	0.018%
40	15.022	2025	2029	2033	rVB	44325	61238	0.48%	0.048%
41	15.210	2056	2061	2066	rVB2	23552	39341	0.31%	0.031%
42	15.392	2085	2092	2104	rBV	6692226	9613933	76.00%	7.507%
43	15.504	2105	2111	2121	rBV	1732306	2449361	19.36%	1.913%
44	15.633	2129	2133	2142	rVB3	34693	68121	0.54%	0.053%
45	15.969	2186	2190	2196	rVB6	8265	14800	0.12%	0.012%
46	16.227	2231	2234	2239	rBV7	13496	18288	0.14%	0.014%
47	16.533	2282	2286	2290	rVB7	9419	12652	0.10%	0.010%
48	16.821	2328	2335	2354	rBV	8982546	11830116	93.52%	9.238%
49	17.180	2389	2396	2405	rBV	4228958	5797986	45.84%	4.528%
50	17.274	2405	2412	2431	rVB	8255002	10889566	86.09%	8.503%
51	17.539	2454	2457	2463	rBV5	16119	30623	0.24%	0.024%
52	17.816	2500	2504	2509	rVV5	40111	54903	0.43%	0.043%
53	17.868	2510	2513	2518	rVB6	26503	36547	0.29%	0.029%
54	18.110	2551	2554	2559	rBV5	23415	32138	0.25%	0.025%
55	19.192	2734	2738	2742	rVB2	73195	94597	0.75%	0.074%
56	19.263	2746	2750	2755	rBV	71370	105848	0.84%	0.083%
57	19.645	2809	2815	2824	rBV	9268470	12649524	100.00%	9.878%
58	21.615	3144	3150	3158	rBV	4277943	6150532	48.62%	4.803%
59	24.745	3672	3682	3708	rVB	4824942	12012269	94.96%	9.380%
60	24.980	3713	3722	3736	rVB2	2304577	6203113	49.04%	4.844%




Sum of corrected areas: 128060258

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020525\
Data File : BP023945.D
Acq On : 05 Feb 2025 21:07
Operator : RC/JU
Sample : Q1226-13
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCZN3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

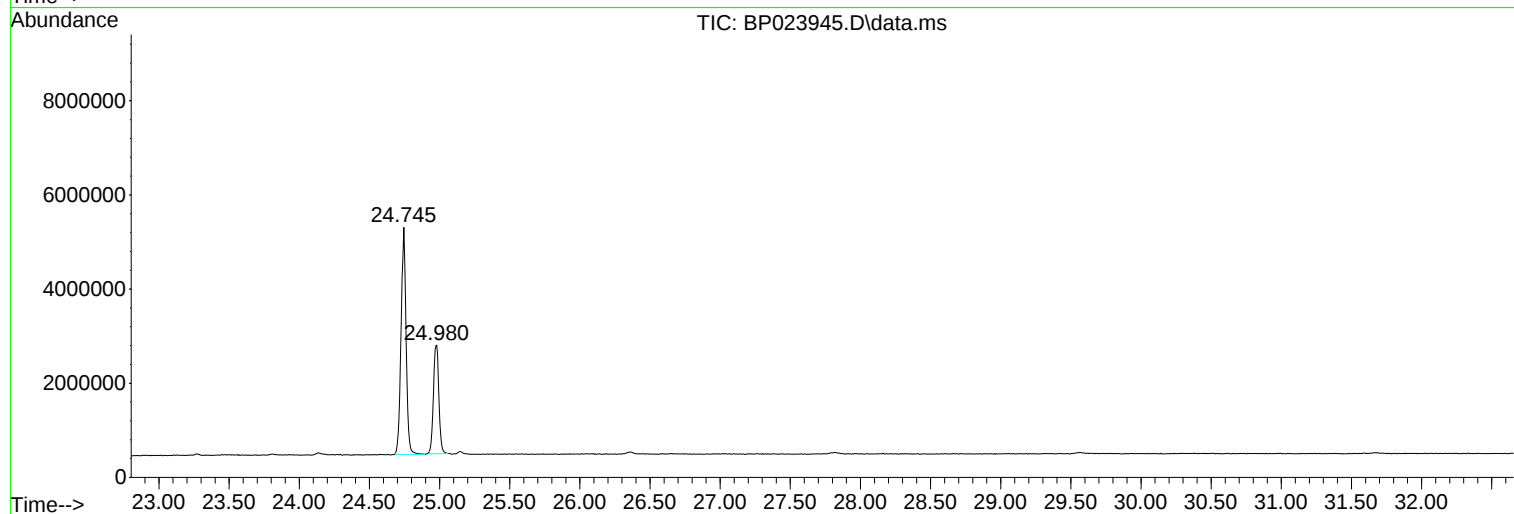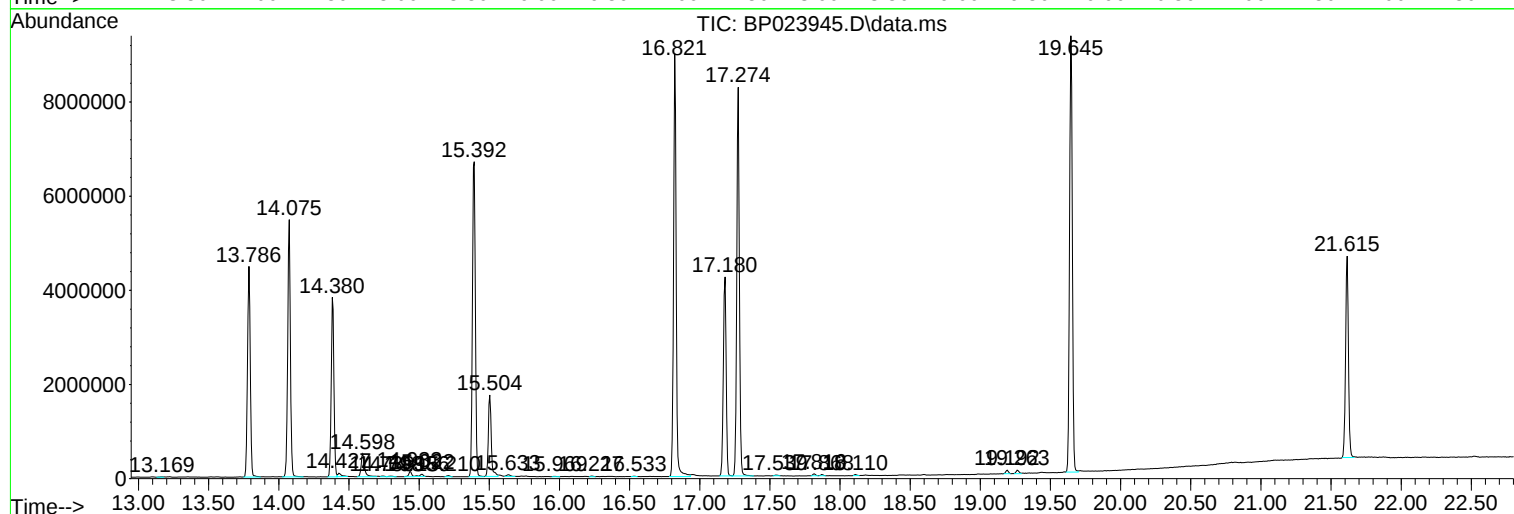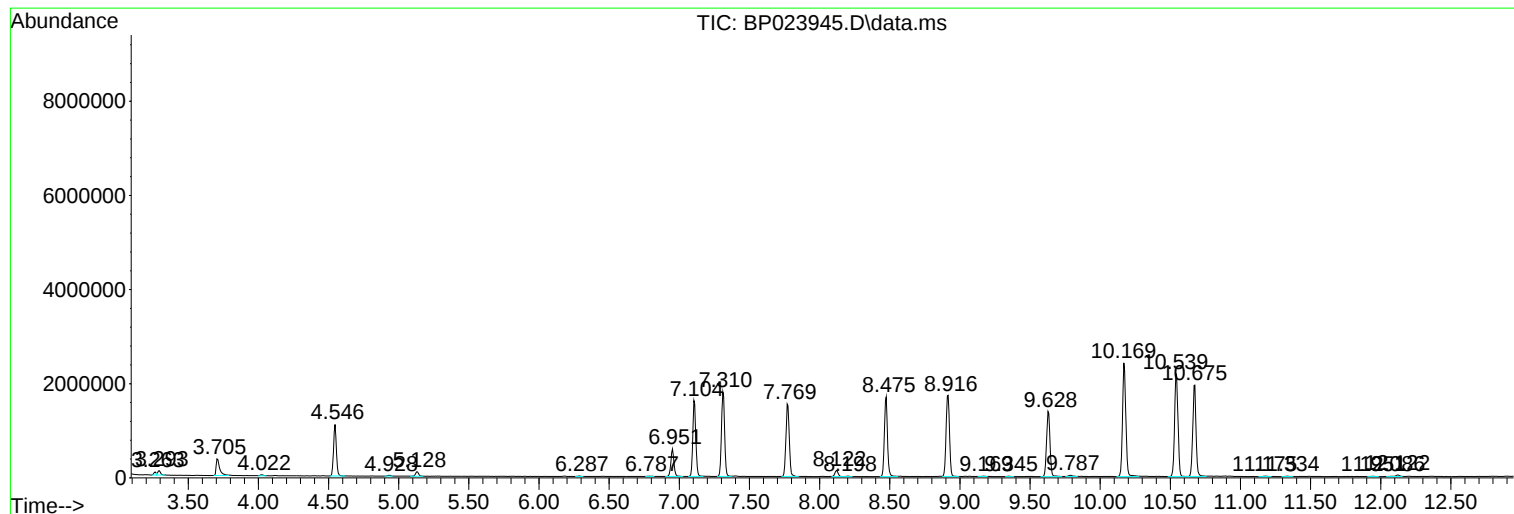

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020525\
Data File : BP023945.D
Acq On : 05 Feb 2025 21:07
Operator : RC/JU
Sample : Q1226-13
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCZN3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020525\
Data File : BP023945.D
Acq On : 05 Feb 2025 21:07
Operator : RC/JU
Sample : Q1226-13
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCZN3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc