

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020525\
 Data File : BP023947.D
 Acq On : 05 Feb 2025 22:28
 Operator : RC/JU
 Sample : Q1226-14
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCZP2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP023947.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.293	31	35	39	rBV	91488	113883	0.99%	0.105%
2	3.711	102	106	119	rBV	260080	439580	3.81%	0.406%
3	4.022	156	159	166	rVB	24041	30851	0.27%	0.028%
4	4.464	231	234	240	rVB3	8858	12421	0.11%	0.011%
5	4.934	308	314	318	rVB2	23591	40017	0.35%	0.037%
6	5.234	361	365	369	rBV5	13277	21537	0.19%	0.020%
7	5.381	385	390	399	rVB7	16364	32537	0.28%	0.030%
8	5.728	444	449	455	rVB4	12194	20991	0.18%	0.019%
9	6.540	582	587	595	rBV	31005	50804	0.44%	0.047%
10	6.952	649	657	667	rBV	698957	1106343	9.60%	1.022%
11	7.105	677	683	696	rVB	1393876	2127404	18.46%	1.965%
12	7.311	711	718	728	rBV	1799739	2705426	23.48%	2.498%
13	7.399	730	733	738	rVB4	9176	13084	0.11%	0.012%
14	7.769	788	796	805	rBV	1448318	2278793	19.77%	2.104%
15	7.834	805	807	814	rVB6	11049	17539	0.15%	0.016%
16	8.005	826	836	846	rBV	962582	1625118	14.10%	1.501%
17	8.240	864	876	882	rVB	34623	62717	0.54%	0.058%
18	8.469	908	915	927	rBV	1869185	2939470	25.51%	2.715%
19	8.822	969	975	979	rBV8	8035	16681	0.14%	0.015%
20	8.910	979	990	999	rVV	1585575	2771695	24.05%	2.560%
21	8.987	999	1003	1006	rVV5	10263	18524	0.16%	0.017%
22	9.034	1006	1011	1015	rVB5	9666	16642	0.14%	0.015%
23	9.169	1024	1034	1041	rBV8	15637	44488	0.39%	0.041%
24	9.293	1048	1055	1060	rVV7	9663	22285	0.19%	0.021%
25	9.352	1060	1065	1072	rVB3	16090	25666	0.22%	0.024%
26	9.475	1081	1086	1090	rBV3	24935	44186	0.38%	0.041%
27	9.552	1095	1099	1104	rVV	31466	47043	0.41%	0.043%
28	9.628	1104	1112	1119	rVV	1498860	2368034	20.55%	2.187%
29	9.693	1119	1123	1130	rVV2	31803	61312	0.53%	0.057%
30	9.787	1134	1139	1148	rVB3	23967	48132	0.42%	0.044%
31	9.899	1154	1158	1164	rVB9	12625	21230	0.18%	0.020%
32	10.081	1182	1189	1196	rBV3	70810	120986	1.05%	0.112%
33	10.169	1196	1204	1212	rBV	2442170	4051052	35.15%	3.741%
34	10.540	1260	1267	1275	rBV	2202245	3407399	29.57%	3.147%
35	10.599	1275	1277	1282	rVB6	8562	12585	0.11%	0.012%
36	10.675	1282	1290	1303	rBV	633404	1095842	9.51%	1.012%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020525\
 Data File : BP023947.D
 Acq On : 05 Feb 2025 22:28
 Operator : RC/JU
 Sample : Q1226-14
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCZP2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
 Title : SVOA CALIBRATION

37	10.781	1303	1308	1314	rBV	27981	49894	0.43%	0.046%
38	10.922	1322	1332	1339	rVB2	50103	103514	0.90%	0.096%
39	11.081	1352	1359	1369	rBV9	13711	34308	0.30%	0.032%
40	11.463	1415	1424	1437	rBV3	135784	361459	3.14%	0.334%
41	11.699	1454	1464	1468	rBV3	9109	25268	0.22%	0.023%
42	11.793	1475	1480	1486	rBV	32325	54193	0.47%	0.050%
43	11.957	1500	1508	1512	rBV	50283	91864	0.80%	0.085%
44	11.993	1512	1514	1523	rVV5	26491	45936	0.40%	0.042%
45	12.122	1525	1536	1544	rVV4	43467	122614	1.06%	0.113%
46	12.193	1544	1548	1554	rVV7	14523	29847	0.26%	0.028%
47	12.257	1555	1559	1566	rVB9	7501	18744	0.16%	0.017%
48	12.440	1584	1590	1594	rVB5	11318	19408	0.17%	0.018%
49	12.904	1664	1669	1675	rBV6	17415	37003	0.32%	0.034%
50	13.046	1689	1693	1697	rVV	31414	42695	0.37%	0.039%
51	13.098	1698	1702	1706	rVB2	18212	25033	0.22%	0.023%
52	13.222	1717	1723	1727	rBV6	11925	20666	0.18%	0.019%
53	13.293	1730	1735	1738	rBV7	8596	15817	0.14%	0.015%
54	13.569	1777	1782	1783	rBV5	11429	13721	0.12%	0.013%
55	13.793	1813	1820	1830	rBV	4098242	5716149	49.60%	5.279%
56	14.081	1862	1869	1882	rVB2	4640826	7024673	60.96%	6.487%
57	14.387	1915	1921	1931	rBV	3183852	4471884	38.80%	4.130%
58	14.598	1950	1957	1970	rBV	503521	925414	8.03%	0.855%
59	14.698	1971	1974	1978	rVV3	22810	34585	0.30%	0.032%
60	14.745	1979	1982	1987	rVB6	15599	24147	0.21%	0.022%
61	15.145	2045	2050	2055	rBV	116513	170187	1.48%	0.157%
62	15.216	2058	2062	2066	rVB2	25901	44838	0.39%	0.041%
63	15.392	2086	2092	2104	rBV	6322868	9005066	78.14%	8.316%
64	15.510	2106	2112	2119	rBV	1727434	2215609	19.23%	2.046%
65	15.634	2130	2133	2139	rVB5	30452	52741	0.46%	0.049%
66	15.763	2150	2155	2163	rBV	267398	390209	3.39%	0.360%
67	16.234	2231	2235	2241	rVB2	42003	60025	0.52%	0.055%
68	16.804	2330	2332	2333	rBV2	16663	12442	0.11%	0.011%
69	17.181	2389	2396	2403	rBV	3527828	5231110	45.39%	4.831%
70	17.281	2407	2413	2424	rVV	6984268	9868304	85.63%	9.113%
71	17.545	2454	2458	2466	rBV2	75246	111261	0.97%	0.103%
72	17.881	2512	2515	2520	rVB3	45250	56645	0.49%	0.052%
73	18.110	2550	2554	2561	rBV2	94765	162450	1.41%	0.150%
74	19.192	2735	2738	2743	rVB	75678	99998	0.87%	0.092%
75	19.269	2747	2751	2755	rVV	70014	99315	0.86%	0.092%
76	19.645	2809	2815	2824	rBV	8240863	11524048	100.00%	10.642%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020525\
Data File : BP023947.D
Acq On : 05 Feb 2025 22:28
Operator : RC/JU
Sample : Q1226-14
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCZP2

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Title : SVOA CALIBRATION

77	21.610	3143	3149	3159	rBV2	3470019	5632611	48.88%	5.202%
78	24.733	3671	3680	3697	rVB	4333199	10682852	92.70%	9.865%
79	24.974	3711	3721	3739	rVB	1988524	5726322	49.69%	5.288%




Sum of corrected areas: 108287166

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020525\
Data File : BP023947.D
Acq On : 05 Feb 2025 22:28
Operator : RC/JU
Sample : Q1226-14
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCZP2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

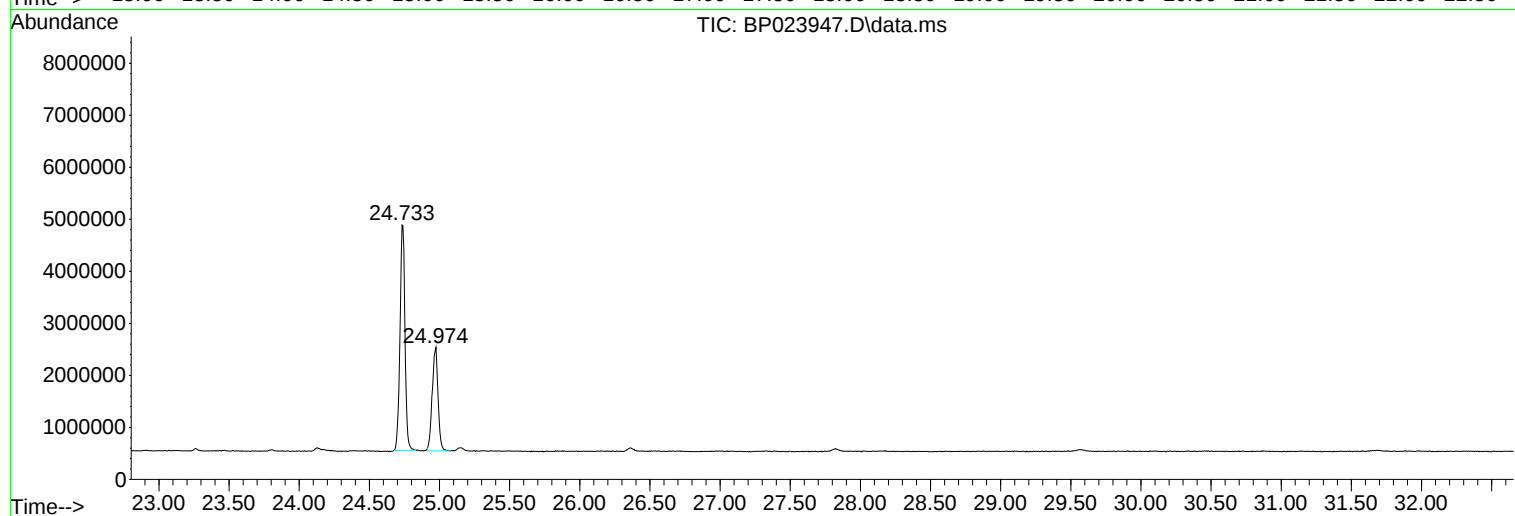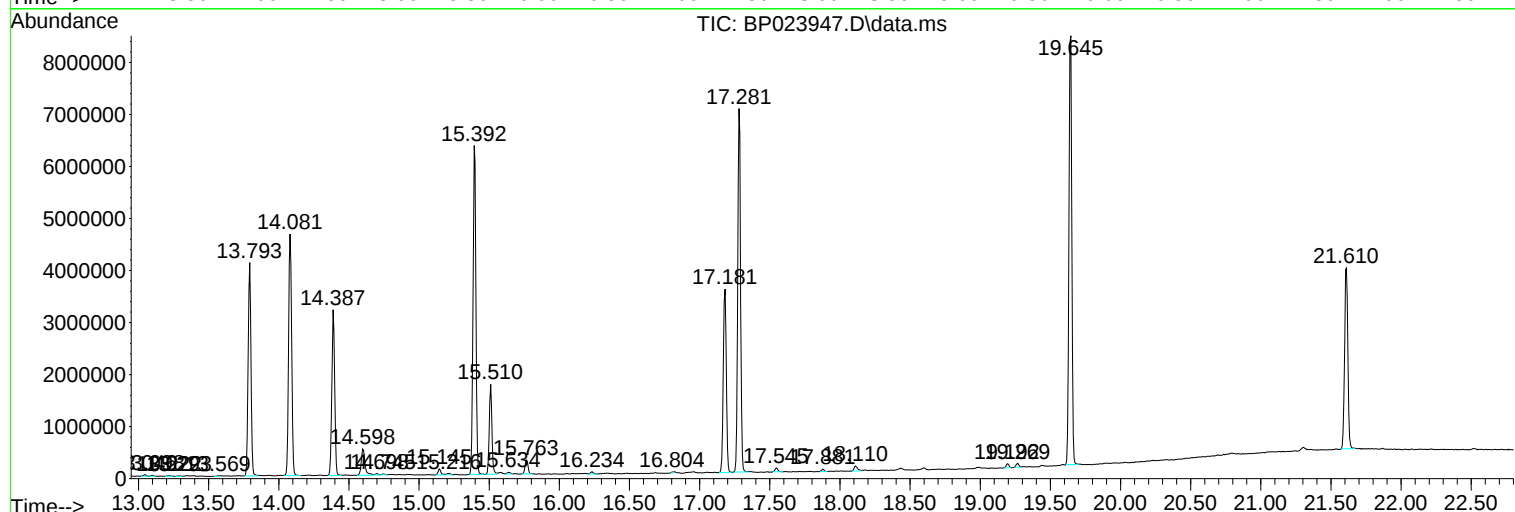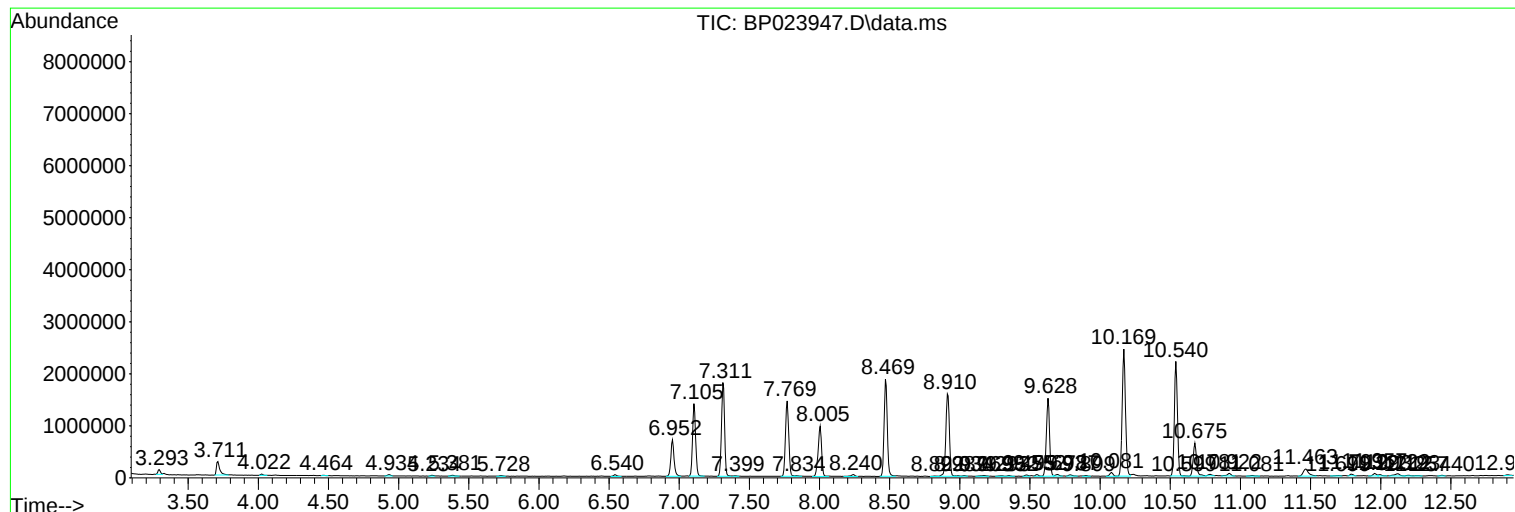

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020525\
Data File : BP023947.D
Acq On : 05 Feb 2025 22:28
Operator : RC/JU
Sample : Q1226-14
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCZP2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020525\
Data File : BP023947.D
Acq On : 05 Feb 2025 22:28
Operator : RC/JU
Sample : Q1226-14
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCZP2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc