

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020525\
 Data File : BP023958.D
 Acq On : 06 Feb 2025 06:33
 Operator : RC/JU
 Sample : Q1202-12
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E29A3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP023958.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.293	31	35	43	rVB	103276	143767	0.99%	0.106%
2	3.705	101	105	118	rBV	379724	609991	4.19%	0.449%
3	4.022	155	159	163	rBV	28300	40066	0.28%	0.030%
4	4.464	230	234	243	rVB	26739	38149	0.26%	0.028%
5	4.928	307	313	320	rBV2	100283	154202	1.06%	0.114%
6	6.958	647	658	669	rBV	711778	1169483	8.03%	0.861%
7	7.105	675	683	695	rBV	1941932	3027703	20.79%	2.230%
8	7.311	711	718	730	rBV	2379564	3539649	24.30%	2.607%
9	7.399	730	733	743	rVB5	11544	21382	0.15%	0.016%
10	7.769	786	796	803	rBV	1624901	2542104	17.45%	1.873%
11	8.187	864	867	875	rVB2	10953	17853	0.12%	0.013%
12	8.475	907	916	930	rBV	2058917	3385085	23.24%	2.494%
13	8.910	983	990	999	rBV	2367665	3776942	25.93%	2.782%
14	9.040	1008	1012	1019	rBV5	10002	17229	0.12%	0.013%
15	9.346	1056	1064	1071	rBV3	18406	31974	0.22%	0.024%
16	9.628	1104	1112	1125	rBV	1920628	3228334	22.17%	2.378%
17	10.175	1197	1205	1217	rBV	3145687	5232711	35.93%	3.855%
18	10.540	1261	1267	1275	rVB	2225580	3870064	26.57%	2.851%
19	10.675	1283	1290	1303	rBV	2255349	3905363	26.81%	2.877%
20	11.346	1399	1404	1410	rBV10	8707	21370	0.15%	0.016%
21	11.893	1492	1497	1503	rVB	32808	51904	0.36%	0.038%
22	12.128	1531	1537	1543	rBV2	46548	80981	0.56%	0.060%
23	12.581	1605	1614	1617	rBV9	11068	23987	0.16%	0.018%
24	12.651	1619	1626	1629	rBV8	6096	15111	0.10%	0.011%
25	12.751	1638	1643	1654	rVB8	15861	48899	0.34%	0.036%
26	12.993	1681	1684	1688	rBV5	9992	15497	0.11%	0.011%
27	13.116	1696	1705	1708	rBV5	14619	35611	0.24%	0.026%
28	13.222	1710	1723	1733	rVB2	66099	221085	1.52%	0.163%
29	13.569	1774	1782	1785	rVV6	23201	62101	0.43%	0.046%
30	13.598	1785	1787	1797	rVB2	28870	50953	0.35%	0.038%
31	13.798	1811	1821	1830	rBV	5365007	7548045	51.82%	5.560%
32	13.910	1838	1840	1852	rVB	9029	20864	0.14%	0.015%
33	14.081	1861	1869	1885	rBV	6484988	9689236	66.52%	7.137%
34	14.387	1914	1921	1933	rBV	3655607	5446099	37.39%	4.012%
35	14.616	1951	1960	1974	rBV	490800	931984	6.40%	0.687%
36	14.751	1979	1983	1988	rVV6	16360	32014	0.22%	0.024%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020525\
 Data File : BP023958.D
 Acq On : 06 Feb 2025 06:33
 Operator : RC/JU
 Sample : Q1202-12
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E29A3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
 Title : SVOA CALIBRATION

37	14.810	1989	1993	1999	rVB8	14069	26618	0.18%	0.020%
38	15.063	2031	2036	2040	rVB7	10688	18379	0.13%	0.014%
39	15.216	2058	2062	2067	rVB3	16736	25523	0.18%	0.019%
40	15.392	2084	2092	2106	rBV	8190607	11882809	81.59%	8.753%
41	15.510	2106	2112	2127	rVV	2108166	2966375	20.37%	2.185%
42	15.628	2129	2132	2139	rVB	35837	61740	0.42%	0.045%
43	15.763	2150	2155	2161	rVB	130869	182095	1.25%	0.134%
44	16.339	2248	2253	2257	rBV	42670	57814	0.40%	0.043%
45	16.845	2336	2339	2346	rVB8	11447	18831	0.13%	0.014%
46	16.957	2355	2358	2364	rVB2	15105	24180	0.17%	0.018%
47	17.175	2388	2395	2406	rBV2	3870159	6125558	42.06%	4.512%
48	17.281	2406	2413	2423	rBV	9811465	12656942	86.90%	9.323%
49	18.110	2551	2554	2561	rBV4	24624	40494	0.28%	0.030%
50	19.198	2735	2739	2744	rBV2	110296	163858	1.13%	0.121%
51	19.275	2748	2752	2756	rVV	107318	142578	0.98%	0.105%
52	19.651	2810	2816	2825	rBV	10487035	14564806	100.00%	10.729%
53	21.610	3144	3149	3157	rVB2	4083636	6452844	44.30%	4.753%
54	24.751	3674	3683	3697	rVB	5831684	14358295	98.58%	10.577%
55	24.980	3714	3722	3738	rVB	2640548	6936840	47.63%	5.110%




Sum of corrected areas: 135754371

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020525\
Data File : BP023958.D
Acq On : 06 Feb 2025 06:33
Operator : RC/JU
Sample : Q1202-12
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E29A3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

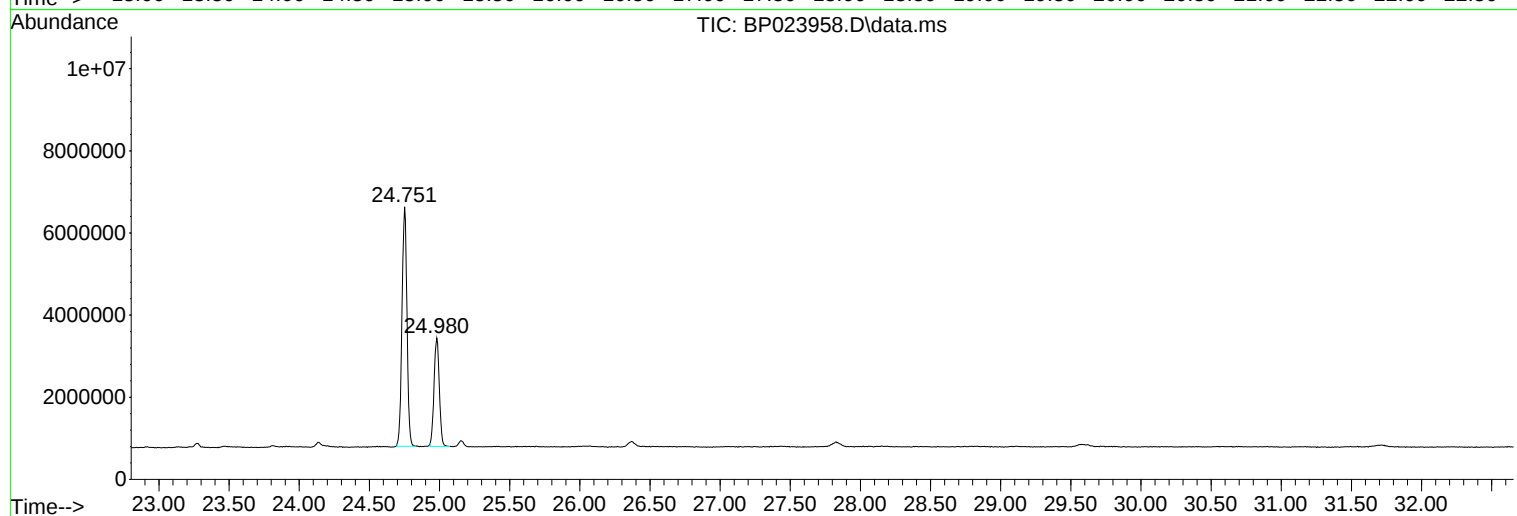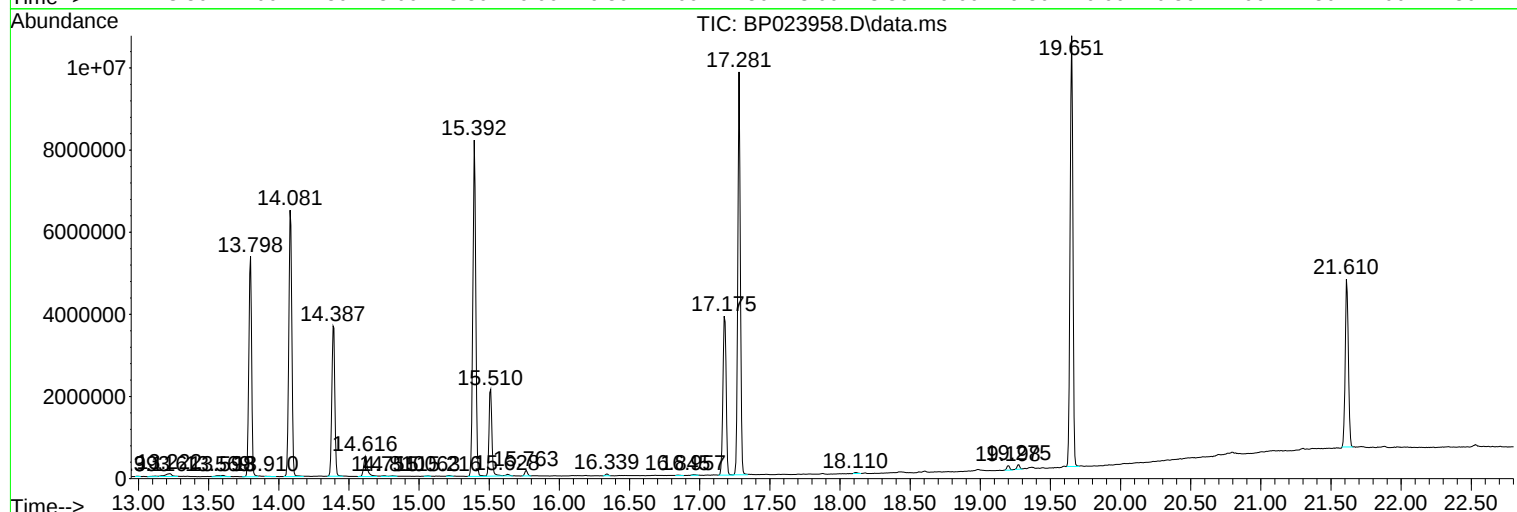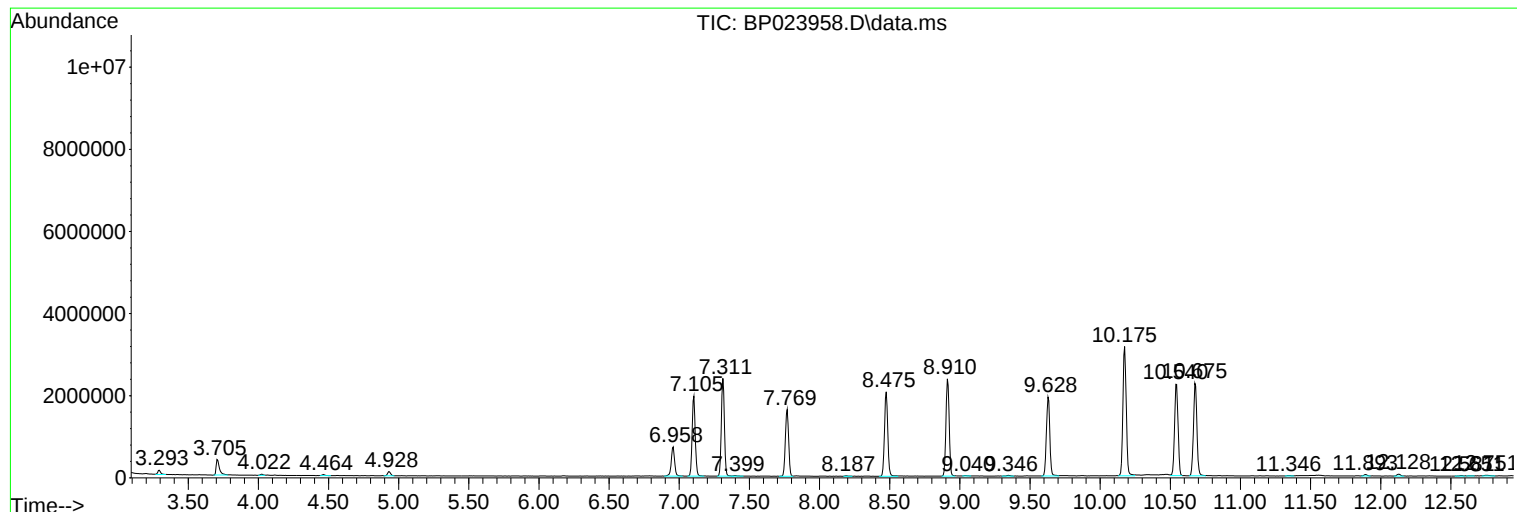

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020525\
Data File : BP023958.D
Acq On : 06 Feb 2025 06:33
Operator : RC/JU
Sample : Q1202-12
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E29A3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020525\
Data File : BP023958.D
Acq On : 06 Feb 2025 06:33
Operator : RC/JU
Sample : Q1202-12
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E29A3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------