

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020525\
 Data File : BP023970.D
 Acq On : 06 Feb 2025 14:39
 Operator : RC/JU
 Sample : Q1226-26
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCZP4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP023970.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.293	31	35	48	rVB	113732	157953	1.15%	0.131%
2	3.710	102	106	120	rBV	285403	491676	3.58%	0.407%
3	4.022	155	159	166	rBV	29381	40327	0.29%	0.033%
4	4.463	231	234	239	rVB	13284	16031	0.12%	0.013%
5	4.934	308	314	321	rVB2	34582	55132	0.40%	0.046%
6	6.957	649	658	669	rBV	674399	1049074	7.65%	0.868%
7	7.104	676	683	698	rBV	1689075	2603381	18.98%	2.155%
8	7.310	711	718	728	rBV	1939658	3036703	22.14%	2.514%
9	7.398	730	733	742	rVB3	11528	20136	0.15%	0.017%
10	7.769	789	796	805	rBV	1637388	2534810	18.48%	2.098%
11	7.846	805	809	816	rVB6	8290	17525	0.13%	0.015%
12	8.475	908	916	932	rBV	1859572	2941674	21.45%	2.435%
13	8.916	983	991	1001	rBV	1886344	3124974	22.78%	2.587%
14	9.345	1056	1064	1070	rVB2	29538	46386	0.34%	0.038%
15	9.475	1082	1086	1092	rBV7	10162	15921	0.12%	0.013%
16	9.628	1105	1112	1125	rBV	1544664	2590897	18.89%	2.145%
17	9.798	1132	1141	1149	rBV	32504	71525	0.52%	0.059%
18	10.175	1194	1205	1220	rBV	2645860	4335539	31.61%	3.589%
19	10.475	1251	1256	1260	rVB	15637	25077	0.18%	0.021%
20	10.539	1260	1267	1277	rBV	2369747	3826837	27.90%	3.168%
21	10.675	1282	1290	1307	rBV	524963	938100	6.84%	0.777%
22	11.886	1489	1496	1503	rBV	118686	209076	1.52%	0.173%
23	11.969	1505	1510	1515	rVB6	12024	22858	0.17%	0.019%
24	12.122	1529	1536	1542	rBV2	39256	67277	0.49%	0.056%
25	12.339	1569	1573	1582	rVB2	6641	14847	0.11%	0.012%
26	13.222	1717	1723	1732	rVB2	87875	154840	1.13%	0.128%
27	13.598	1777	1787	1791	rBV	34384	61814	0.45%	0.051%
28	13.639	1791	1794	1802	rVB4	13163	22026	0.16%	0.018%
29	13.792	1814	1820	1838	rBV	4681454	6482507	47.26%	5.367%
30	14.080	1858	1869	1879	rBV	5122693	7905382	57.64%	6.545%
31	14.392	1914	1922	1928	rBV	3687855	5173205	37.72%	4.283%
32	14.445	1928	1931	1949	rVB	95719	225234	1.64%	0.186%
33	14.616	1954	1960	1979	rVV	539318	1009856	7.36%	0.836%
34	14.751	1979	1983	1987	rVV7	12373	26003	0.19%	0.022%
35	14.816	1989	1994	1999	rVB9	10152	21142	0.15%	0.018%
36	15.204	2055	2060	2065	rBV4	13031	25070	0.18%	0.021%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020525\
 Data File : BP023970.D
 Acq On : 06 Feb 2025 14:39
 Operator : RC/JU
 Sample : Q1226-26
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCZP4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
 Title : SVOA CALIBRATION

37	15.398	2086	2093	2107	rBV	7552251	10165823	74.12%	8.416%
38	15.516	2107	2113	2127	rVV	2089407	2599914	18.96%	2.152%
39	15.633	2130	2133	2139	rVB	29572	50385	0.37%	0.042%
40	15.763	2150	2155	2163	rVB	165183	240183	1.75%	0.199%
41	16.827	2331	2336	2339	rBV5	19364	36598	0.27%	0.030%
42	16.963	2354	2359	2364	rVB	17308	28236	0.21%	0.023%
43	17.174	2389	2395	2406	rBV	4185740	6005105	43.78%	4.971%
44	17.280	2406	2413	2426	rBV	7958174	11755564	85.71%	9.732%
45	17.569	2458	2462	2466	rBV3	15359	25025	0.18%	0.021%
46	17.880	2512	2515	2519	rVB6	21031	24166	0.18%	0.020%
47	18.110	2551	2554	2563	rBV2	64180	91145	0.66%	0.075%
48	19.198	2735	2739	2744	rVB	91011	122169	0.89%	0.101%
49	19.268	2747	2751	2756	rBV	83334	126108	0.92%	0.104%
50	19.645	2809	2815	2826	rBV	9647001	13715500	100.00%	11.354%
51	21.621	3145	3151	3162	rVB	4265031	6360824	46.38%	5.266%
52	24.756	3674	3684	3703	rVB	5002010	13574480	98.97%	11.238%
53	24.992	3715	3724	3735	rVB	2402104	6512218	47.48%	5.391%




Sum of corrected areas: 120794258

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020525\
Data File : BP023970.D
Acq On : 06 Feb 2025 14:39
Operator : RC/JU
Sample : Q1226-26
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCZP4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

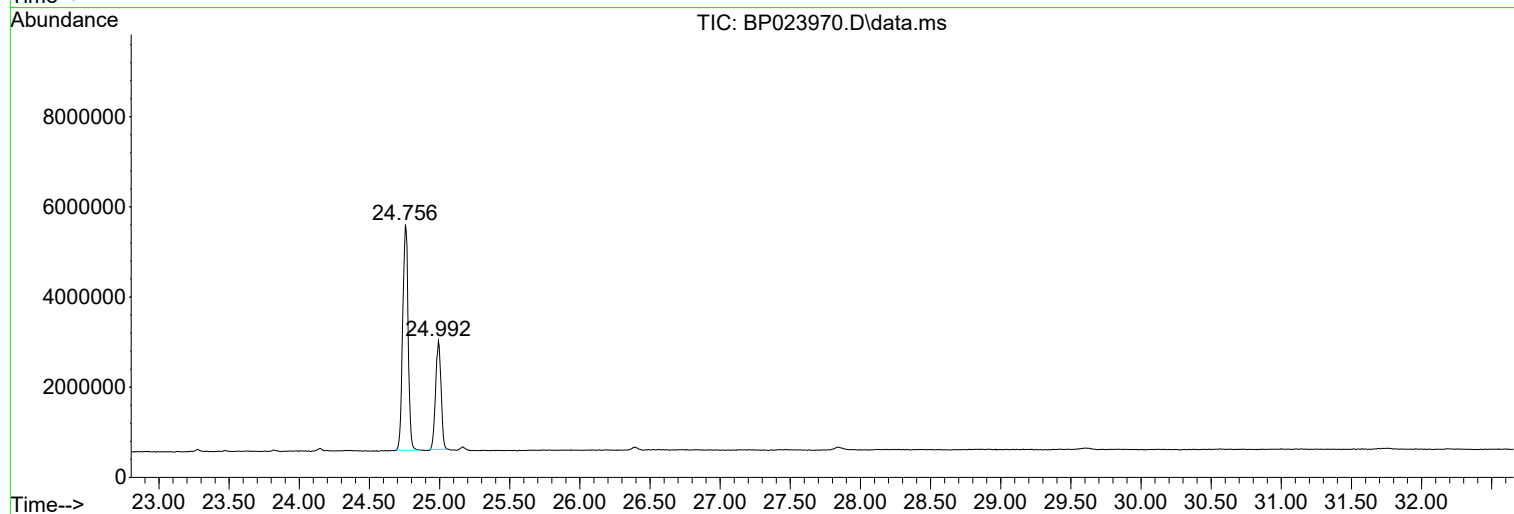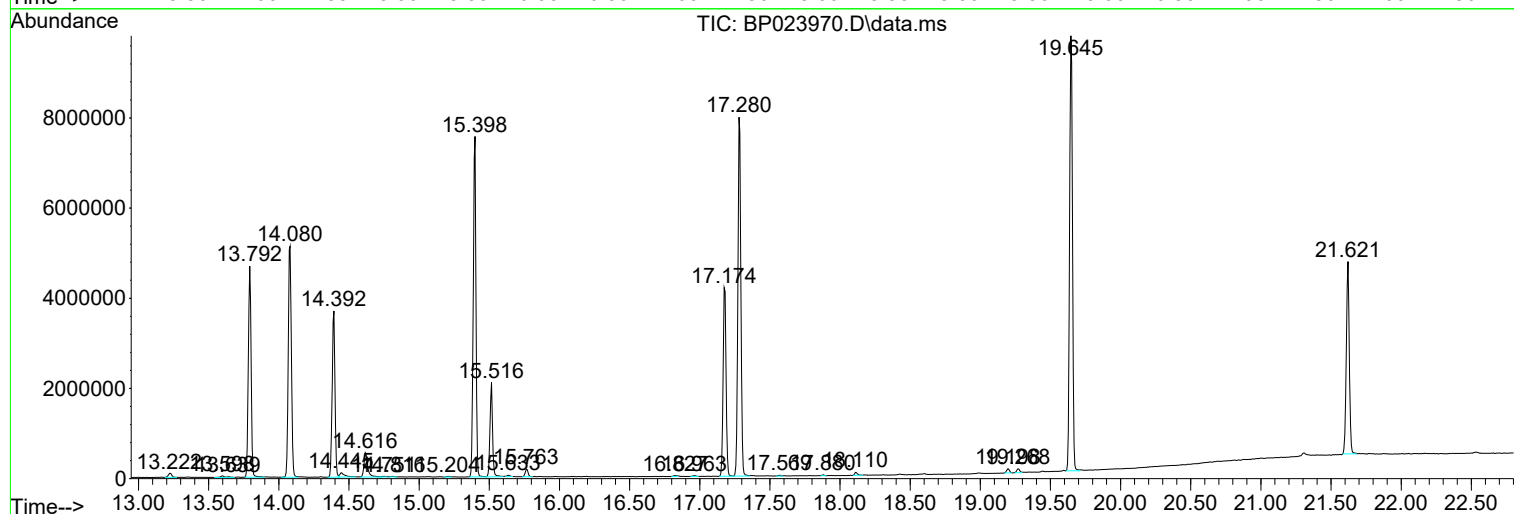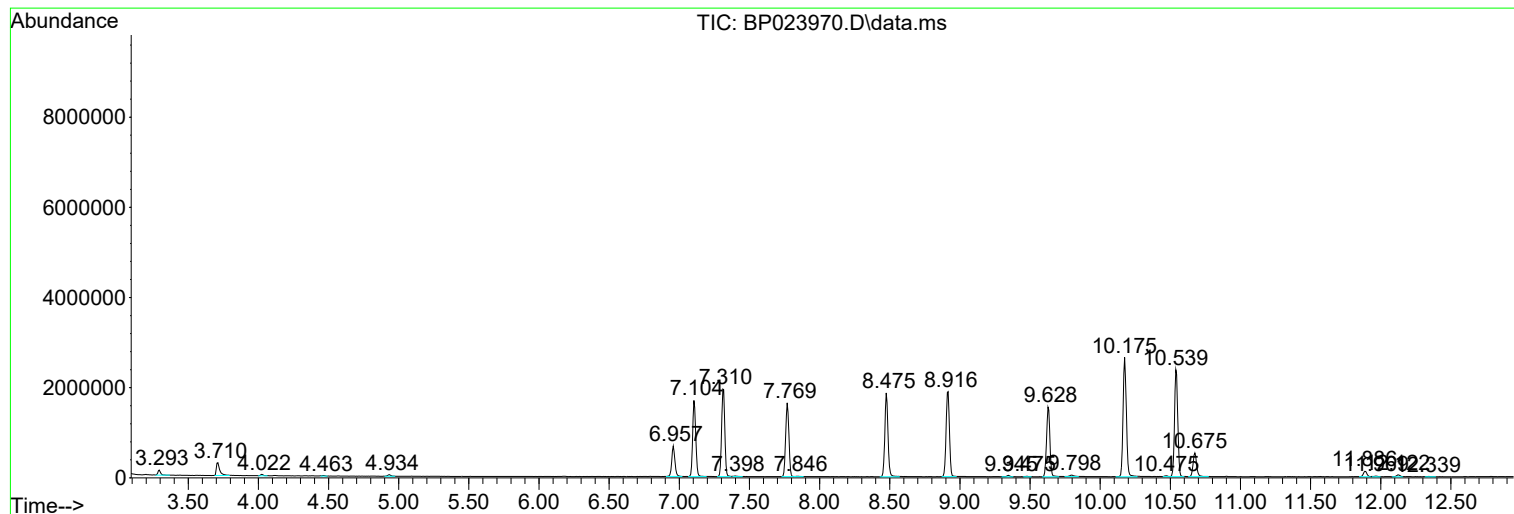

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020525\
Data File : BP023970.D
Acq On : 06 Feb 2025 14:39
Operator : RC/JU
Sample : Q1226-26
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCZP4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020525\
Data File : BP023970.D
Acq On : 06 Feb 2025 14:39
Operator : RC/JU
Sample : Q1226-26
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCZP4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------