

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020525\
 Data File : BP023971.D
 Acq On : 06 Feb 2025 15:19
 Operator : RC/JU
 Sample : Q1226-23
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCZN9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP023971.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	26	30	32	rBV	95769	122207	0.95%	0.097%
2	3.287	32	34	44	rVB	116632	155835	1.22%	0.124%
3	3.705	101	105	121	rBV	508810	788867	6.16%	0.628%
4	4.022	155	159	166	rVB	30362	44674	0.35%	0.036%
5	4.540	241	247	261	rVB	1731993	2474785	19.31%	1.969%
6	4.934	308	314	321	rBV2	55812	86235	0.67%	0.069%
7	5.128	344	347	354	rVB2	14124	21118	0.16%	0.017%
8	5.810	458	463	469	rVB	37534	53737	0.42%	0.043%
9	6.181	521	526	531	rVB5	7570	13748	0.11%	0.011%
10	6.281	536	543	548	rBV	38163	60535	0.47%	0.048%
11	6.769	619	626	629	rBV5	7214	15132	0.12%	0.012%
12	6.957	649	658	669	rBV	461164	729510	5.69%	0.580%
13	7.105	676	683	690	rBV	1521937	2323705	18.14%	1.849%
14	7.169	690	694	703	rVB	90065	135967	1.06%	0.108%
15	7.310	711	718	729	rBV	1764047	2667327	20.82%	2.122%
16	7.422	730	737	743	rVB	88152	146836	1.15%	0.117%
17	7.769	788	796	806	rBV	1660172	2561767	19.99%	2.038%
18	7.887	810	816	822	rVB	57516	86507	0.68%	0.069%
19	8.122	850	856	866	rVB2	28011	77427	0.60%	0.062%
20	8.410	900	905	909	rBV8	7134	14109	0.11%	0.011%
21	8.475	909	916	926	rBV	1534649	2307566	18.01%	1.836%
22	8.910	983	990	1003	rVB	1749781	2838597	22.15%	2.258%
23	9.628	1103	1112	1125	rBV	1437430	2322703	18.13%	1.848%
24	9.793	1135	1140	1149	rVB2	14623	31595	0.25%	0.025%
25	9.975	1164	1171	1183	rBV2	27319	65579	0.51%	0.052%
26	10.175	1195	1205	1213	rBV	2290369	3913654	30.54%	3.114%
27	10.240	1213	1216	1228	rVB3	64057	128070	1.00%	0.102%
28	10.469	1250	1255	1260	rVB3	13319	21247	0.17%	0.017%
29	10.540	1260	1267	1274	rBV	2416171	3896506	30.41%	3.100%
30	10.593	1274	1276	1282	rVB	29287	36788	0.29%	0.029%
31	10.675	1282	1290	1308	rBV	2343858	3954819	30.86%	3.147%
32	10.922	1326	1332	1338	rVB7	11481	21220	0.17%	0.017%
33	11.151	1365	1371	1384	rBV	49076	126971	0.99%	0.101%
34	11.345	1397	1404	1410	rBV	9158	22257	0.17%	0.018%
35	11.569	1438	1442	1450	rVB4	7673	15159	0.12%	0.012%
36	11.663	1450	1458	1465	rBV4	5460	16732	0.13%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020525\
 Data File : BP023971.D
 Acq On : 06 Feb 2025 15:19
 Operator : RC/JU
 Sample : Q1226-23
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCZN9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
 Title : SVOA CALIBRATION

37	12.075	1522	1528	1532	rBV8	12798	23913	0.19%	0.019%
38	12.128	1532	1537	1544	rVB	37724	63127	0.49%	0.050%
39	12.363	1569	1577	1583	rVV6	15075	34369	0.27%	0.027%
40	12.422	1583	1587	1593	rVB7	10197	14321	0.11%	0.011%

41	12.716	1629	1637	1641	rBV7	6906	13189	0.10%	0.010%
42	12.816	1647	1654	1662	rVB2	38495	65236	0.51%	0.052%
43	12.898	1662	1668	1676	rBV	80543	124697	0.97%	0.099%
44	13.069	1691	1697	1701	rBV8	8195	14624	0.11%	0.012%
45	13.122	1701	1706	1712	rBV2	38046	70550	0.55%	0.056%

46	13.228	1719	1724	1730	rVB	148099	209642	1.64%	0.167%
47	13.351	1741	1745	1750	rVB3	8660	12917	0.10%	0.010%
48	13.428	1754	1758	1764	rVB9	9211	16511	0.13%	0.013%
49	13.592	1782	1786	1791	rVV	59887	79825	0.62%	0.064%
50	13.634	1791	1793	1801	rVB8	9331	13193	0.10%	0.010%

51	13.792	1814	1820	1835	rBV	4483372	6174539	48.19%	4.913%
52	14.081	1860	1869	1879	rBV	5156278	7404167	57.78%	5.891%
53	14.216	1888	1892	1902	rVB	15592	31859	0.25%	0.025%
54	14.392	1915	1922	1929	rBV	3745939	5381918	42.00%	4.282%
55	14.616	1954	1960	1970	rVV	376237	652749	5.09%	0.519%

56	14.798	1988	1991	1999	rVB5	23773	43950	0.34%	0.035%
57	14.945	2007	2016	2021	rBV	96599	159963	1.25%	0.127%
58	15.034	2022	2031	2036	rVV	296169	480219	3.75%	0.382%
59	15.145	2046	2050	2056	rVB4	9886	16255	0.13%	0.013%
60	15.210	2057	2061	2068	rVB2	21805	37238	0.29%	0.030%

61	15.398	2086	2093	2105	rBV	6954582	9673758	75.50%	7.697%
62	15.510	2105	2112	2117	rVV	1593407	2436869	19.02%	1.939%
63	15.557	2117	2120	2130	rVV2	353701	687668	5.37%	0.547%
64	15.651	2131	2136	2145	rVB2	58106	123908	0.97%	0.099%
65	16.239	2233	2236	2240	rVB6	10930	13227	0.10%	0.011%

66	16.833	2330	2337	2350	rBV	1658436	2559226	19.97%	2.036%
67	16.963	2354	2359	2364	rVB3	21812	53615	0.42%	0.043%
68	17.186	2390	2397	2408	rBV2	4316001	6396376	49.92%	5.089%
69	17.292	2408	2415	2434	rVB	7380516	10921045	85.23%	8.689%
70	17.827	2502	2506	2511	rBV4	40253	55304	0.43%	0.044%

71	17.880	2512	2515	2520	rVB6	20787	28807	0.22%	0.023%
72	18.122	2554	2556	2561	rVB6	18862	23146	0.18%	0.018%
73	19.204	2736	2740	2746	rBV3	87986	139936	1.09%	0.111%
74	19.280	2749	2753	2757	rVV	73665	104135	0.81%	0.083%
75	19.657	2811	2817	2827	rBV	9712545	12813364	100.00%	10.195%

76	21.627	3146	3152	3164	rBV	4536371	6873943	53.65%	5.469%
----	--------	------	------	------	-----	---------	---------	--------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020525\
Data File : BP023971.D
Acq On : 06 Feb 2025 15:19
Operator : RC/JU
Sample : Q1226-23
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCZN9

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Title : SVOA CALIBRATION

77	24.774	3676	3687	3703	rVB	4916725	12355581	96.43%	9.830%
78	24.998	3716	3725	3740	rVB	2449148	6988071	54.54%	5.560%




Sum of corrected areas: 125686441

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020525\
Data File : BP023971.D
Acq On : 06 Feb 2025 15:19
Operator : RC/JU
Sample : Q1226-23
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCZN9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

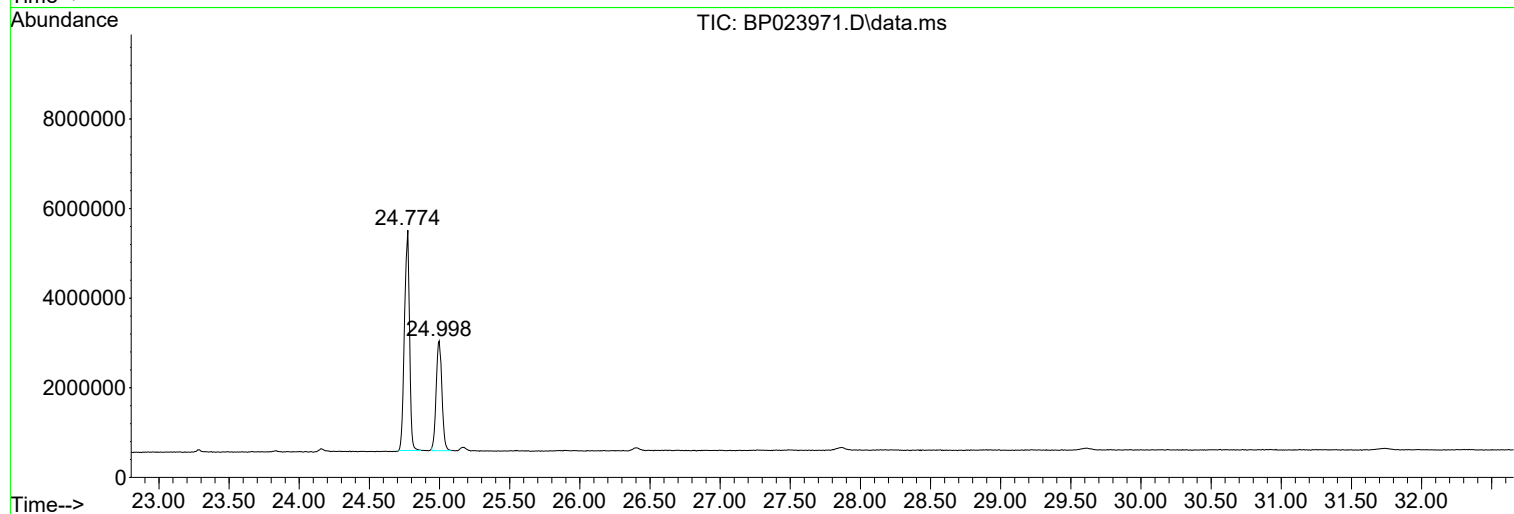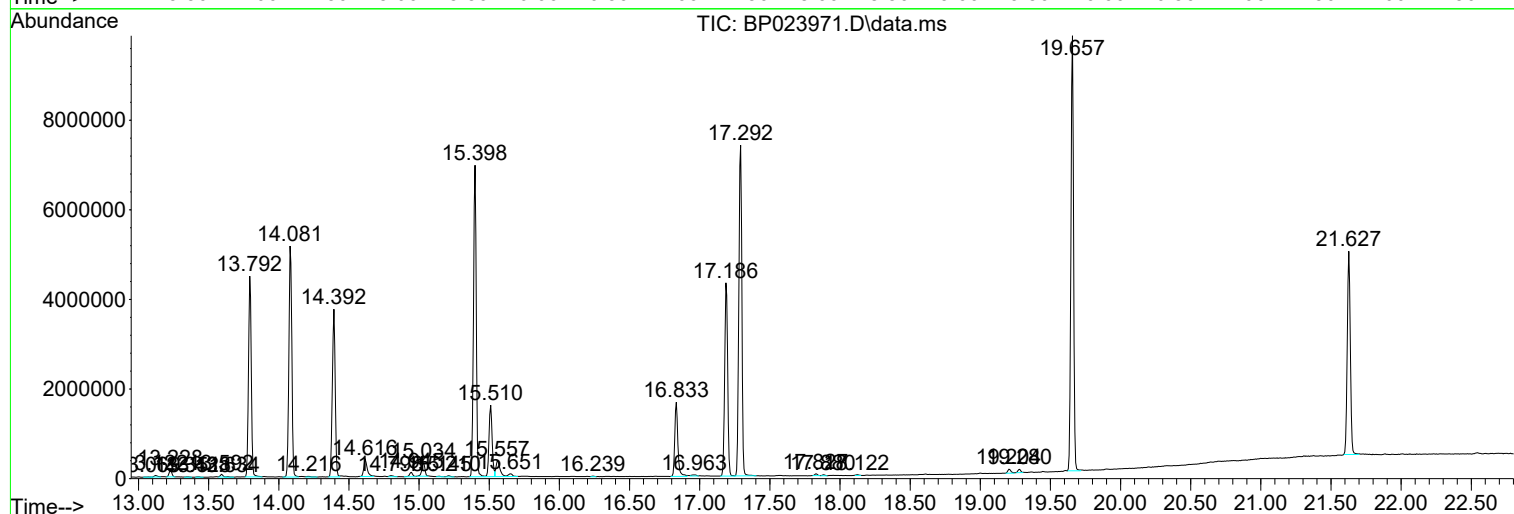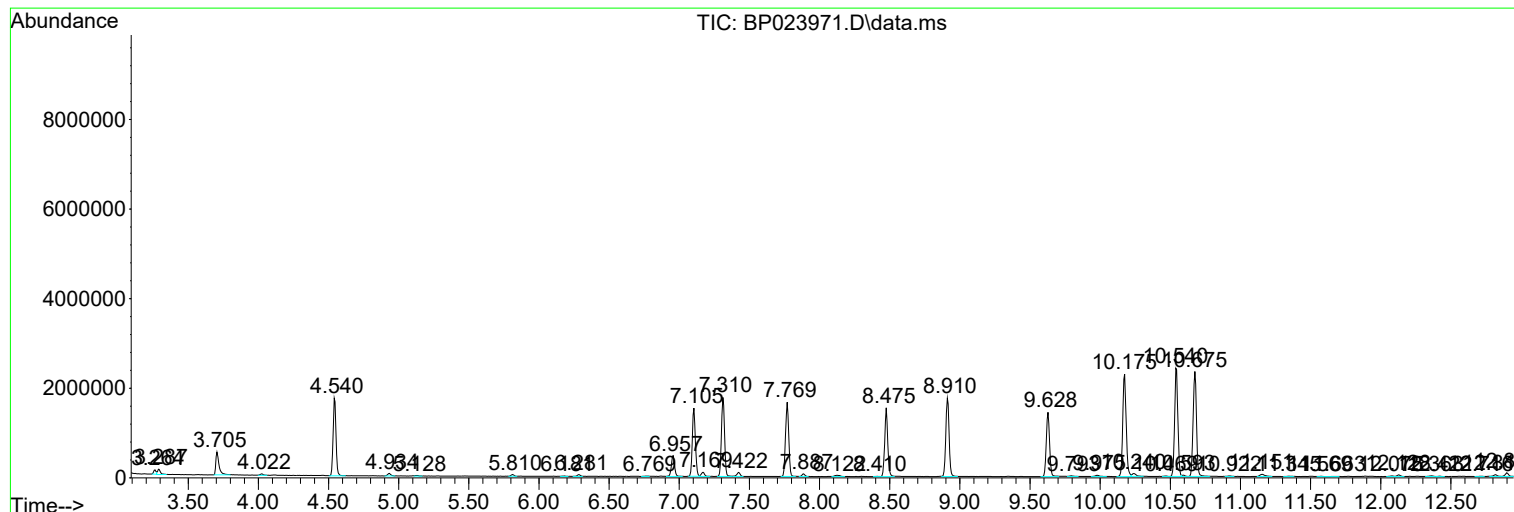

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020525\
Data File : BP023971.D
Acq On : 06 Feb 2025 15:19
Operator : RC/JU
Sample : Q1226-23
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCZN9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020525\
Data File : BP023971.D
Acq On : 06 Feb 2025 15:19
Operator : RC/JU
Sample : Q1226-23
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCZN9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc