

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020525\
 Data File : BP023979.D
 Acq On : 06 Feb 2025 20:43
 Operator : RC/JU
 Sample : Q1229-02
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E2991

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP023979.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.287	30	34	42	rVB	110022	153210	1.01%	0.117%
2	3.711	102	106	121	rBV	200408	348445	2.31%	0.265%
3	4.022	155	159	165	rBV	23845	30236	0.20%	0.023%
4	4.464	230	234	239	rVB	26294	36308	0.24%	0.028%
5	4.934	307	314	321	rBV2	36901	58643	0.39%	0.045%
6	6.958	648	658	670	rVB	591683	953145	6.31%	0.725%
7	7.105	676	683	697	rBV	1935187	2971611	19.68%	2.260%
8	7.316	711	719	729	rBV	2096013	3297603	21.84%	2.508%
9	7.769	788	796	804	rBV	1634267	2511666	16.64%	1.911%
10	7.840	804	808	814	rVB3	9281	16707	0.11%	0.013%
11	8.187	862	867	874	rVB	9331	15894	0.11%	0.012%
12	8.469	908	915	931	rBV	1832574	2962503	19.62%	2.254%
13	8.910	983	990	1000	rBV	2264623	3595981	23.82%	2.735%
14	9.346	1055	1064	1072	rBV	36648	57260	0.38%	0.044%
15	9.628	1103	1112	1128	rBV	1857362	2975350	19.71%	2.263%
16	10.175	1197	1205	1221	rBV	3066649	4886021	32.36%	3.717%
17	10.487	1252	1258	1260	rBV5	11247	18210	0.12%	0.014%
18	10.546	1260	1268	1280	rVB	2319995	3828610	25.36%	2.912%
19	10.675	1282	1290	1308	rBV	2153290	3652009	24.19%	2.778%
20	11.340	1399	1403	1413	rBV	9112	19920	0.13%	0.015%
21	11.834	1482	1487	1491	rBV	31608	44790	0.30%	0.034%
22	11.887	1491	1496	1502	rVV	40911	65077	0.43%	0.050%
23	12.128	1531	1537	1545	rVB2	44271	76355	0.51%	0.058%
24	12.998	1679	1685	1692	rVB2	19066	32397	0.21%	0.025%
25	13.793	1813	1820	1837	rBV	5048154	7334387	48.58%	5.579%
26	14.081	1860	1869	1879	rBV	5769330	8639967	57.23%	6.572%
27	14.387	1910	1921	1930	rBV	3469825	5216885	34.56%	3.968%
28	14.610	1953	1959	1975	rBV	415276	739978	4.90%	0.563%
29	14.745	1978	1982	1988	rVV2	21332	33448	0.22%	0.025%
30	14.822	1988	1995	2002	rVV3	33531	56235	0.37%	0.043%
31	15.392	2084	2092	2105	rBV	7956335	11502628	76.19%	8.750%
32	15.504	2105	2111	2126	rVV	2183101	2791228	18.49%	2.123%
33	15.628	2128	2132	2138	rVB2	36507	62581	0.41%	0.048%
34	16.098	2207	2212	2218	rBV8	14013	29259	0.19%	0.022%
35	16.187	2224	2227	2233	rVB7	13093	18654	0.12%	0.014%
36	16.963	2356	2359	2365	rVB2	16091	27107	0.18%	0.021%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020525\
 Data File : BP023979.D
 Acq On : 06 Feb 2025 20:43
 Operator : RC/JU
 Sample : Q1229-02
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E2991

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
 Title : SVOA CALIBRATION

37	17.063	2371	2376	2379	rBV4	15008	28738	0.19%	0.022%
38	17.181	2389	2396	2407	rBV2	3890459	6072207	40.22%	4.619%
39	17.287	2407	2414	2428	rBV	8488223	12753178	84.47%	9.701%
40	17.886	2513	2516	2521	rVB6	13436	16581	0.11%	0.013%
41	18.122	2551	2556	2561	rBV	91506	145441	0.96%	0.111%
42	18.451	2608	2612	2618	rBV6	24773	45230	0.30%	0.034%
43	19.210	2736	2741	2746	rBV	97047	144741	0.96%	0.110%
44	19.286	2749	2754	2759	rBV	91430	137487	0.91%	0.105%
45	19.457	2780	2783	2787	rBV	47635	57695	0.38%	0.044%
46	19.616	2807	2810	2812	rBV2	32726	40293	0.27%	0.031%
47	19.669	2812	2819	2828	rVV	11645068	15097164	100.00%	11.484%
48	19.910	2857	2860	2865	rVB	41290	52873	0.35%	0.040%
49	21.633	3147	3153	3165	rBV2	4168324	6540144	43.32%	4.975%
50	24.786	3679	3689	3703	rVB	6296436	14612955	96.79%	11.116%
51	24.998	3718	3725	3741	rVB	2613726	6656633	44.09%	5.064%




Sum of corrected areas: 131461668

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020525\
Data File : BP023979.D
Acq On : 06 Feb 2025 20:43
Operator : RC/JU
Sample : Q1229-02
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E2991

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

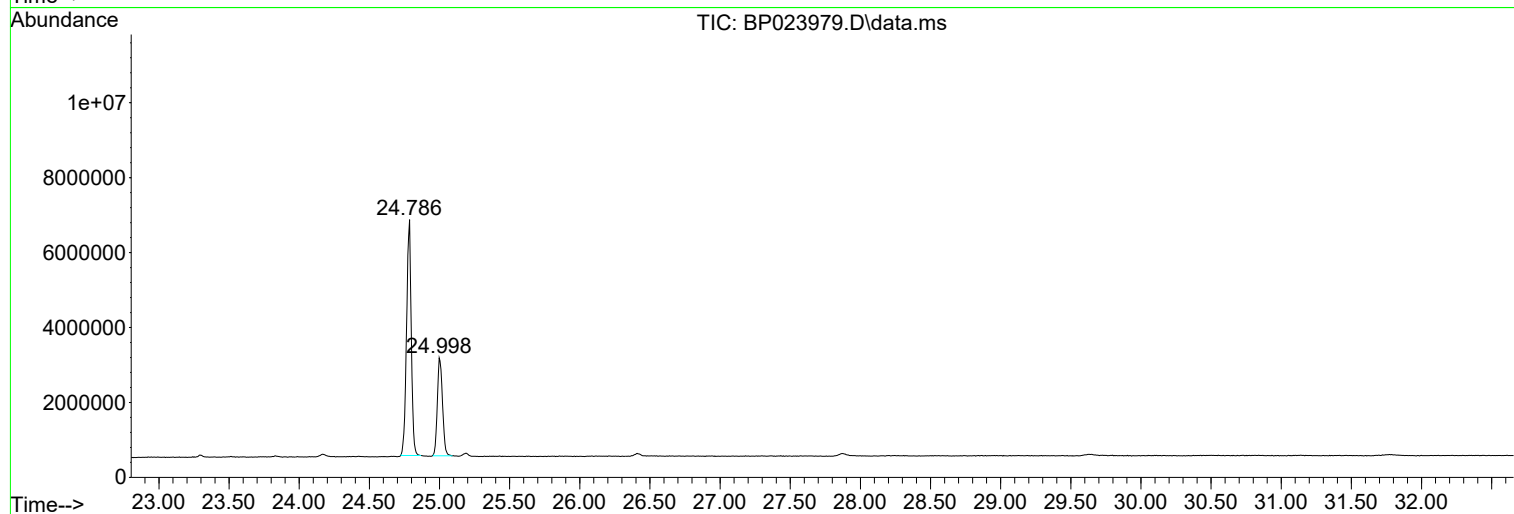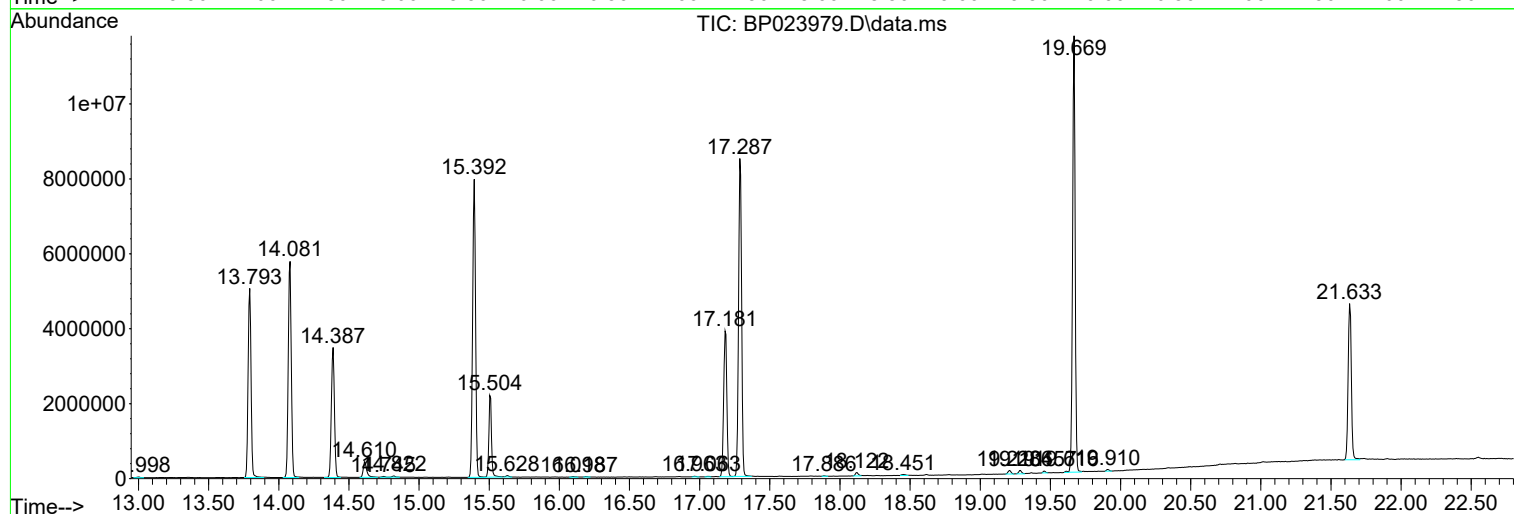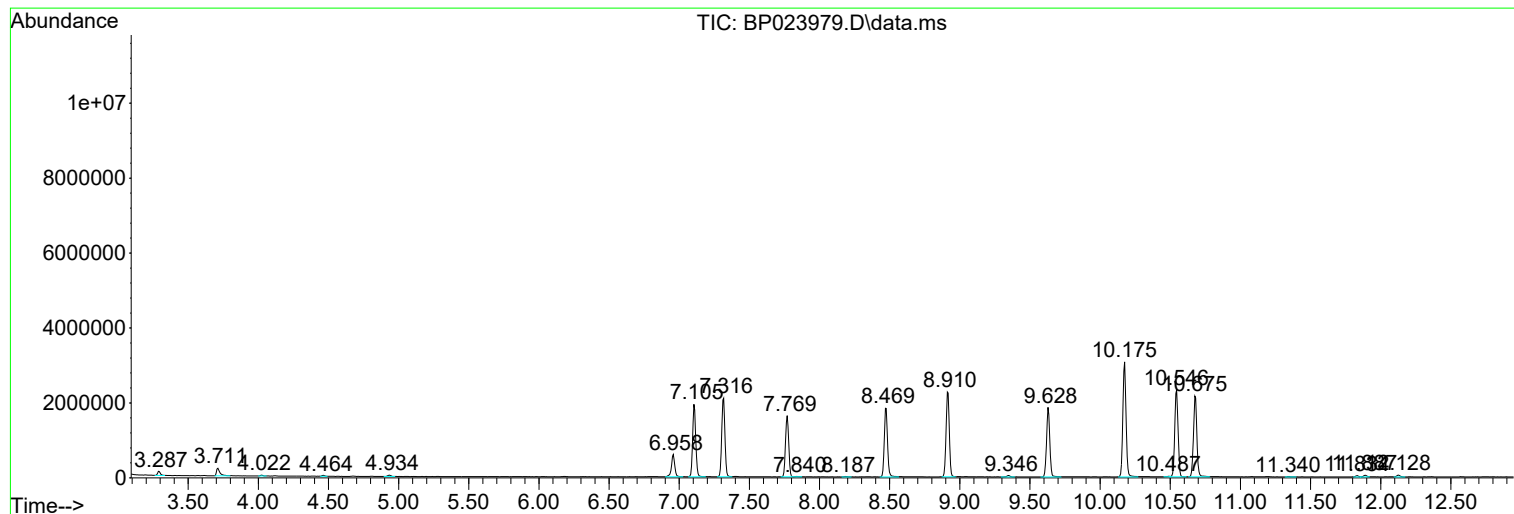

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020525\
Data File : BP023979.D
Acq On : 06 Feb 2025 20:43
Operator : RC/JU
Sample : Q1229-02
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E2991

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020525\
Data File : BP023979.D
Acq On : 06 Feb 2025 20:43
Operator : RC/JU
Sample : Q1229-02
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E2991

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc