

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020525\
 Data File : BP023988.D
 Acq On : 07 Feb 2025 03:29
 Operator : RC/JU
 Sample : Q1229-12
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E29B8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP023988.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.287	30	34	44	rVB	112447	146973	0.90%	0.104%
2	3.705	101	105	119	rBV	417330	684241	4.20%	0.483%
3	4.022	155	159	163	rVB	20171	27459	0.17%	0.019%
4	4.458	229	233	238	rBV	15366	21070	0.13%	0.015%
5	4.928	308	313	319	rVB2	17384	29993	0.18%	0.021%
6	6.181	518	526	531	rBV9	8954	17173	0.11%	0.012%
7	6.952	647	657	669	rBV	789350	1237263	7.59%	0.874%
8	7.105	676	683	692	rBV	1989563	3028384	18.58%	2.138%
9	7.311	711	718	730	rBV	2189053	3539218	21.71%	2.499%
10	7.769	789	796	804	rBV	1676697	2421831	14.86%	1.710%
11	8.469	906	915	926	rBV	2389826	3733547	22.90%	2.636%
12	8.910	980	990	1006	rBV	2325401	3803224	23.33%	2.685%
13	9.340	1058	1063	1071	rVB2	15543	24620	0.15%	0.017%
14	9.622	1104	1111	1125	rBV	2012930	3232325	19.83%	2.282%
15	10.169	1195	1204	1224	rBV	3120947	5333972	32.72%	3.766%
16	10.540	1259	1267	1275	rVB	2129435	3700737	22.70%	2.613%
17	10.669	1280	1289	1309	rBV	2568652	4453032	27.32%	3.144%
18	12.122	1530	1536	1544	rVB	44697	79926	0.49%	0.056%
19	13.222	1718	1723	1728	rVB3	11043	17164	0.11%	0.012%
20	13.346	1738	1744	1751	rVB5	8828	18599	0.11%	0.013%
21	13.793	1813	1820	1837	rBV	5706619	8208387	50.35%	5.795%
22	14.081	1861	1869	1883	rBV2	6291834	9759981	59.87%	6.891%
23	14.393	1915	1922	1932	rBV	3542246	5111227	31.35%	3.609%
24	14.475	1933	1936	1945	rVB10	11980	22418	0.14%	0.016%
25	14.616	1954	1960	1979	rBV	520308	1013353	6.22%	0.715%
26	14.751	1980	1983	1989	rVV4	15886	31065	0.19%	0.022%
27	14.816	1989	1994	1999	rVB4	41700	64144	0.39%	0.045%
28	15.028	2025	2030	2035	rBV8	10300	21185	0.13%	0.015%
29	15.222	2058	2063	2068	rVB3	10978	20242	0.12%	0.014%
30	15.398	2086	2093	2106	rBV	9164538	12899997	79.13%	9.108%
31	15.516	2106	2113	2129	rVV	2265477	3319936	20.37%	2.344%
32	15.640	2130	2134	2143	rVB2	43025	73482	0.45%	0.052%
33	16.192	2225	2228	2234	rBV7	9198	16419	0.10%	0.012%
34	16.834	2332	2337	2347	rBV3	58546	112835	0.69%	0.080%
35	16.969	2355	2360	2367	rVB2	20354	32204	0.20%	0.023%
36	17.192	2390	2398	2408	rBV	3871140	5910323	36.26%	4.173%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020525\
Data File : BP023988.D
Acq On : 07 Feb 2025 03:29
Operator : RC/JU
Sample : Q1229-12
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E29B8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Title : SVOA CALIBRATION

37	17.286	2408	2414	2427	rVV	10588788	14332159	87.92%	10.119%
38	17.881	2513	2515	2519	rVB5	15086	16863	0.10%	0.012%
39	18.128	2553	2557	2564	rBV4	28435	50441	0.31%	0.036%
40	19.204	2735	2740	2746	rBV	122665	167925	1.03%	0.119%
41	19.275	2748	2752	2757	rVV	93439	134152	0.82%	0.095%
42	19.651	2810	2816	2826	rBV	11474655	16301464	100.00%	11.509%
43	21.627	3145	3152	3164	rBV2	3633244	6197393	38.02%	4.375%
44	24.768	3675	3686	3700	rVB	5408667	15822996	97.06%	11.171%
45	24.992	3716	3724	3743	rVB	2323593	6449614	39.56%	4.553%




Sum of corrected areas: 141640956

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020525\
Data File : BP023988.D
Acq On : 07 Feb 2025 03:29
Operator : RC/JU
Sample : Q1229-12
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E29B8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

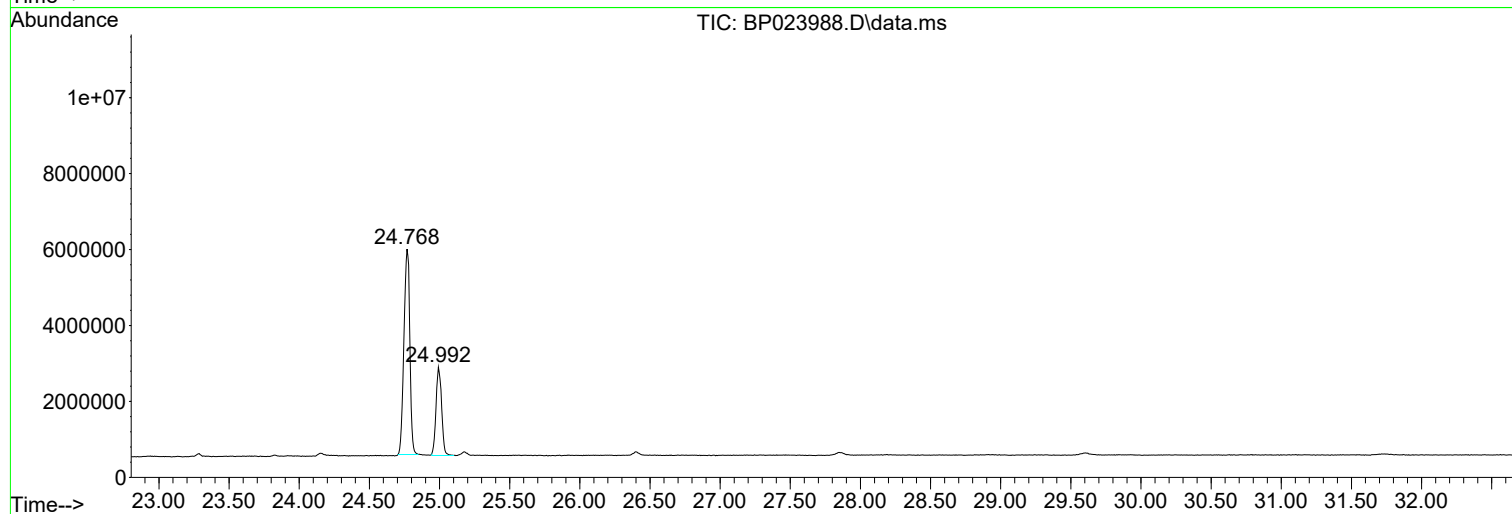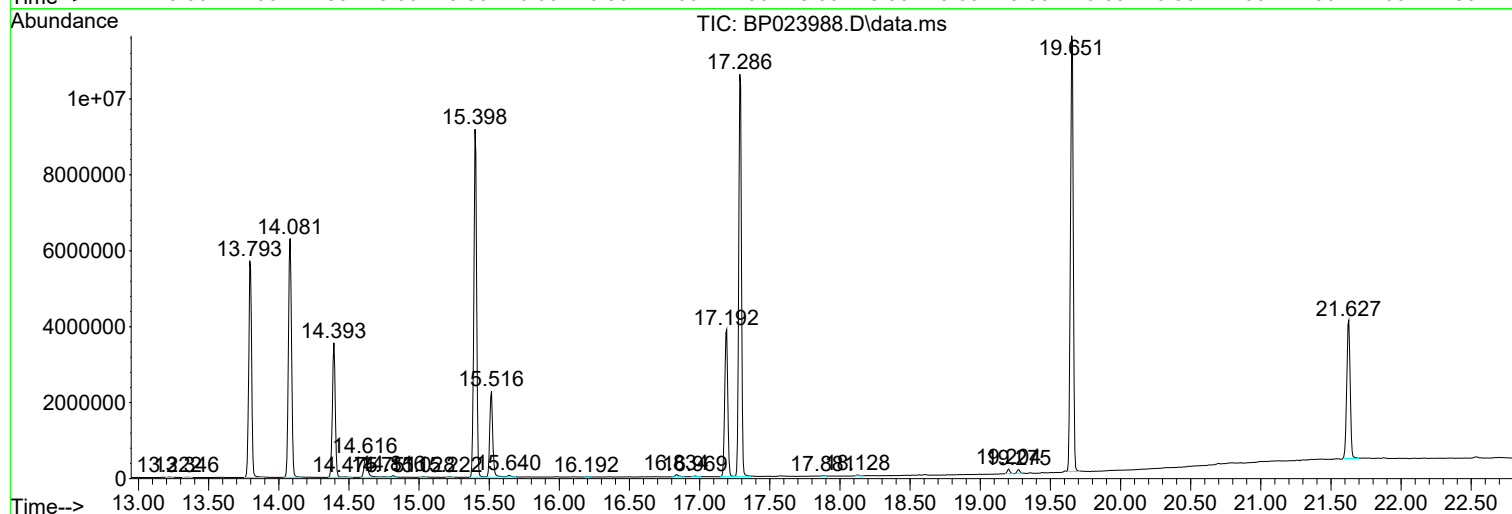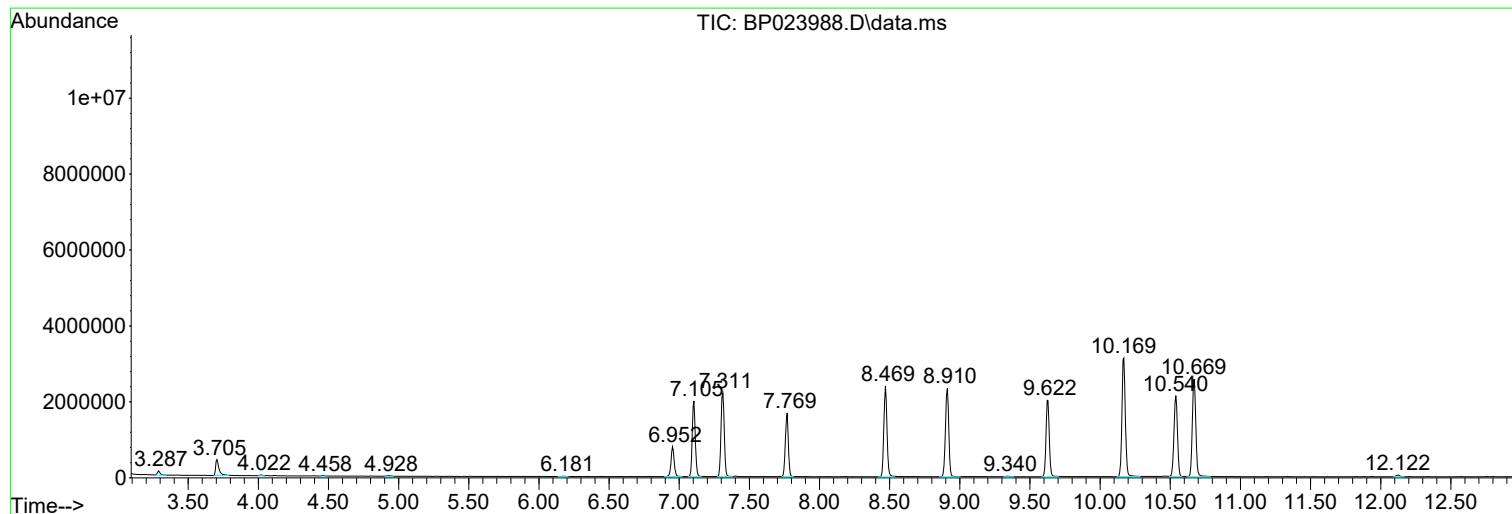

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020525\
Data File : BP023988.D
Acq On : 07 Feb 2025 03:29
Operator : RC/JU
Sample : Q1229-12
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E29B8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020525\
Data File : BP023988.D
Acq On : 07 Feb 2025 03:29
Operator : RC/JU
Sample : Q1229-12
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E29B8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc