

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020624\
Data File : BP019578.D
Acq On : 06 Feb 2024 17:34
Operator : MA/JU
Sample : PB158822BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB158822BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP019578.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.028	325	330	339	rBV	51400	75338	1.96%	0.344%
2	5.481	400	407	421	rBV	1714477	2572667	67.00%	11.743%
3	7.081	670	679	691	rBV	1585263	2597007	67.63%	11.854%
4	7.910	813	820	828	rBV	355852	569709	14.84%	2.600%
5	9.075	1008	1018	1032	rBV	1002524	1715917	44.69%	7.832%
6	10.710	1287	1296	1305	rBV	392073	704594	18.35%	3.216%
7	13.169	1706	1714	1724	rBV	2522428	3768636	98.15%	17.201%
8	14.539	1940	1947	1956	rBV	550772	847529	22.07%	3.868%
9	16.033	2190	2201	2220	rBV	1590677	2317285	60.35%	10.577%
10	17.292	2409	2415	2426	rBV	544147	837434	21.81%	3.822%
11	19.863	2846	2852	2862	rBV	3076942	3839818	100.00%	17.526%
12	21.386	3106	3111	3117	rBV	727567	918561	23.92%	4.193%
13	23.804	3514	3522	3530	rBV	549928	1144288	29.80%	5.223%




Sum of corrected areas: 21908783

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020624\
Data File : BP019578.D
Acq On : 06 Feb 2024 17:34
Operator : MA/JU
Sample : PB158822BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB158822BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

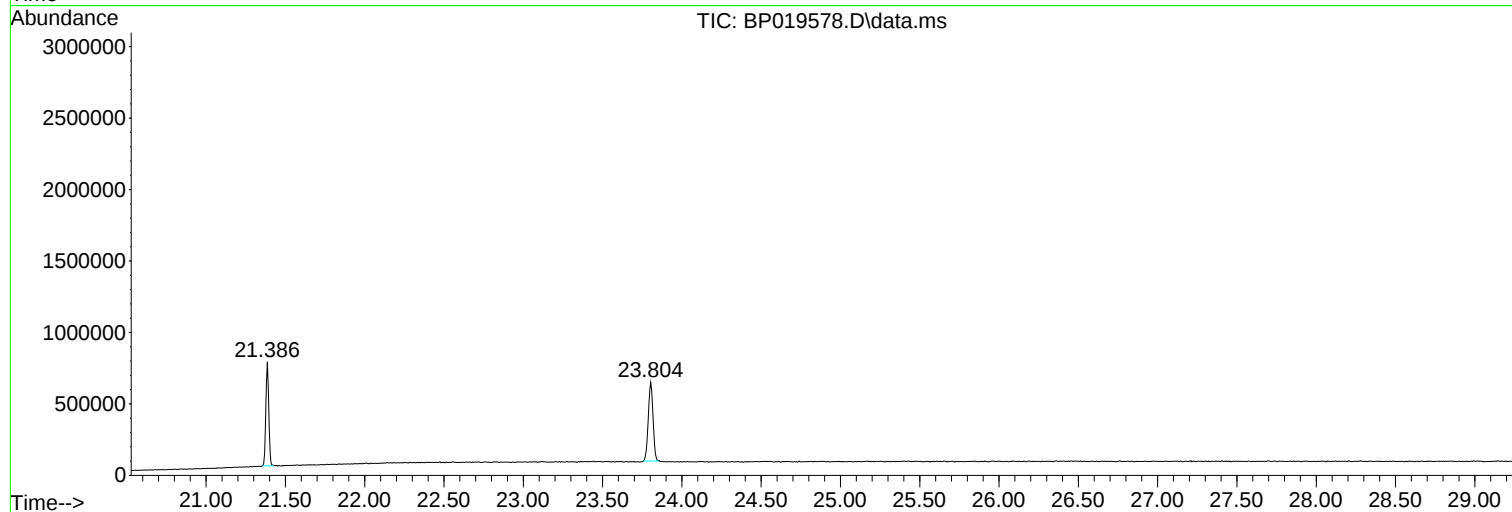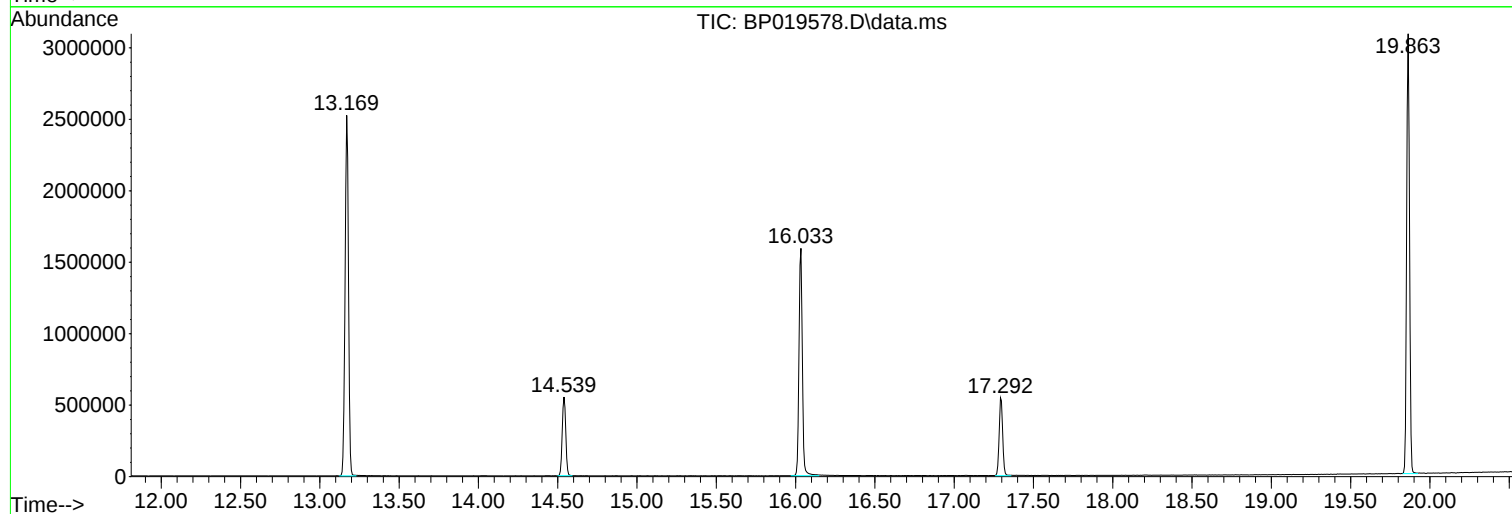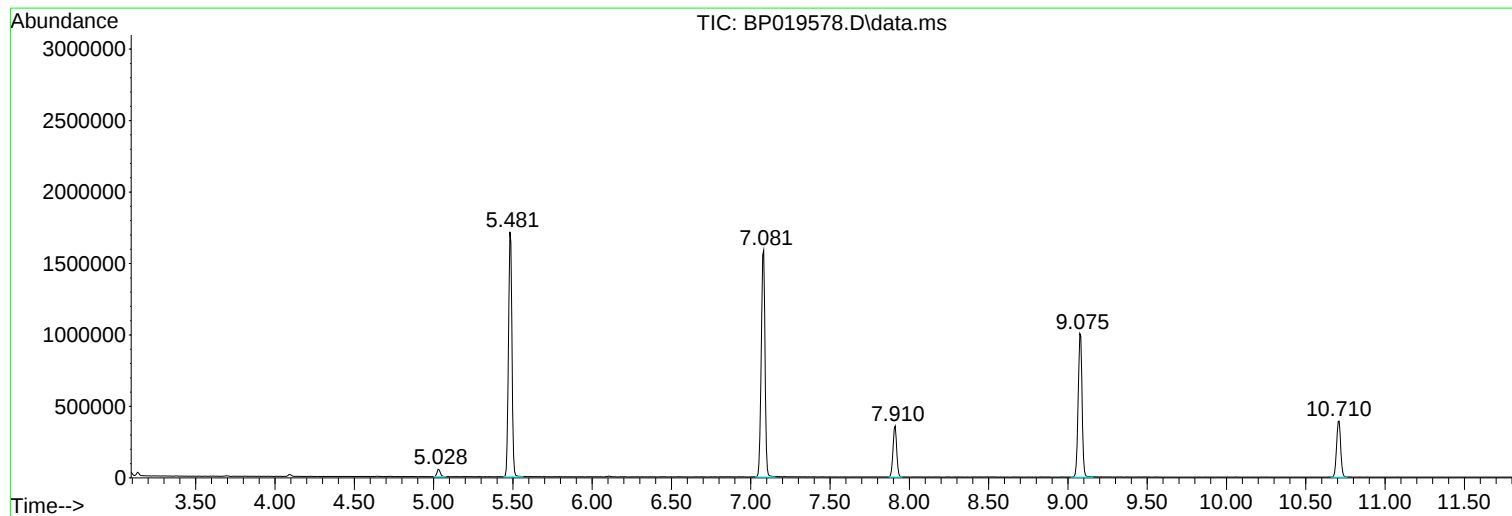

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020624\
Data File : BP019578.D
Acq On : 06 Feb 2024 17:34
Operator : MA/JU
Sample : PB158822BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB158822BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.028	2.64 ng	75338	1,4-Dichlorobenzene-d4	7.910

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	72		
2	Propane, 1-ethoxy-2-methyl-	102	C6H14O	000627-02-1	38		
3	2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	25		
4	2-Hexanol, 2-methyl-	116	C7H16O	000625-23-0	25		
5	Butyl aldoxime, 3-methyl-, syn-	101	C5H11NO	005780-40-5	17		

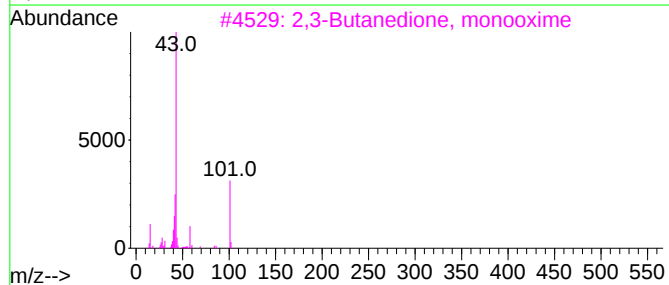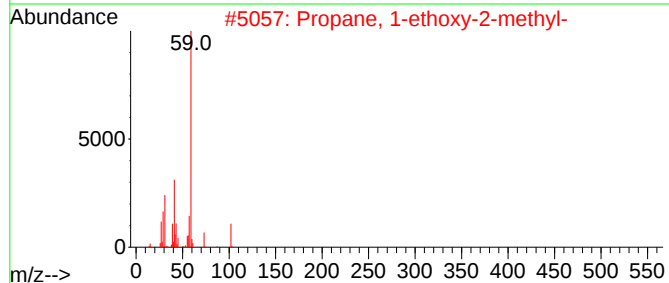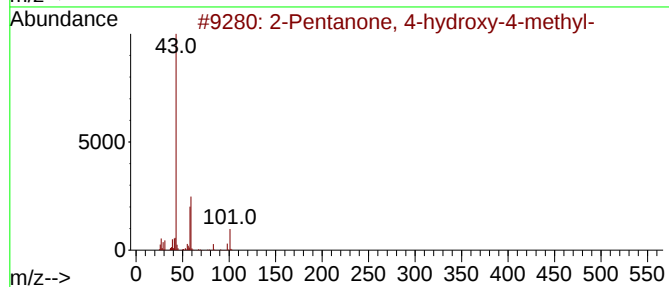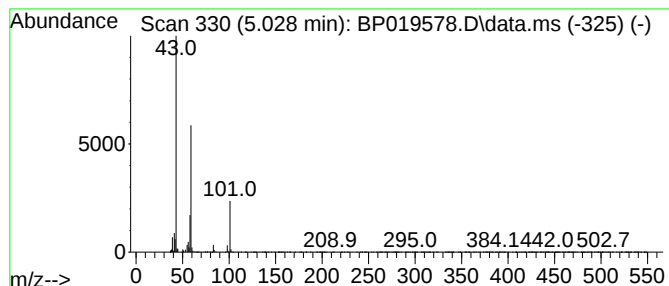

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020624\
Data File : BP019578.D
Acq On : 06 Feb 2024 17:34
Operator : MA/JU
Sample : PB158822BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB158822BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.028	2.6	ng	75338	1	7.910	569709	20.0