
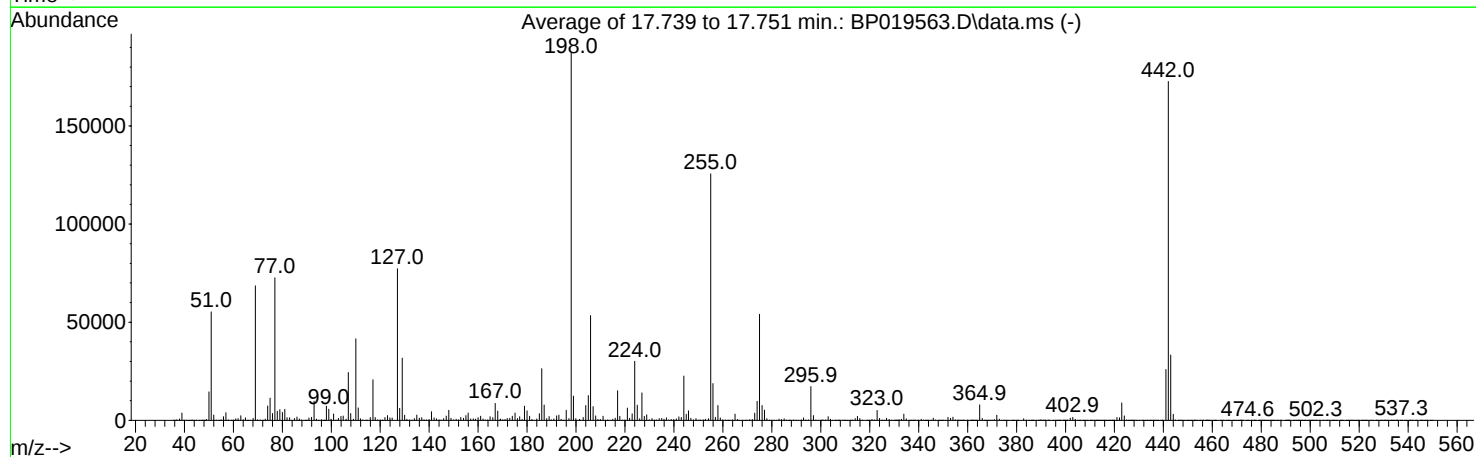


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020624\
Data File : BP019563.D
Acq On : 06 Feb 2024 08:53
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Feb 01 00:51:48 2024

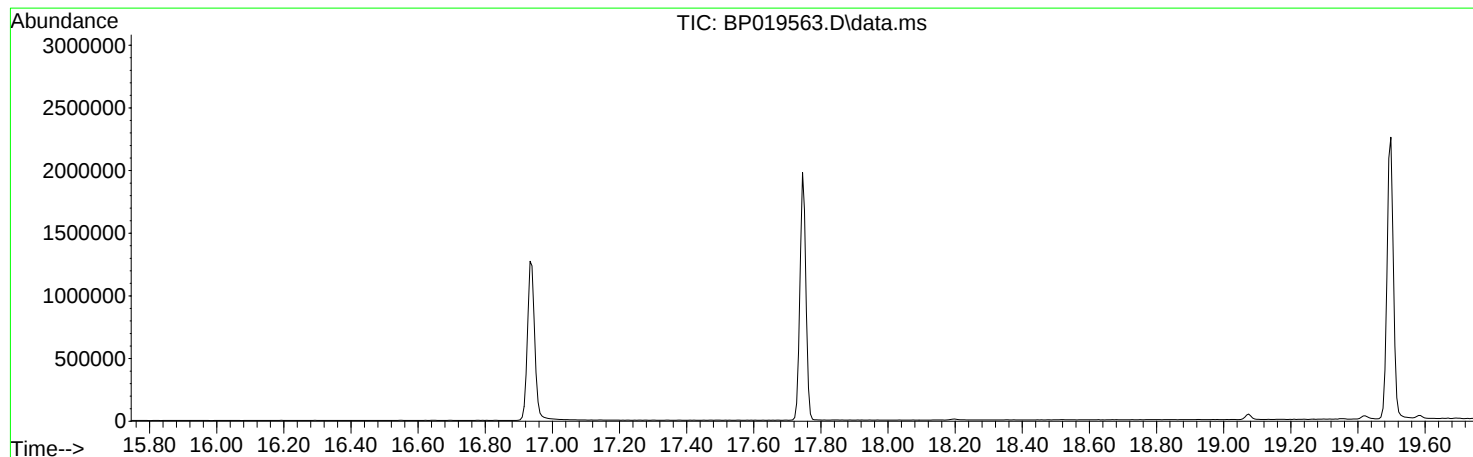




AutoFind: Scans 2491, 2492, 2493; Background Corrected with Scan 2481

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.5	55246	PASS
68	69	0.00	2	1.6	1067	PASS
69	198	0.00	100	36.6	68568	PASS
70	69	0.00	2	0.5	332	PASS
127	198	10	80	41.2	77296	PASS
197	198	0.00	2	0.5	869	PASS
198	198	100	100	100.0	187392	PASS
199	198	5	9	6.6	12439	PASS
275	198	10	60	28.8	54051	PASS
365	198	1	100	4.2	7891	PASS
441	198	0.01	100	13.8	25951	PASS
442	442	100	100	100.0	172672	PASS
443	442	15	24	19.3	33267	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020624\
Data File : BP019563.D
Acq On : 06 Feb 2024 08:53
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Feb 07 06:55:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 01 00:51:48 2024
Response via : Initial Calibration

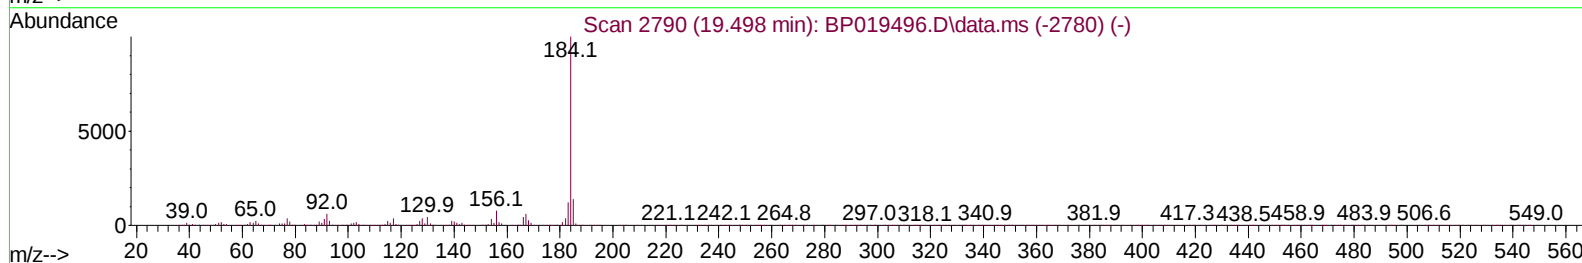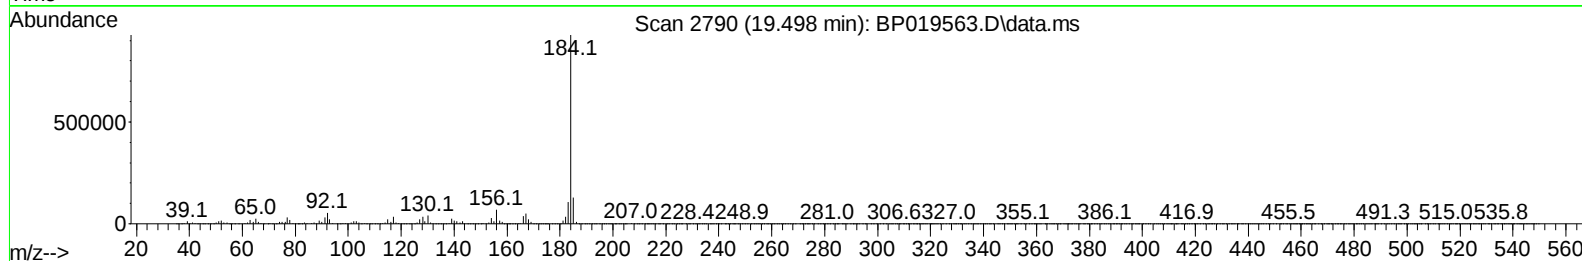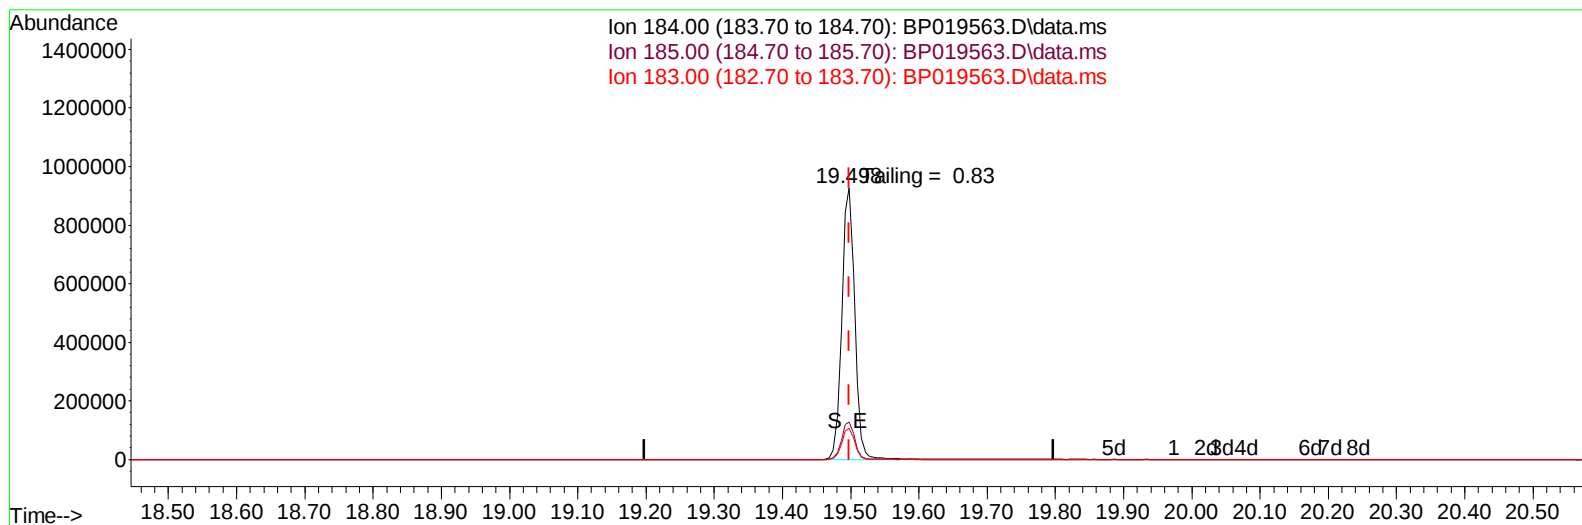

TIC: BP019563.D\data.ms

(77) Benzidine

19.498min (+ 0.000) 3221886.90 ng m

response 1212461

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	13.86
183.00	12.10	11.55
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/7/2024	BNA_P	BP019563.D
Compound Name	Response	Retention Time
DDT	712079	20.698
DDD	13228	20.269
DDE	117	19.774
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13345	725424	1.84

Instrument :
BNA_P
ClientSampleId :
DFTPP