
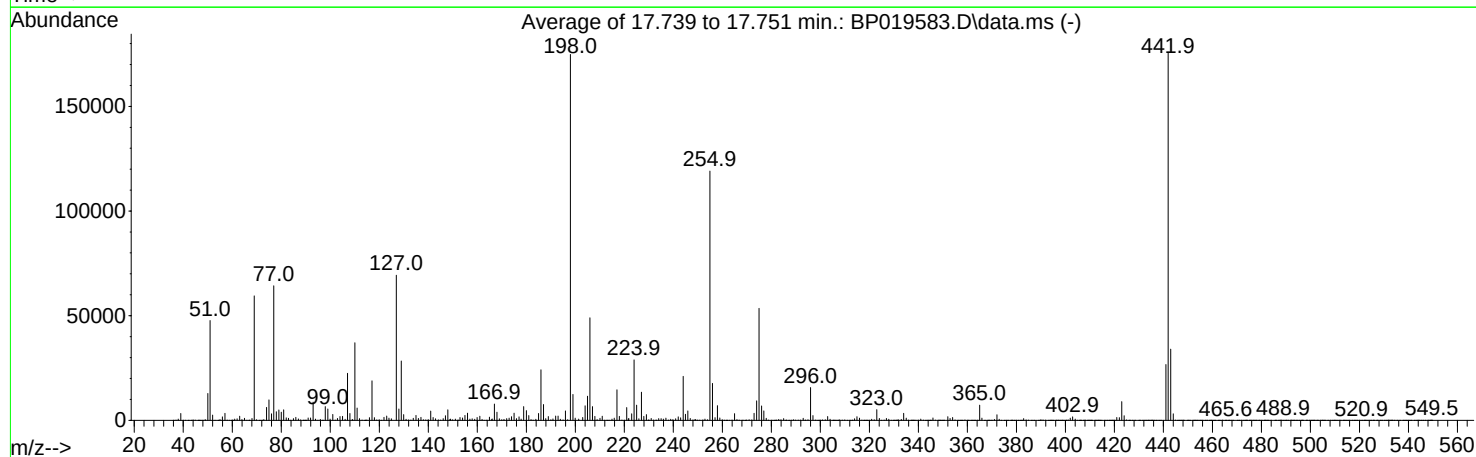


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020724\
Data File : BP019583.D
Acq On : 07 Feb 2024 08:54
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Feb 01 00:51:48 2024

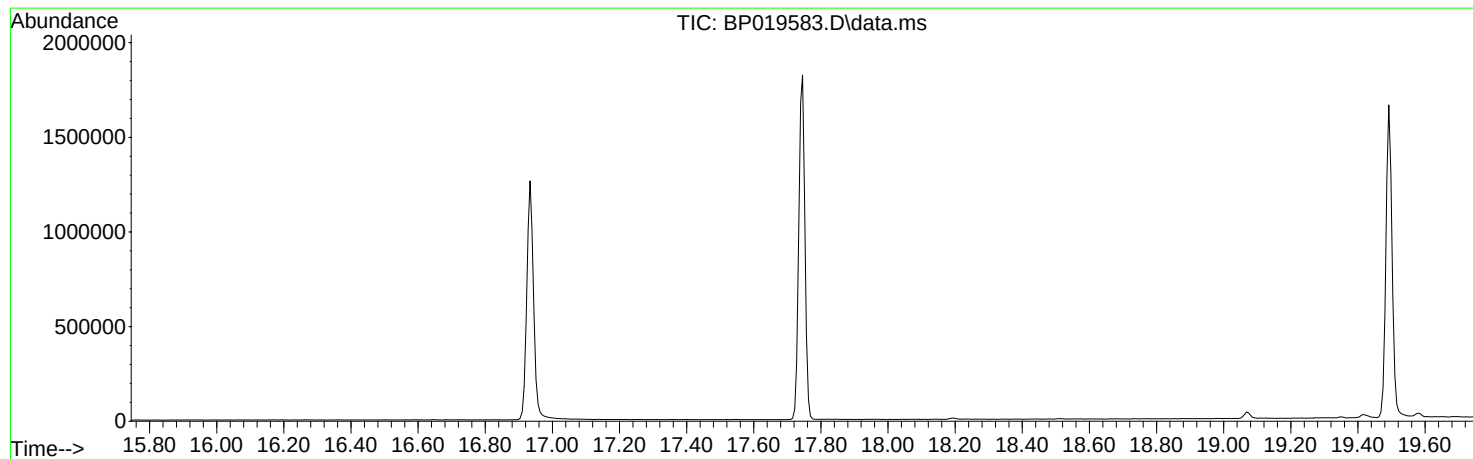




AutoFind: Scans 2491, 2492, 2493; Background Corrected with Scan 2482

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.3	47726	PASS
68	69	0.00	2	1.5	912	PASS
69	198	0.00	100	34.0	59458	PASS
70	69	0.00	2	0.5	309	PASS
127	198	10	80	39.7	69329	PASS
197	198	0.00	2	0.2	323	PASS
198	198	100	100	100.0	174797	PASS
199	198	5	9	7.1	12393	PASS
275	198	10	60	30.6	53529	PASS
365	198	1	100	4.1	7246	PASS
441	198	0.01	100	15.3	26718	PASS
442	442	100	100	100.0	175743	PASS
443	442	15	24	19.4	34009	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020724\
Data File : BP019583.D
Acq On : 07 Feb 2024 08:54
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Feb 07 10:23:15 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 01 00:51:48 2024
Response via : Initial Calibration

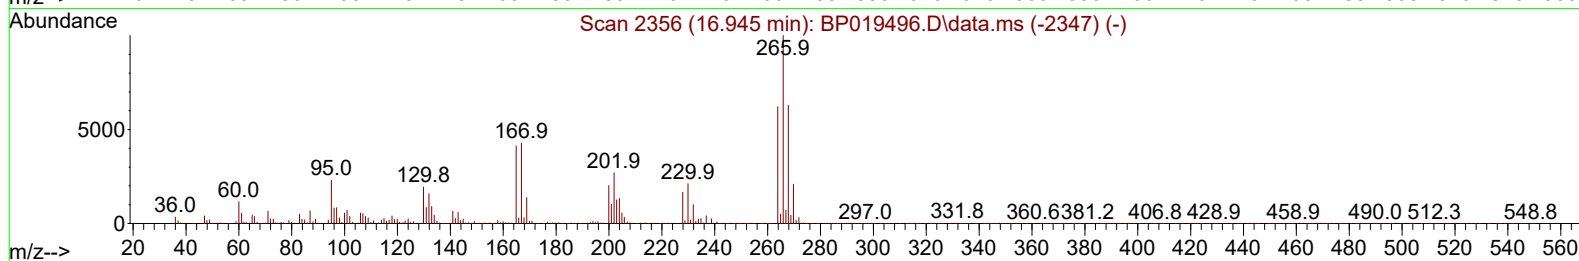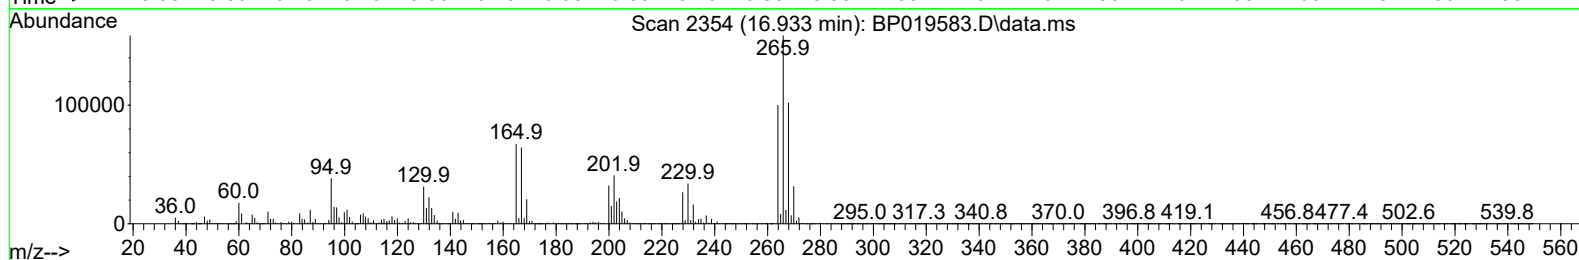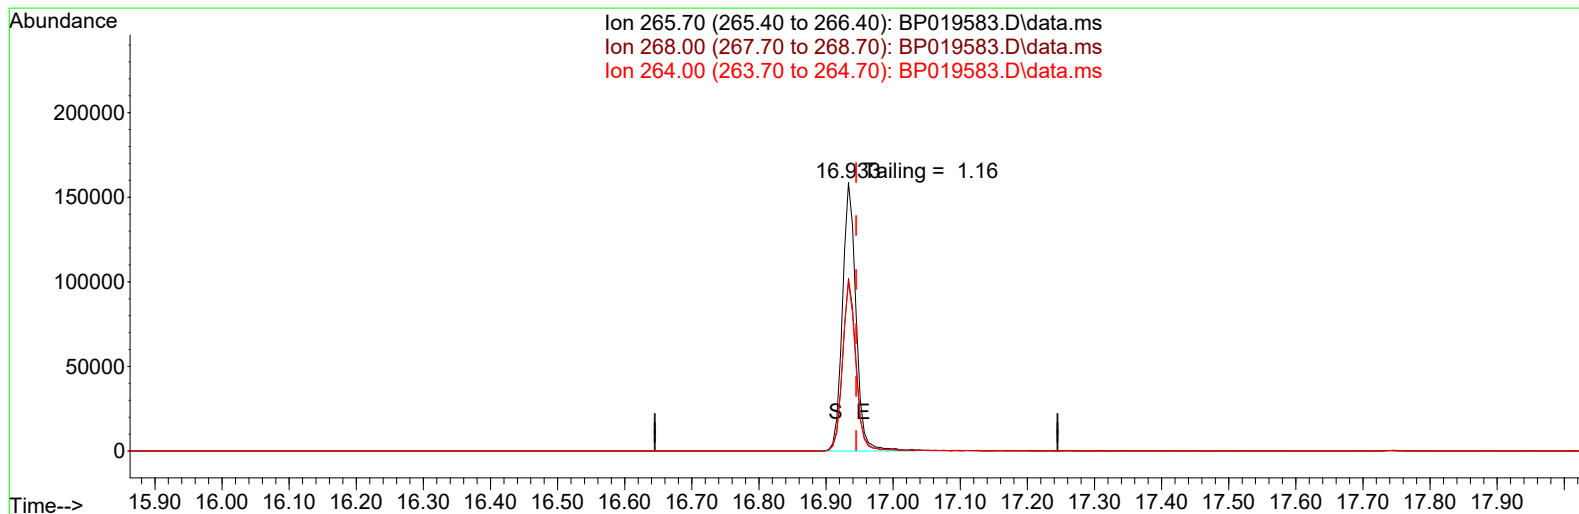

TIC: BP019583.D\data.ms

(70) Pentachlorophenol (C)

16.933min (-0.012) 365976.74 ng




response 222920

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	64.23
264.00	62.10	62.99
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020724\
Data File : BP019583.D
Acq On : 07 Feb 2024 08:54
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Feb 07 10:23:15 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 01 00:51:48 2024
Response via : Initial Calibration

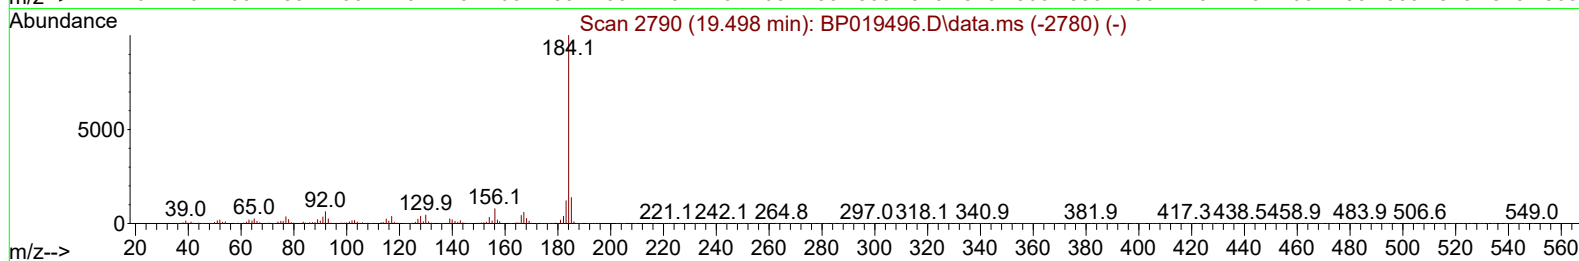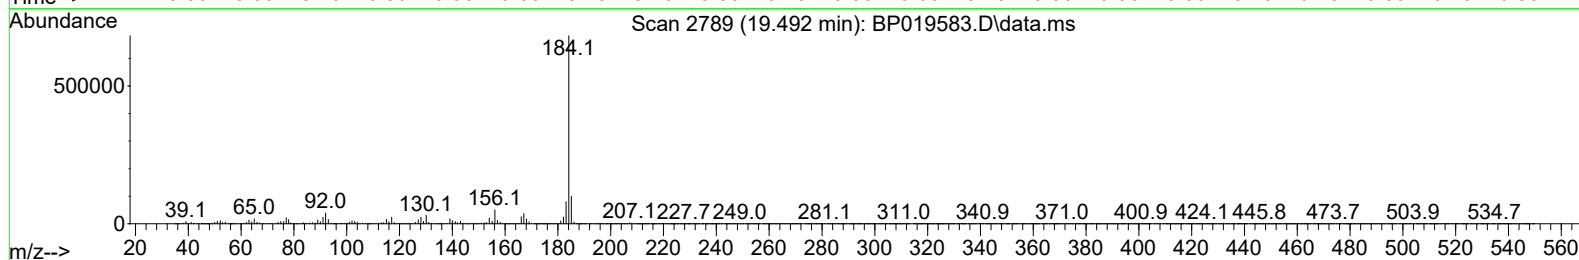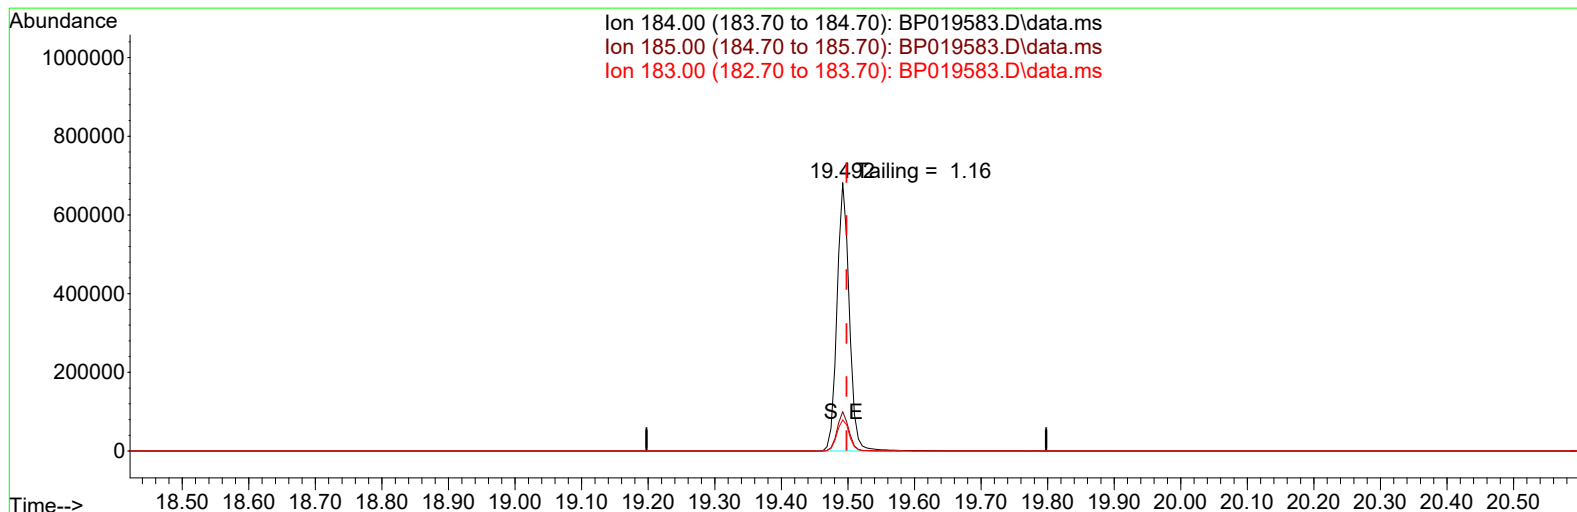

TIC: BP019583.D\data.ms

(77) Benzidine

19.492min (-0.006) 76680.68 ng

response 870504

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.66
183.00	12.10	11.67
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/7/2024	BNA_P	<u>BP019583.D</u>
Compound Name	Response	Retention Time
DDT	488167	20.692
DDD	11434	20.263
DDE	894	19.763
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12328	500495	2.46

Instrument :
BNA_P
ClientSampleId :
DFTPP