

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020725\
 Data File : BP023998.D
 Acq On : 07 Feb 2025 11:47
 Operator : RC/JU
 Sample : PB166554BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK554

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP023998.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.287	30	34	41	rBV	106645	137328	1.40%	0.132%
2	3.699	100	104	125	rBV	1472117	2211714	22.52%	2.122%
3	4.023	154	159	165	rVB	26940	40347	0.41%	0.039%
4	6.952	649	657	673	rBV	2021445	3036093	30.91%	2.913%
5	7.099	676	682	695	rVB	1439466	2193097	22.33%	2.104%
6	7.311	710	718	729	rBV	1954302	3065590	31.21%	2.941%
7	7.769	786	796	807	rBV	1412714	2197007	22.37%	2.108%
8	8.469	907	915	932	rBV	2394690	3852069	39.22%	3.696%
9	8.911	983	990	1002	rBV	1645054	2673312	27.22%	2.565%
10	9.040	1007	1012	1017	rBV2	11241	18443	0.19%	0.018%
11	9.622	1103	1111	1127	rBV	1336414	2188087	22.28%	2.099%
12	10.169	1197	1204	1220	rBV	2363551	3829697	38.99%	3.674%
13	10.540	1259	1267	1278	rBV	2097689	3384379	34.46%	3.247%
14	10.669	1281	1289	1308	rBV	2239283	3752000	38.20%	3.600%
15	12.122	1531	1536	1542	rBV	37708	61375	0.62%	0.059%
16	12.340	1565	1573	1577	rBV10	5329	13967	0.14%	0.013%
17	13.351	1740	1745	1751	rVB6	7560	14803	0.15%	0.014%
18	13.787	1813	1819	1836	rBV	3755681	5165551	52.59%	4.956%
19	14.075	1860	1868	1883	rBV	4726616	6656684	67.77%	6.386%
20	14.387	1913	1921	1933	rBV	3037154	4651113	47.35%	4.462%
21	14.604	1952	1958	1981	rBV	1274721	2212602	22.53%	2.123%
22	15.051	2028	2034	2041	rBV8	10215	19594	0.20%	0.019%
23	15.393	2085	2092	2100	rBV	5738241	8195038	83.43%	7.862%
24	15.510	2106	2112	2125	rBV	622036	821217	8.36%	0.788%
25	15.634	2128	2133	2141	rVB3	27301	48545	0.49%	0.047%
26	16.192	2223	2228	2234	rVB9	6984	10199	0.10%	0.010%
27	16.851	2335	2340	2346	rVB7	8516	14576	0.15%	0.014%
28	16.963	2354	2359	2363	rBV2	13446	20352	0.21%	0.020%
29	17.175	2389	2395	2406	rBV	3976503	5378579	54.76%	5.160%
30	17.281	2406	2413	2434	rVV2	5992980	8841921	90.02%	8.483%
31	18.122	2553	2556	2561	rBV6	7683	13887	0.14%	0.013%
32	19.204	2736	2740	2747	rBV	68795	92009	0.94%	0.088%
33	19.275	2749	2752	2756	rVB	57698	73708	0.75%	0.071%
34	19.657	2811	2817	2827	rBV	7461726	9822241	100.00%	9.423%
35	21.627	3146	3152	3160	rBV	3699890	5325662	54.22%	5.109%
36	24.763	3676	3685	3706	rVB	3422164	8898510	90.60%	8.537%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020725\
Data File : BP023998.D
Acq On : 07 Feb 2025 11:47
Operator : RC/JU
Sample : PB166554BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK554

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Title : SVOA CALIBRATION

37 24.986 3715 3723 3740 rVB 2090806 5302131 53.98% 5.087%




Sum of corrected areas: 104233427

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020725\
Data File : BP023998.D
Acq On : 07 Feb 2025 11:47
Operator : RC/JU
Sample : PB166554BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK554

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

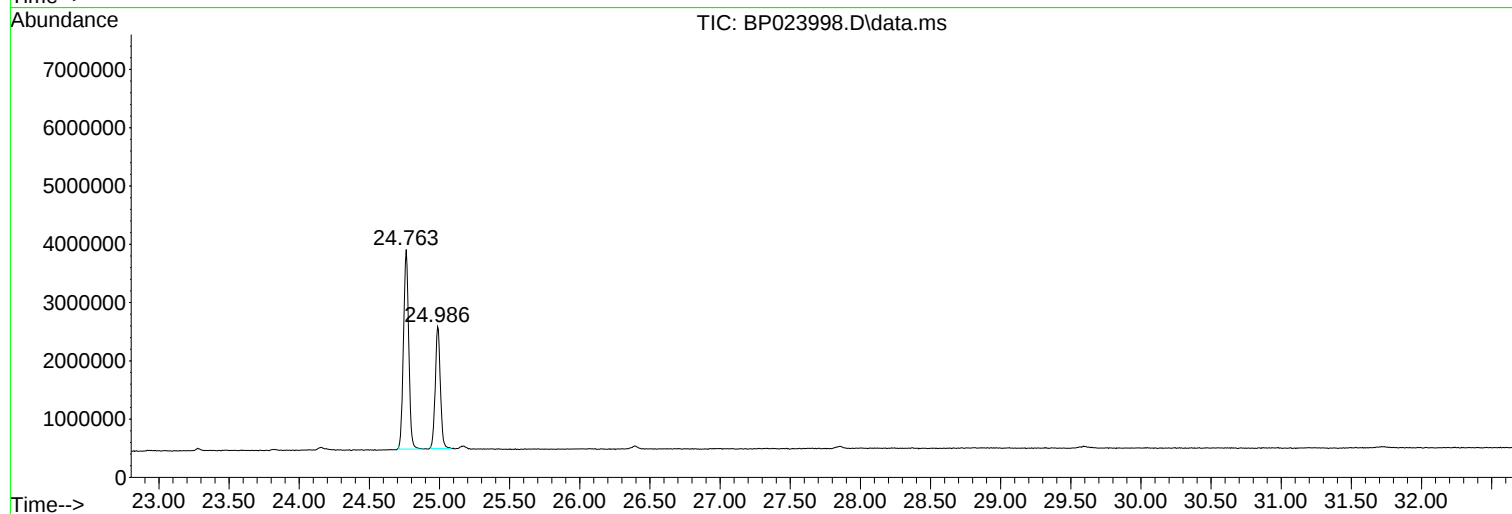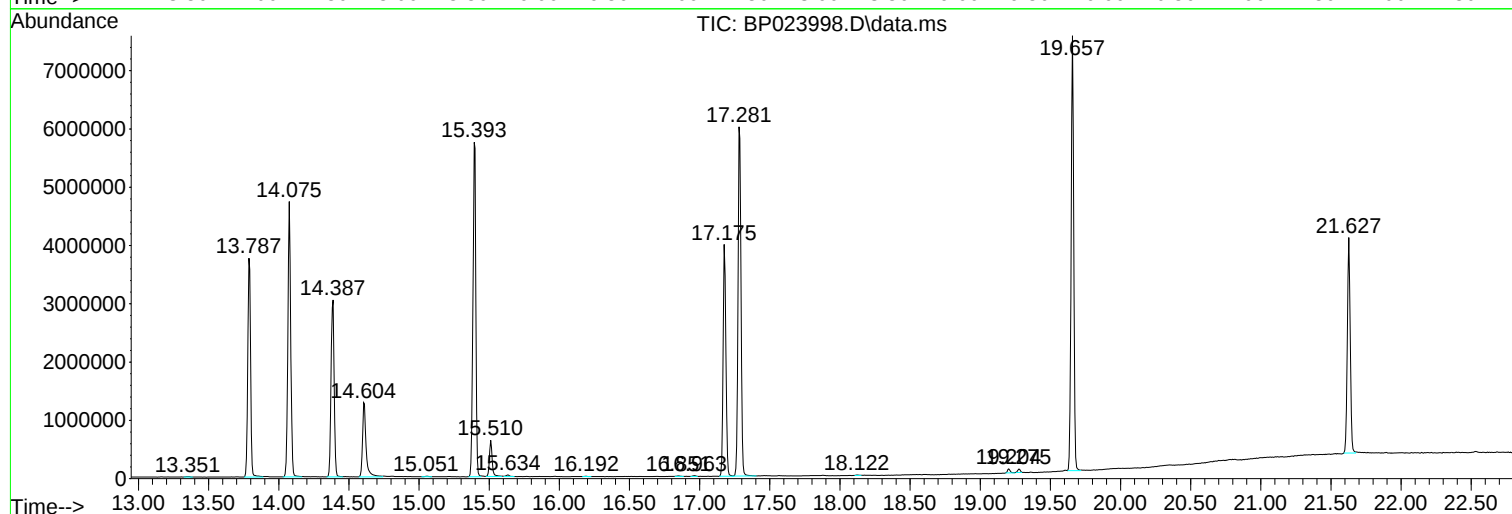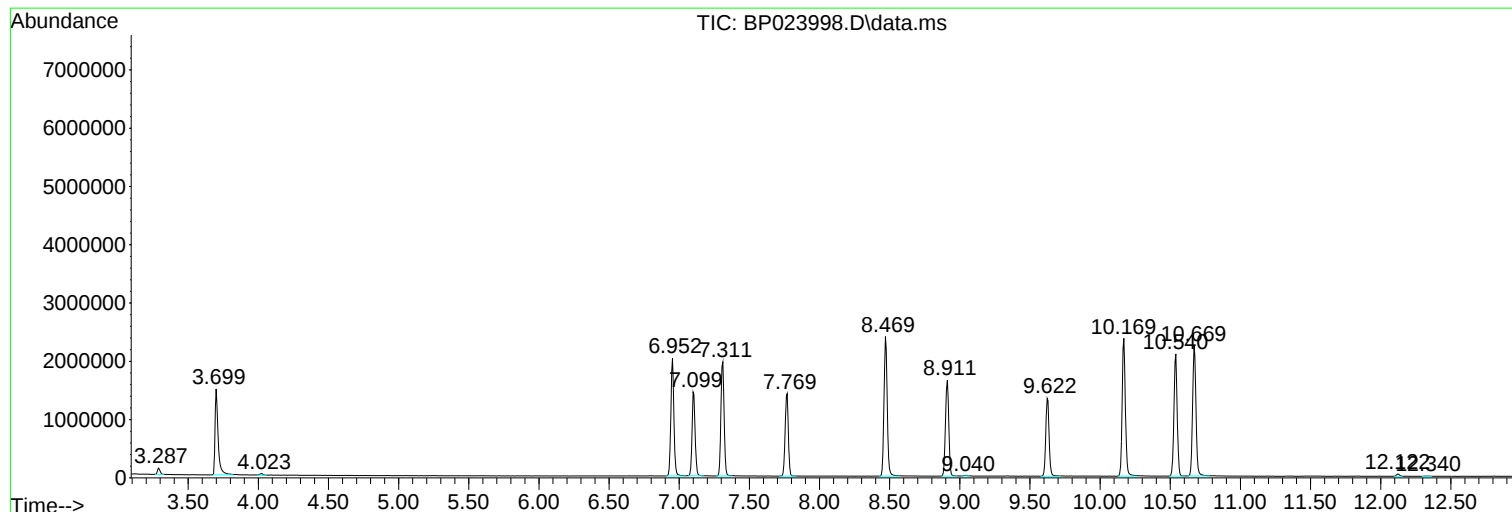

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020725\
Data File : BP023998.D
Acq On : 07 Feb 2025 11:47
Operator : RC/JU
Sample : PB166554BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK554

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020725\
Data File : BP023998.D
Acq On : 07 Feb 2025 11:47
Operator : RC/JU
Sample : PB166554BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK554

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc